

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
 Data File : PD087291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 11:46
 Operator : AR\AJ
 Sample : P5267-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E28Z0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2024
 Supervised By : Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 23:58:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 23:32:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.883	16996587	90973274	8.302	7.818
2) SA Decachlor...	9.077	8.079	17536063	98249921	5.742m	7.458m#
Target Compounds						
13) MA Dieldrin	6.351	5.515	1335489	13806747	0.369m	0.902m#
19) B Endosulfa...	7.149	6.487	4296096	11101809	1.482m	0.840m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
Data File : PD087291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 11:46
Operator : AR\AJ
Sample : P5267-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 23:58:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 23:32:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

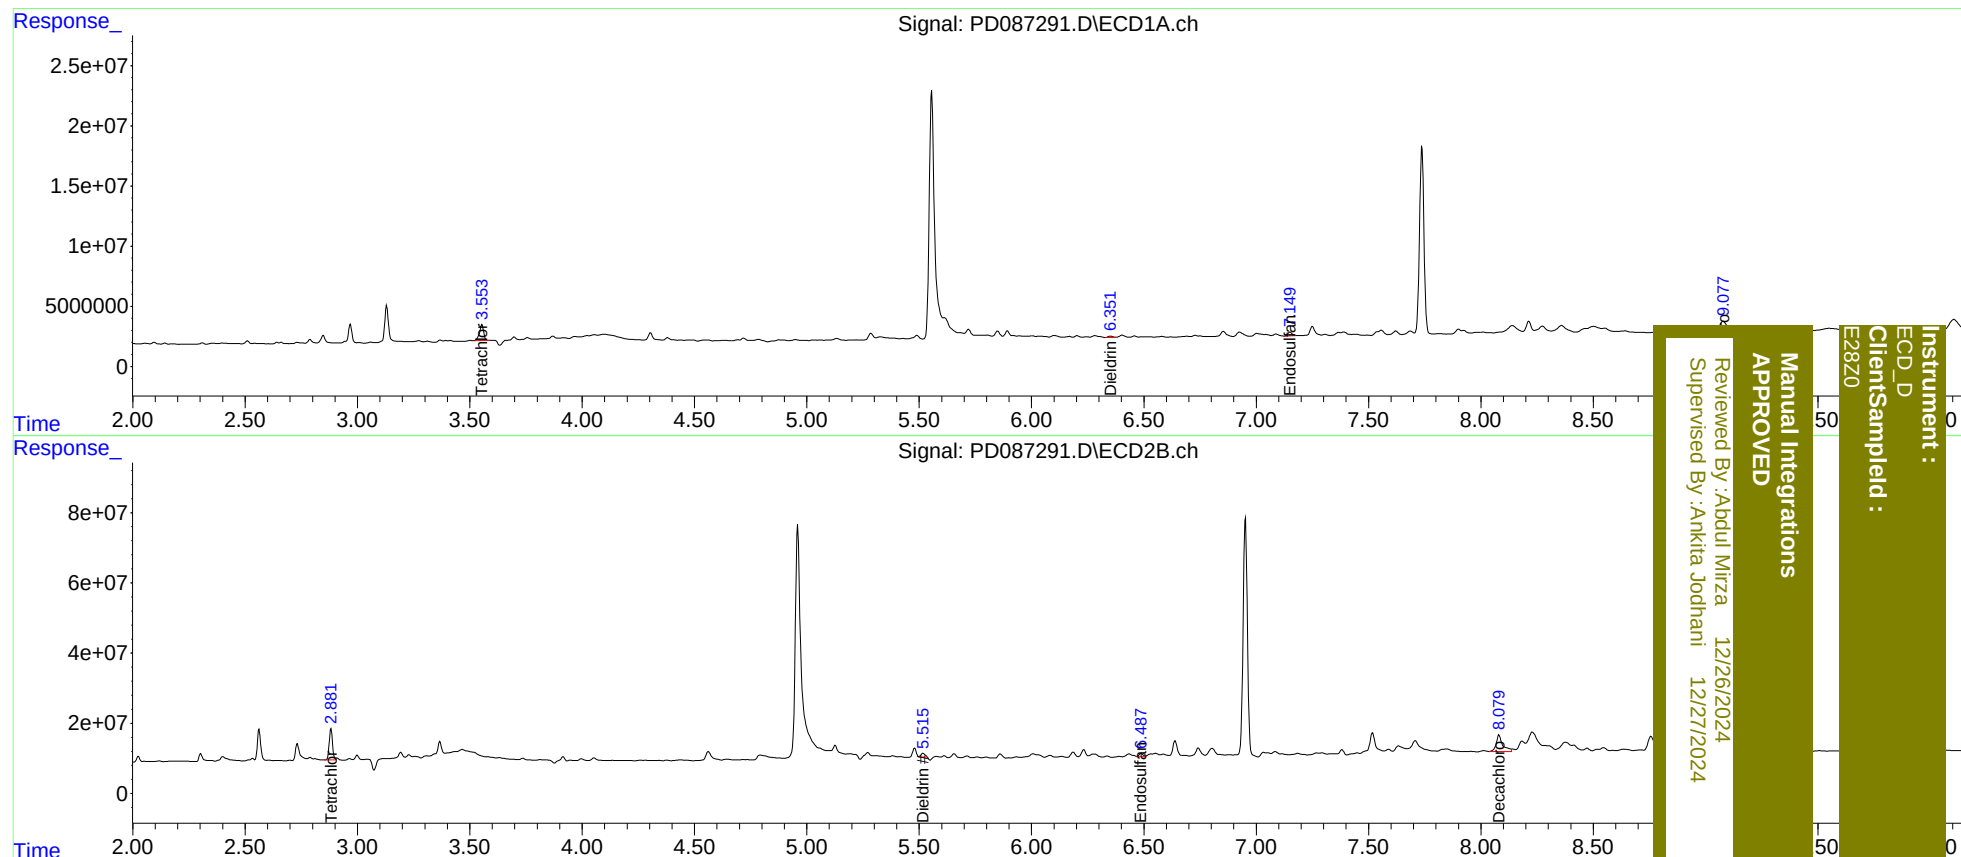

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/26/2024
Supervised By: Ankita Jodhani 12/27/2024

Instrument :
ECD_D
Client Sampled :
E2820