

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
 Data File : PD087305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 15:44
 Operator : AR\AJ
 Sample : P5302-05MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2AR6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:02:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 23:32:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	28867847	169.6E6	14.100	14.570
2)	SA Decachlor...	9.079	8.081	32862304	142.6E6	10.760	10.822
Target Compounds							
2)	A alpha-BHC	4.004	3.396	187.2E6	785.6E6	46.397	43.098
3)	MA gamma-BHC...	4.335	3.733	181.6E6	725.6E6	46.490	42.886
4)	MA Heptachlor	4.935	4.087	176.4E6	698.7E6	44.446	40.409
5)	MB Aldrin	5.277	4.374	173.7E6	688.2E6	44.600	41.123
6)	B beta-BHC	4.519	4.028	70609041	294.9E6	40.379	37.682
7)	B delta-BHC	4.767	4.265	182.3E6	717.8E6	45.848	41.348
8)	B Heptachlo...	5.696	4.878	154.6E6	633.1E6	42.843	40.382
9)	A Endosulfan I	6.078	5.252	143.1E6	598.2E6	42.850m	41.270m
10)	B trans-Chl...	5.951	5.131	148.7E6	653.6E6	42.534	40.170
11)	B cis-Chlor...	6.031	5.195	157.2E6	650.1E6	44.257m	41.389m
12)	B 4,4'-DDE	6.201	5.382	292.5E6	1220.9E6	88.399	81.954
13)	MA Dieldrin	6.353	5.519	322.0E6	1246.2E6	89.022	81.400
14)	MA Endrin	6.580	5.795	266.4E6	1111.9E6	89.174	79.589
15)	B Endosulfa...	6.790	6.086	257.0E6	1060.3E6	85.969	78.088
16)	A 4,4'-DDD	6.710	5.936	234.3E6	1003.2E6	90.379	82.387
17)	MA 4,4'-DDT	7.026	6.190	206.8E6	952.8E6	77.135	75.571
18)	B Endrin al...	6.919	6.264	174.0E6	735.8E6	74.139	70.421
19)	B Endosulfa...	7.154	6.488	242.0E6	1027.3E6	83.501	77.704
20)	A Methoxychlor	7.497	6.762	585.8E6	2010.9E6	393.748	344.924
21)	B Endrin ke...	7.635	6.997	264.8E6	1096.9E6	82.516	75.884

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
Data File : PD087305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 15:44
Operator : AR\AJ
Sample : P5302-05MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:02:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 23:32:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

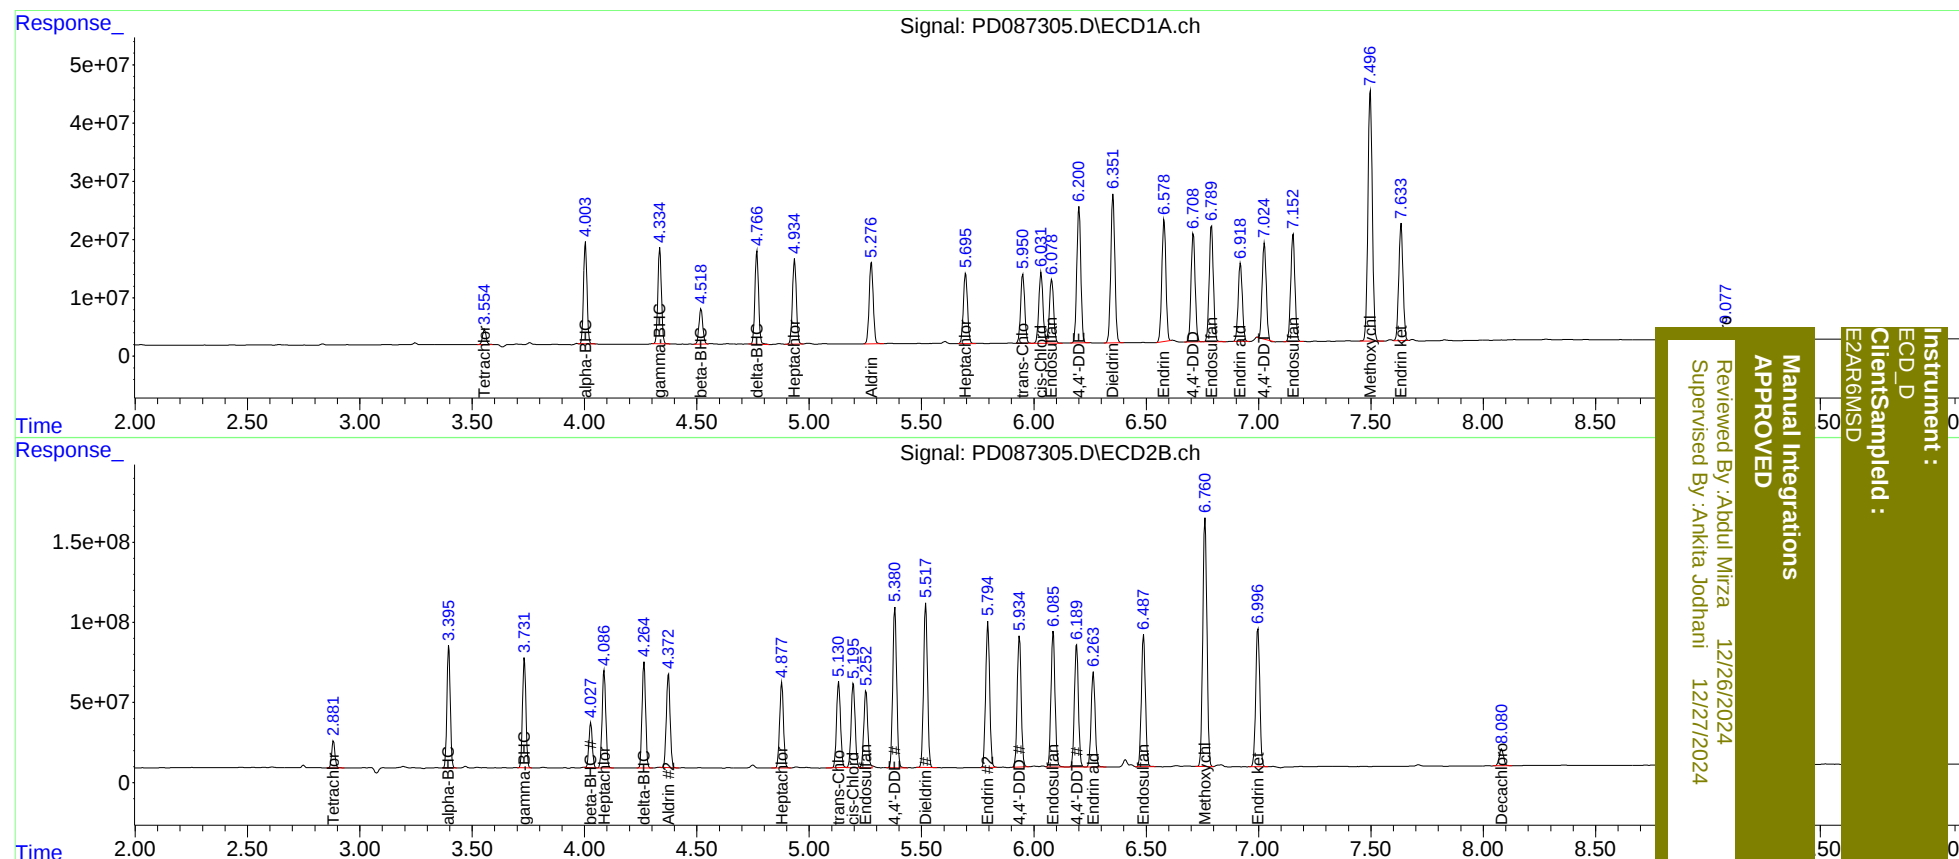

Instrument :
ECD_D
Client Sampled :
EZAR6MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 12/26/2024
Supervised By: Ankita Jodhani 12/27/2024