

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
 Data File : PD087323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 20:29
 Operator : AR\AJ
 Sample : P5331-03MSD
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2AQ1MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:07:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 23:32:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	26834788	156.2E6	13.107	13.423
2)	SA Decachlor...	9.079	8.081	28928855	124.1E6	9.472	9.423
Target Compounds							
2)	A alpha-BHC	4.004	3.396	211.6E6	864.2E6	52.441	47.412
3)	MA gamma-BHC...	4.335	3.733	205.9E6	795.4E6	52.714	47.009
4)	MA Heptachlor	4.935	4.088	201.3E6	780.5E6	50.732	45.140
5)	MB Aldrin	5.277	4.374	196.3E6	757.6E6	50.403	45.267
6)	B beta-BHC	4.519	4.028	78404569	328.8E6	44.837	42.013
7)	B delta-BHC	4.768	4.265	207.1E6	794.3E6	52.085	45.751
8)	B Heptachlo...	5.696	4.878	174.5E6	694.0E6	48.339	44.267
9)	A Endosulfan I	6.078	5.251	161.3E6	658.6E6	48.276m	45.438m
10)	B trans-Chl...	5.951	5.131	168.3E6	721.2E6	48.153	44.321
11)	B cis-Chlor...	6.031	5.195	179.1E6	715.1E6	50.430m	45.522m
12)	B 4,4'-DDE	6.201	5.382	331.3E6	1342.3E6	100.117	90.103
13)	MA Dieldrin	6.352	5.519	364.1E6	1380.2E6	100.675	90.157
14)	MA Endrin	6.580	5.795	300.7E6	1239.7E6	100.659	88.735
15)	B Endosulfa...	6.791	6.086	280.5E6	1165.0E6	93.836	85.803
16)	A 4,4'-DDD	6.710	5.936	264.0E6	1091.9E6	101.847	89.673
17)	MA 4,4'-DDT	7.026	6.190	254.1E6	1053.5E6	94.764m	83.561
18)	B Endrin al...	6.919	6.264	194.0E6	807.3E6	82.639	77.262
19)	B Endosulfa...	7.154	6.488	274.3E6	1129.6E6	94.641	85.444
20)	A Methoxychlor	7.498	6.762	662.8E6	2247.7E6	445.499	385.536
21)	B Endrin ke...	7.635	6.997	298.6E6	1193.7E6	93.069	82.584

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122324\
Data File : PD087323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 20:29
Operator : AR\AJ
Sample : P5331-03MSD
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:07:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 23:32:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

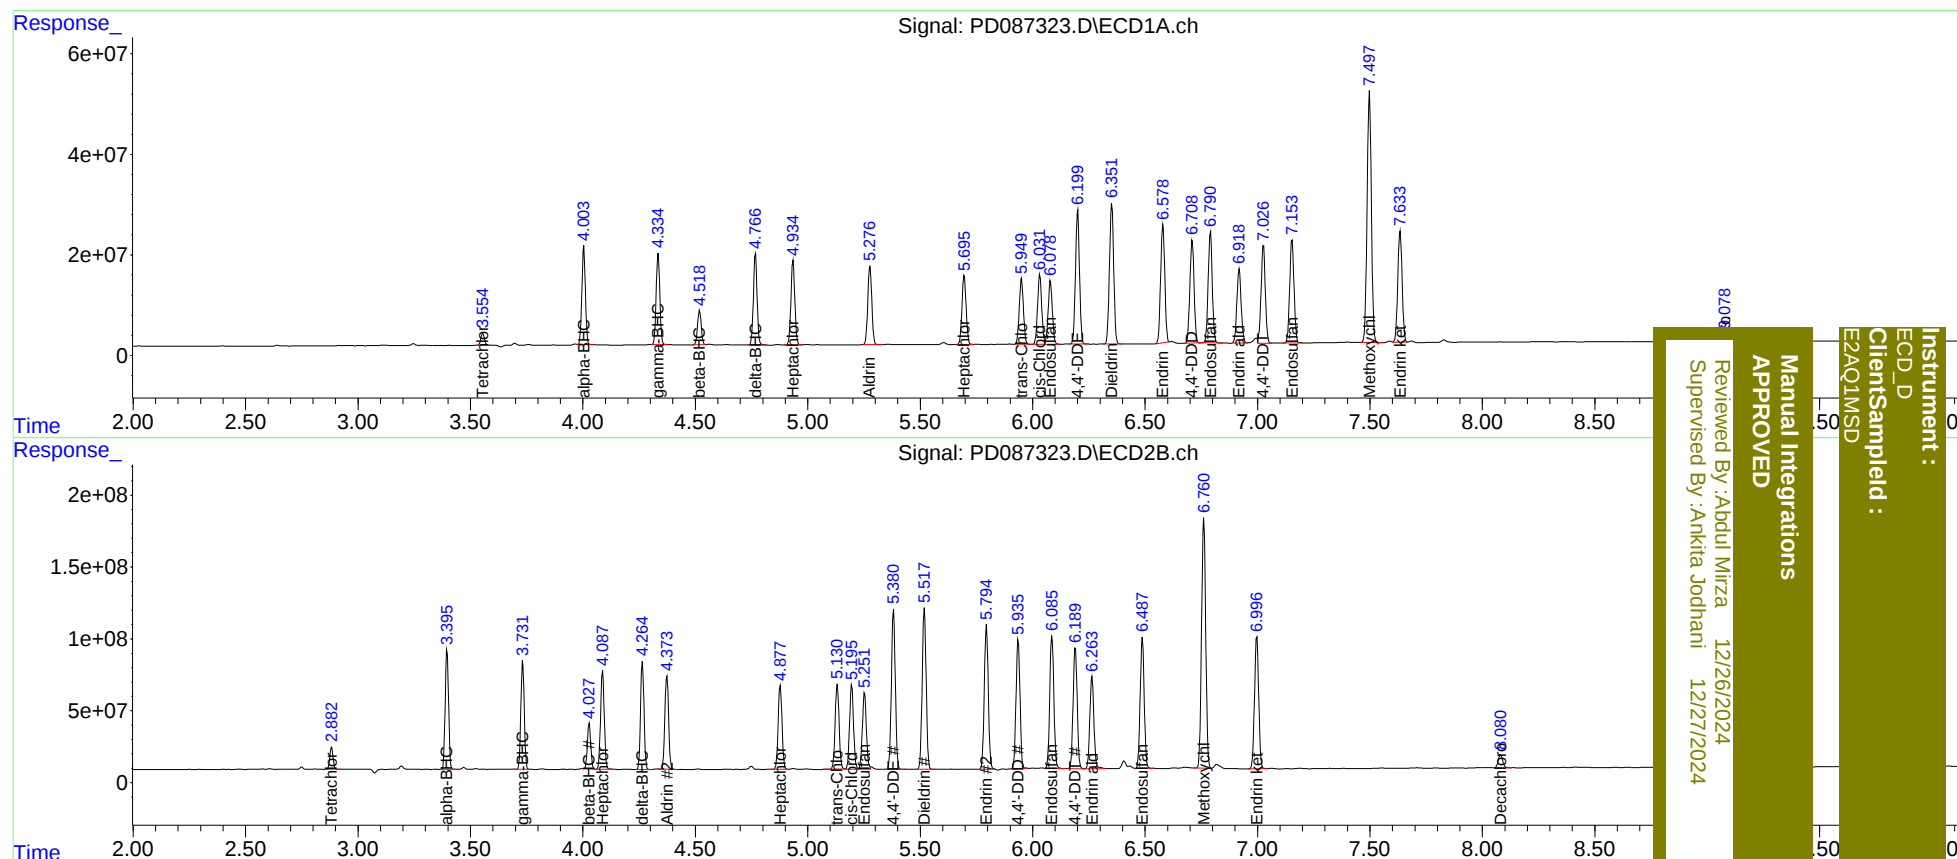

Instrument :
ECD_D
ClientSampled :
EZAQ1MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 12/26/2024
Supervised By: Ankita Jodhani 12/27/2024