

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122324\  
 Data File : PD087330.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Dec 2024 22:08  
 Operator : AR\AJ  
 Sample : P5353-01  
 Misc :  
 ALS Vial : 39 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 E2927

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 24 00:09:55 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD122024CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Dec 20 23:32:53 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|----------|---------|--------|--------|
| -----                       |       |       |          |         |        |        |
| System Monitoring Compounds |       |       |          |         |        |        |
| 1) SA Tetrachlo...          | 3.556 | 2.884 | 39900057 | 245.9E6 | 19.488 | 21.132 |
| 27) SA Decachlor...         | 9.080 | 8.081 | 46510987 | 201.6E6 | 15.229 | 15.307 |


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122324\  
Data File : PD087330.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 23 Dec 2024 22:08  
Operator : AR\AJ  
Sample : P5353-01  
Misc :  
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 24 00:09:55 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD122024CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Dec 20 23:32:53 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

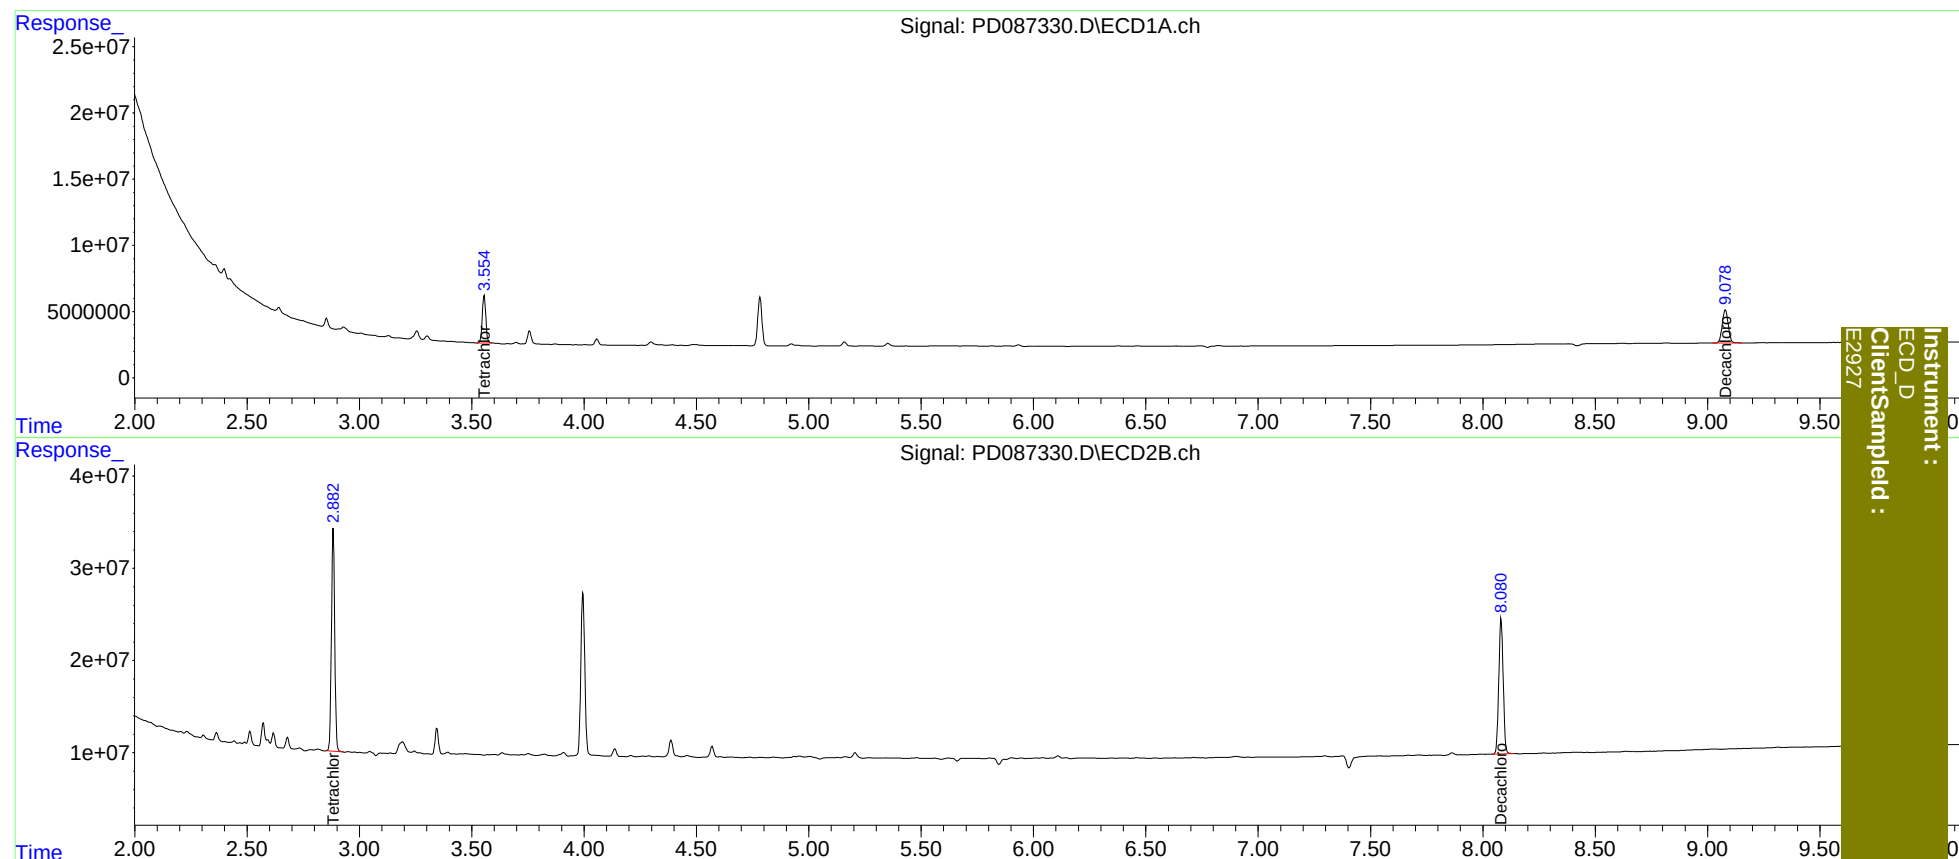

Instrument :  
ECD\_D  
ClientSampled :  
E2927