

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
 Data File : PD080308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 11:23
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 20:44:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	0.000	3.651	0	62486	N.D. <MDL
5) MB	Aldrin	0.000	4.233	0	128168	N.D. <MDL
9) A	Endosulfan I	0.000	5.074f	0	24806	N.D. <MDL
10) B	trans-Chl...	0.000	5.074f	0	24806	N.D. <MDL
11) B	cis-Chlor...	0.000	5.074	0	24806	N.D. <MDL
14) MA	Endrin	0.000	5.680	0	283248	N.D. 0.108
15) B	Endosulfa...	0.000	5.916f	0	219775	N.D. <MDL
18) B	Endrin al...	0.000	6.154	0	137094	N.D. <MDL
22)	Toxaphene-1	0.000	5.074f	0	24806	N.D. 1.455


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 11:23
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 20:44:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

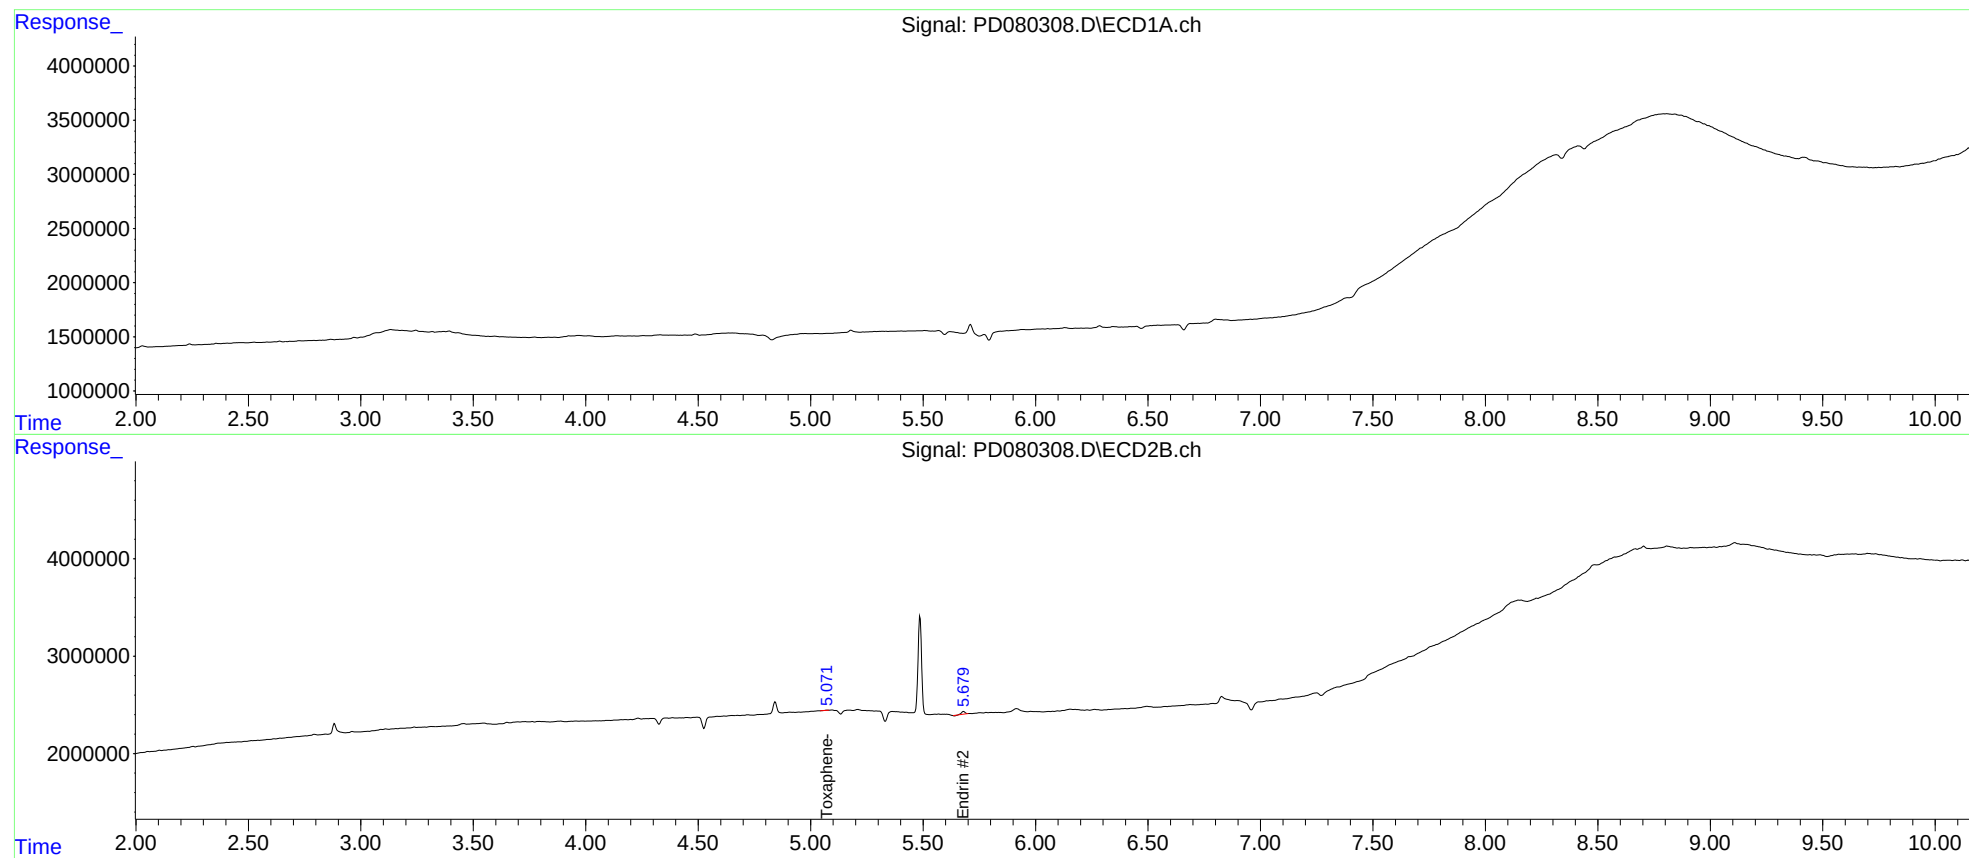

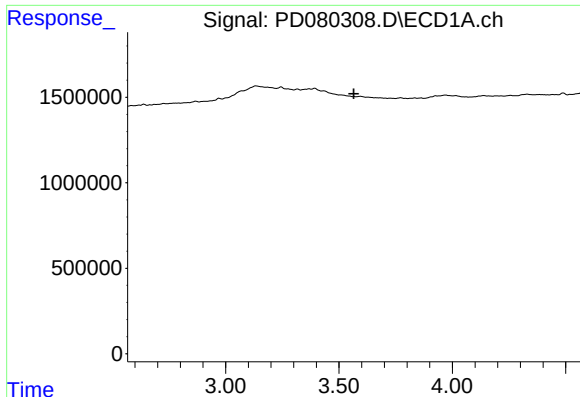


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.566 min
Response: 0
Conc: N.D.

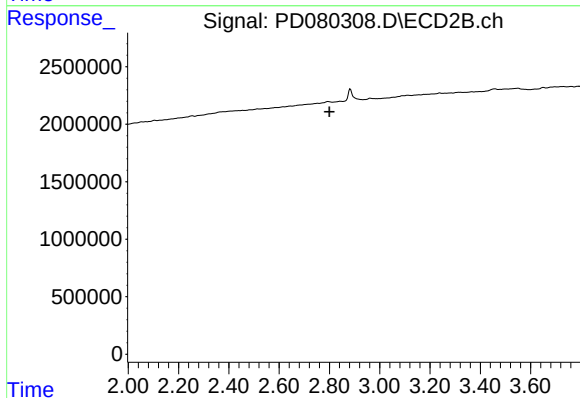


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.800 min
Response: 0
Conc: N.D.

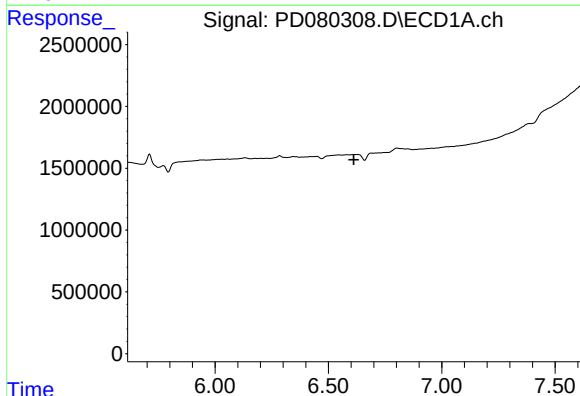


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

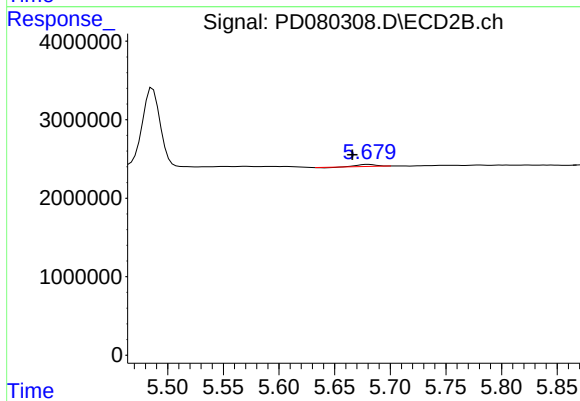


#14 Endrin

R.T.: 5.680 min
Delta R.T.: 0.014 min
Response: 283248
Conc: 0.11 ng/ml

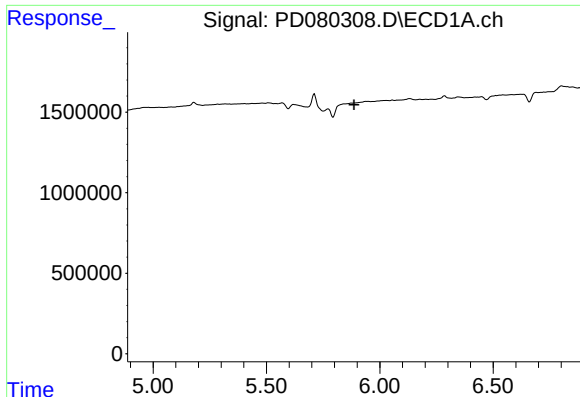


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.886 min
Response: 0
Conc: N.D.

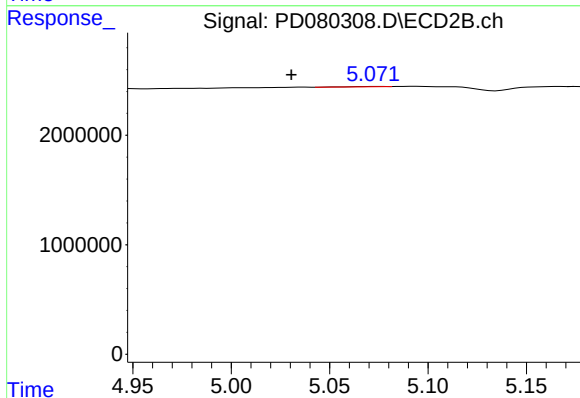


#22 Toxaphene-1

R.T.: 5.074 min
Delta R.T.: 0.043 min
Response: 24806
Conc: 1.46 ng/ml

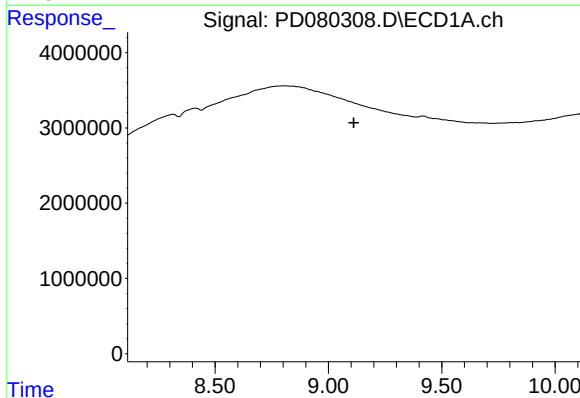

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.

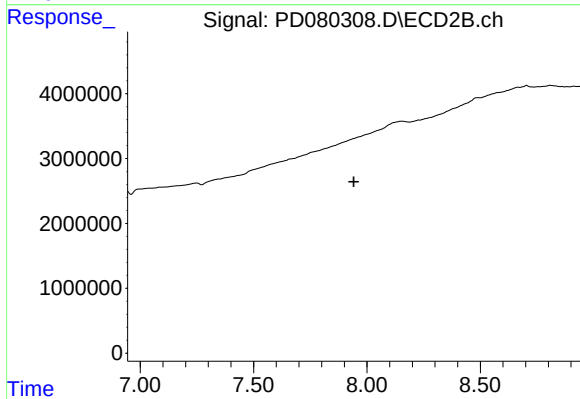

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.942 min
Response: 0
Conc: N.D.