

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
 Data File : PD080350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 22:04
 Operator : AR\AJ
 Sample : 05861-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSD2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2023
 Supervised By : Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 10:43:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.817	20672551	37393028	16.191	16.817m
2)	SA Decachlor...	9.109	7.958	25779542	43445161	16.034m	18.100m
Target Compounds							
8)	B Heptachlo...	5.716	4.773	919547	867630	0.428m	0.256 #
10)	B trans-Chl...	5.972	5.024	918092	1891485	0.447m	0.575 #
11)	B cis-Chlor...	6.055	5.088	1149254	688421	0.548m	0.205 #
13)	MA Dieldrin	6.379	5.406	3464031	6125825	1.861m	2.044m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 22:04
Operator : AR\AJ
Sample : 05861-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 10:43:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

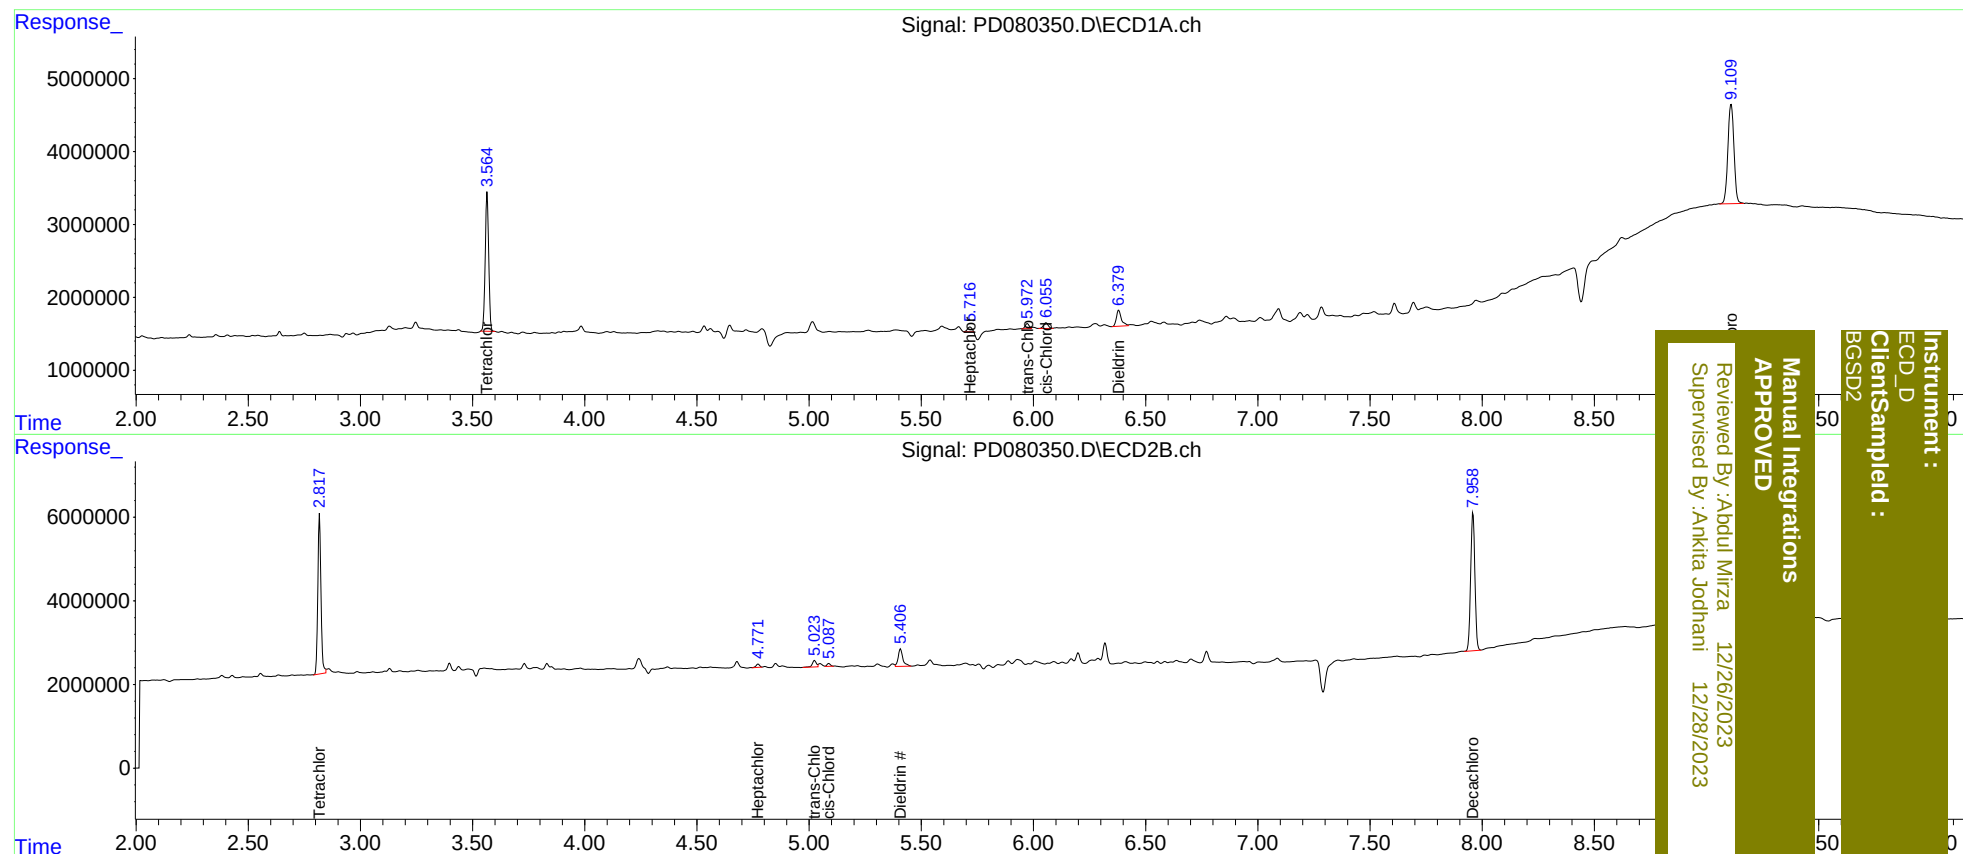

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/26/2023
Supervised By: Ankita Jodhani 12/28/2023

Instrument :
ECD_D
ClientSampled :
BGSD2