

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
 Data File : PD080353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 22:44
 Operator : AR\AJ
 Sample : 05860-10MSD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSC1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2023
 Supervised By : Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 06:00:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.798	25527755	46249462	19.994	20.800
27)	SA Decachlor...	9.111	7.939	32452962	47874947	20.185	19.946
Target Compounds							
2)	A alpha-BHC	4.021	3.300	123.3E6	210.6E6	59.796m	61.782
3)	MA gamma-BHC...	4.354	3.630	110.3E6	193.9E6	55.546m	60.248
4)	MA Heptachlor	4.948	3.971	116.0E6	197.7E6	55.543	61.750
5)	MB Aldrin	5.292	4.252	111.5E6	189.6E6	49.862	53.654
6)	B beta-BHC	4.549	3.925	49282400	84293725	47.479	49.093
7)	B delta-BHC	4.799	4.156	119.9E6	202.1E6	52.186	51.983
8)	B Heptachlo...	5.718	4.753	102.2E6	174.5E6	47.596	51.500
9)	A Endosulfan I	6.104	5.124	96663083	161.4E6	54.263	58.879
10)	B trans-Chl...	5.974	5.003	99263347	172.0E6	48.369	52.260
11)	B cis-Chlor...	6.054	5.068	102.0E6	173.4E6	48.610	51.583
12)	B 4,4'-DDE	6.224	5.257	194.0E6	335.4E6	100.401	106.783
13)	MA Dieldrin	6.380	5.388	211.2E6	363.4E6	113.457	121.269
14)	MA Endrin	6.611	5.663	180.2E6	324.7E6	115.058	123.422
15)	B Endosulfa...	6.828	5.956	176.0E6	299.1E6	93.905	103.170
16)	A 4,4'-DDD	6.741	5.811	156.9E6	271.2E6	113.135	117.966
17)	MA 4,4'-DDT	7.057	6.062	163.7E6	283.8E6	110.788	117.707
18)	B Endrin al...	6.958	6.135	125.2E6	207.1E6	83.922	89.830
19)	B Endosulfa...	7.192	6.357	178.5E6	288.6E6	97.303	102.895
20)	A Methoxychlor	7.531	6.636	435.0E6	680.1E6	549.461	540.241
21)	B Endrin ke...	7.679	6.864	183.3E6	322.5E6	94.185	100.766

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 22:44
Operator : AR\AJ
Sample : 05860-10MSD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 06:00:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

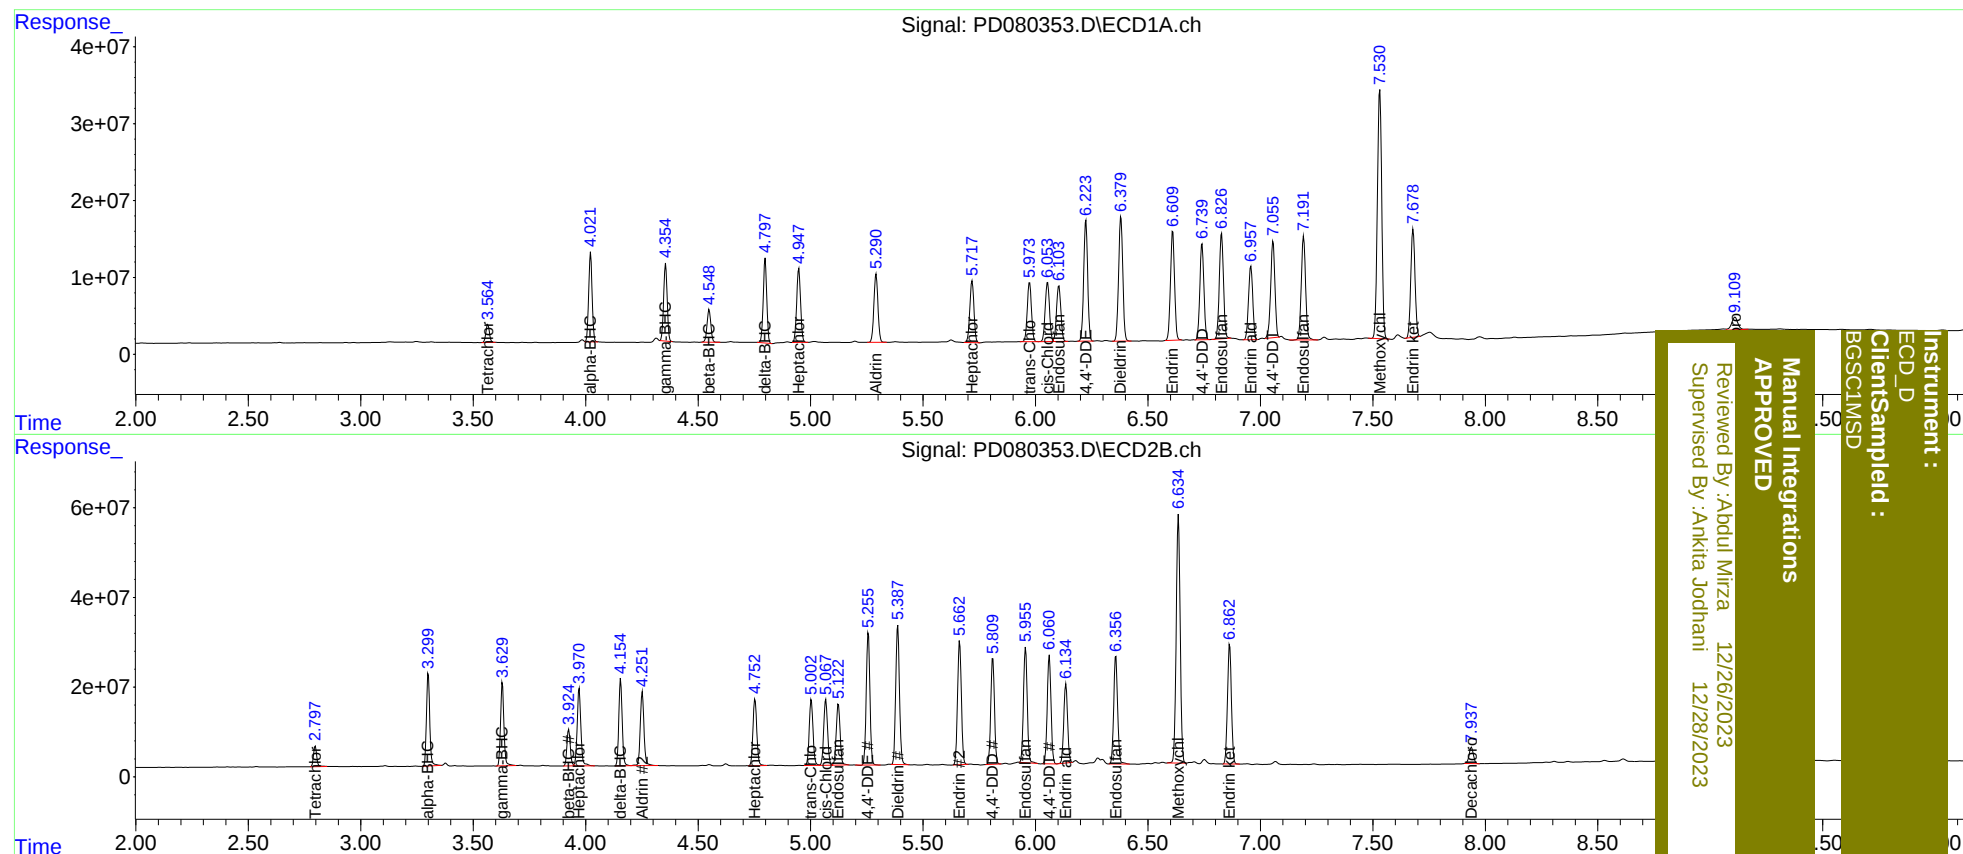

Instrument :
ECD_D
Client Sampled :
BGSCLMSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/26/2023
Supervised By: Ankita Jodhani 12/28/2023