

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
 Data File : PD080377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 04:17
 Operator : AR\AJ
 Sample : 05859-18MS
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRY7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/21/2024
 Supervised By : Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 06:37:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 13 07:09:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.798	21696604	42208717	16.993	18.982
27)	SA Decachlor...	9.110	7.938	24094523	77862364	14.986m	32.439m#
Target Compounds							
2)	A alpha-BHC	4.022	3.301	106.8E6	193.7E6	51.799	56.825
3)	MA gamma-BHC...	4.357	3.629	124.2E6	263.5E6	62.544	81.855 #
4)	MA Heptachlor	4.947	3.971	231.9E6	309.1E6	111.052	96.527
5)	MB Aldrin	5.291	4.253	611.0E6	752.8E6	273.181m	213.081
6)	B beta-BHC	4.550	3.927	60097536	167.8E6	57.898	97.751 #
7)	B delta-BHC	4.797	4.149	124.3E6	567.4E6	54.131m	145.936m#
8)	B Heptachlo...	5.714	4.747	877.7E6	1584.0E6	408.564m	467.404m
9)	A Endosulfan I	6.111	5.134	223.6E6	399.2E6	125.546m	145.633
10)	B trans-Chl...	5.972	5.004	406.7E6	1433.5E6	198.187m	435.473m#
11)	B cis-Chlor...	6.057	5.077	48875075	766.8E6	23.284m	228.073 #
12)	B 4,4'-DDE	6.197	5.244	1486.5E6	2921.4E6	769.506m	930.075m
13)	MA Dieldrin	6.379	5.387	4404.5E6	7223.9E6	2366.644m	2410.413m
14)	MA Endrin	6.582	5.669	1147.7E6	1843.3E6	732.763m	700.598
15)	B Endosulfa...	6.847	5.958	703.6E6	345.3E6	375.292m	119.104m#
16)	A 4,4'-DDD	6.743	5.826	1050.3E6	1157.1E6	757.192m	503.262m#
17)	MA 4,4'-DDT	7.093f	6.066	4513.1E6	1429.5E6	3053.998m	592.853m#
18)	B Endrin al...	6.957	6.145	195.2E6	738.6E6	130.861m	320.295m#
19)	B Endosulfa...	7.187	6.389	4462.6E6	2012.6E6	2433.090m	717.551m#
20)	A Methoxychlor	7.522	6.621	1042.0E6	2868.2E6	1316.014m	2278.546 #
21)	B Endrin ke...	7.659	6.865	1036.8E6	471.8E6	532.847m	147.432m#
22)	Toxaphene-1	5.888	5.030	855.7E6	641.3E6	138085.299	37651.873m#
23)	Toxaphene-2	6.477	5.350	2507.1E6	3007.0E6	140419.907m	172497.409m
24)	Toxaphene-3	7.093	6.621	4587.0E6	2868.2E6	87968.090m	46447.898 #
25)	Toxaphene-4	7.187	6.753	3339.1E6	4932.8E6	85178.650m	58562.226 #
26)	Toxaphene-5	7.608	7.067	2266.8E6	2936.1E6	78760.782m	82755.868

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 04:17
Operator : AR\AJ
Sample : 05859-18MS
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 06:37:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Tue Feb 13 07:09:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

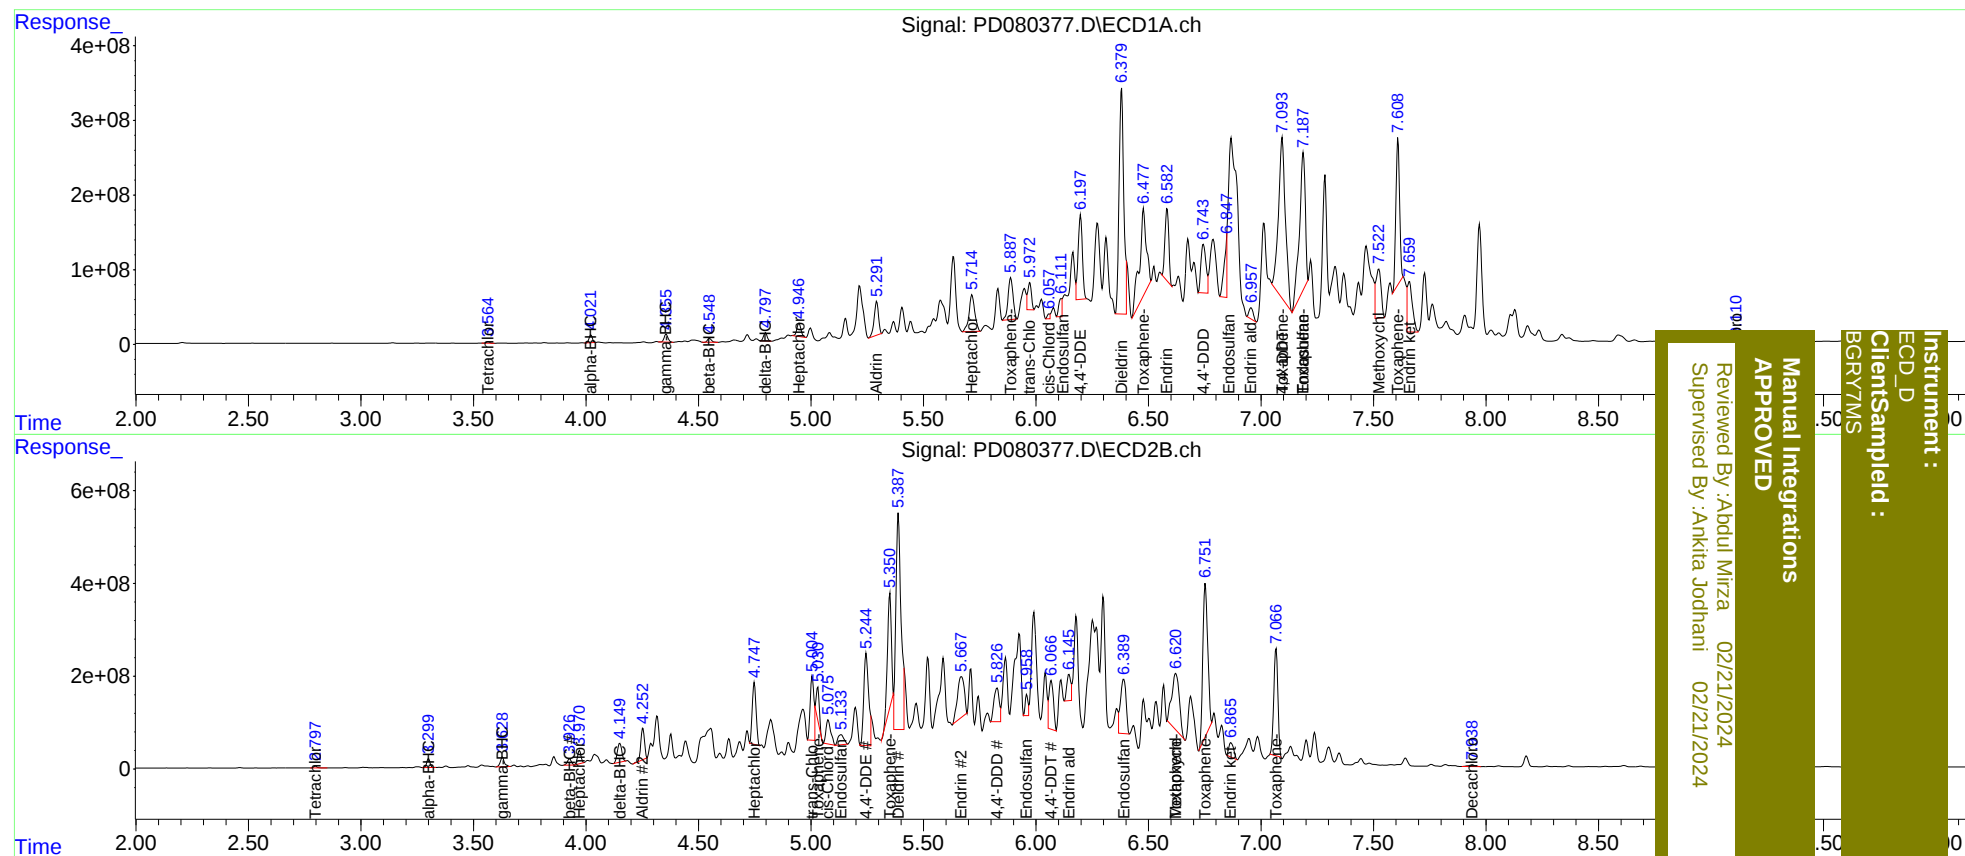

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 02/21/2024
Supervised By: Ankita Jodhani 02/21/2024

Instrument :
ECD_D
Client Sampled :
BGRYTMS