

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 00:18
Operator : AR\AJ
Sample : 05861-03
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGS82

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 06:04:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

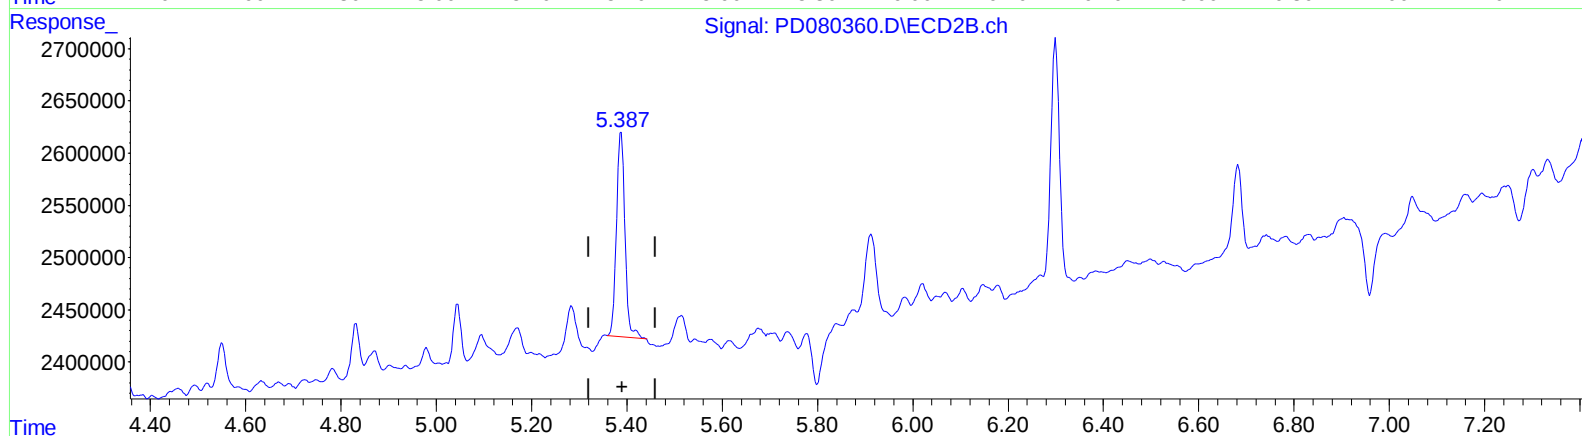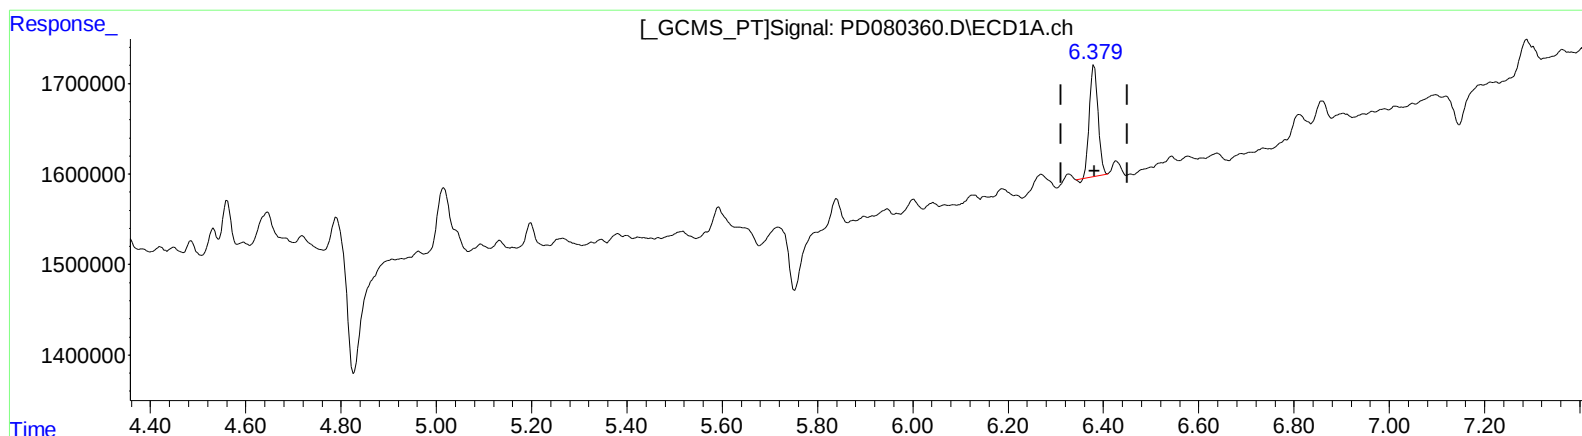

QEdit

(13) Dieldrin (MA)
6.380min 0.830 ng/ml
response 1545252

(13) Dieldrin #2 (MA)
5.388min 0.803 ng/ml
response 2406759

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 00:18
Operator : AR\AJ
Sample : 05861-03
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
BGS82

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 06:04:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

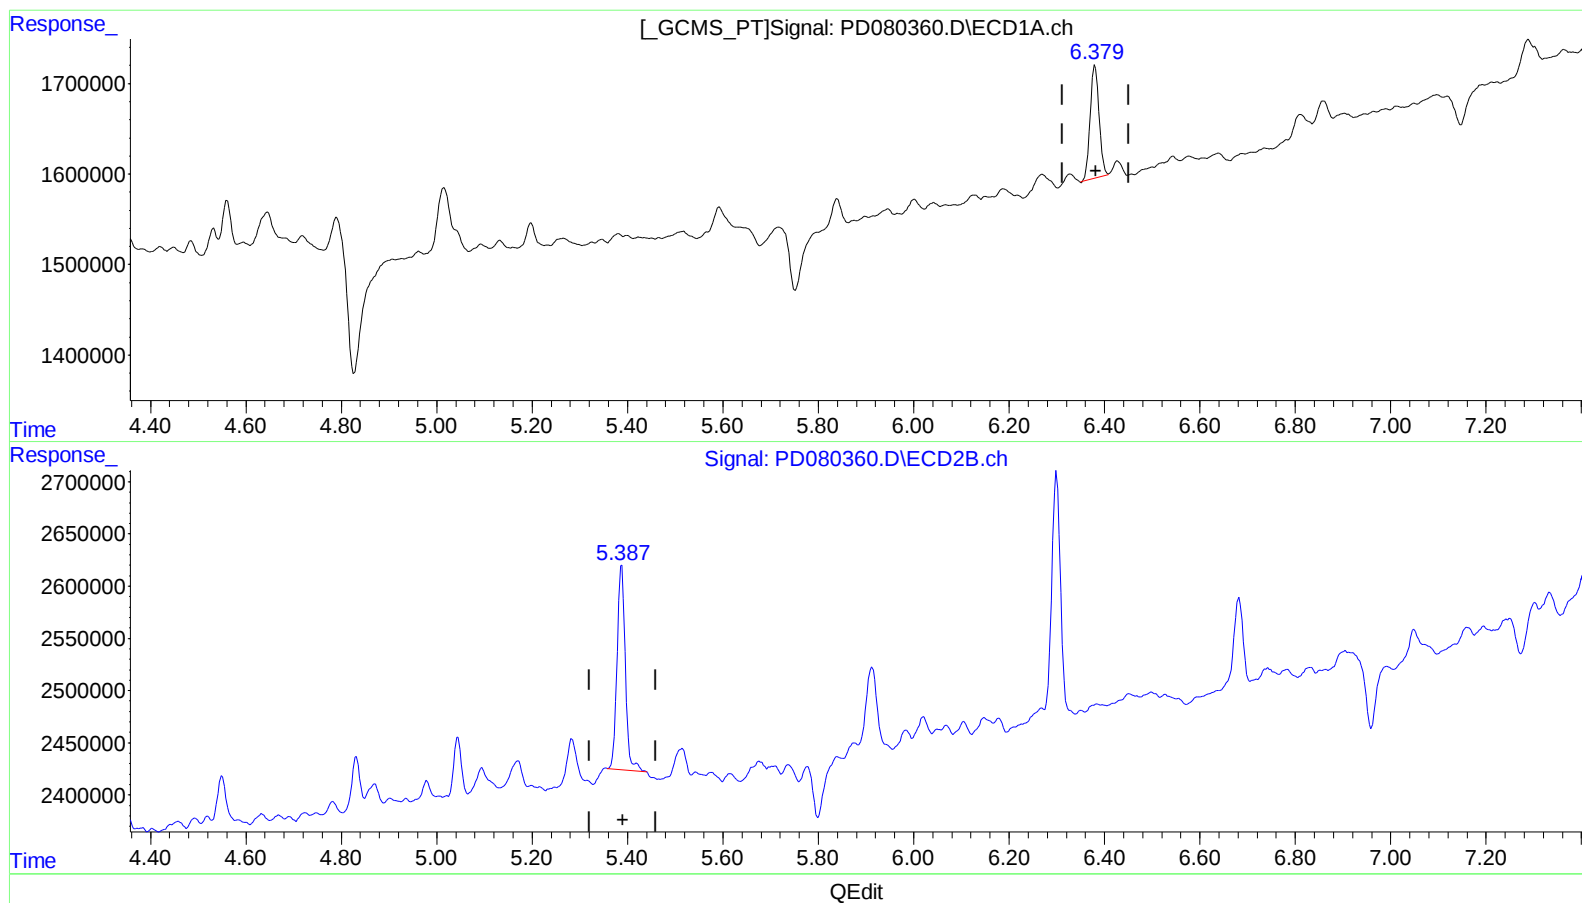

(13) Dieldrin (MA)
6.379min 0.866 ng/ml m
response 1611151

(13) Dieldrin #2 (MA)
5.388min 0.803 ng/ml
response 2406759

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 00:18
Operator : AR\AJ
Sample : 05861-03
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGS82

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 06:04:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

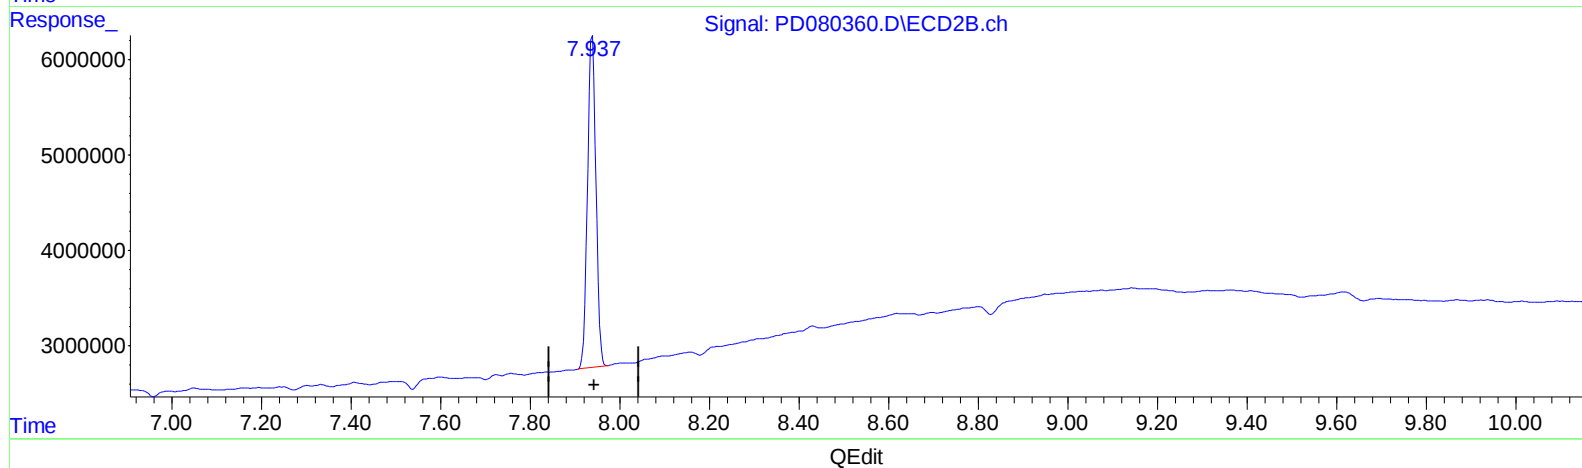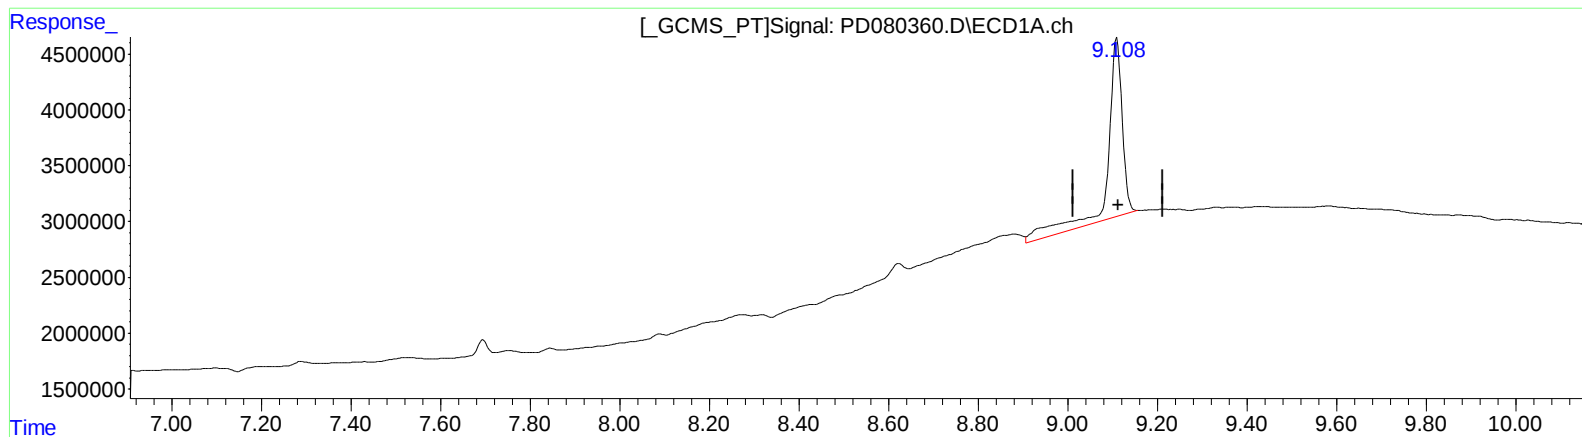

(27) Decachlorobiphenyl (SA)

9.109min 22.838 ng/ml

response 36717455

(27) Decachlorobiphenyl #2 (SA)

7.938min 18.982 ng/ml

response 45560793

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 00:18
Operator : AR\AJ
Sample : 05861-03
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGS82

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 06:04:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

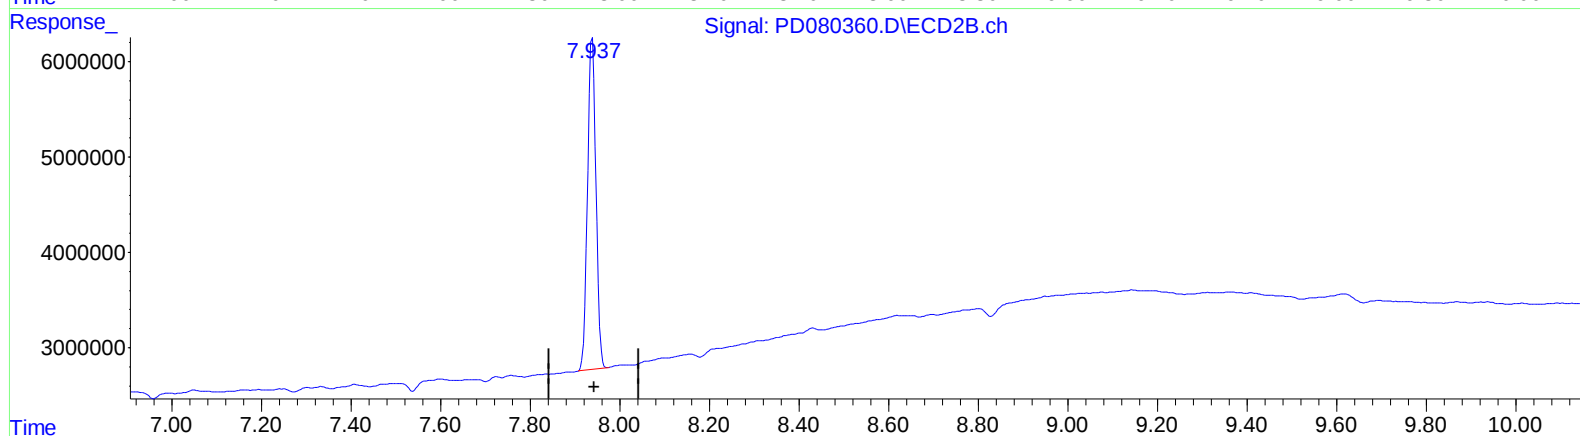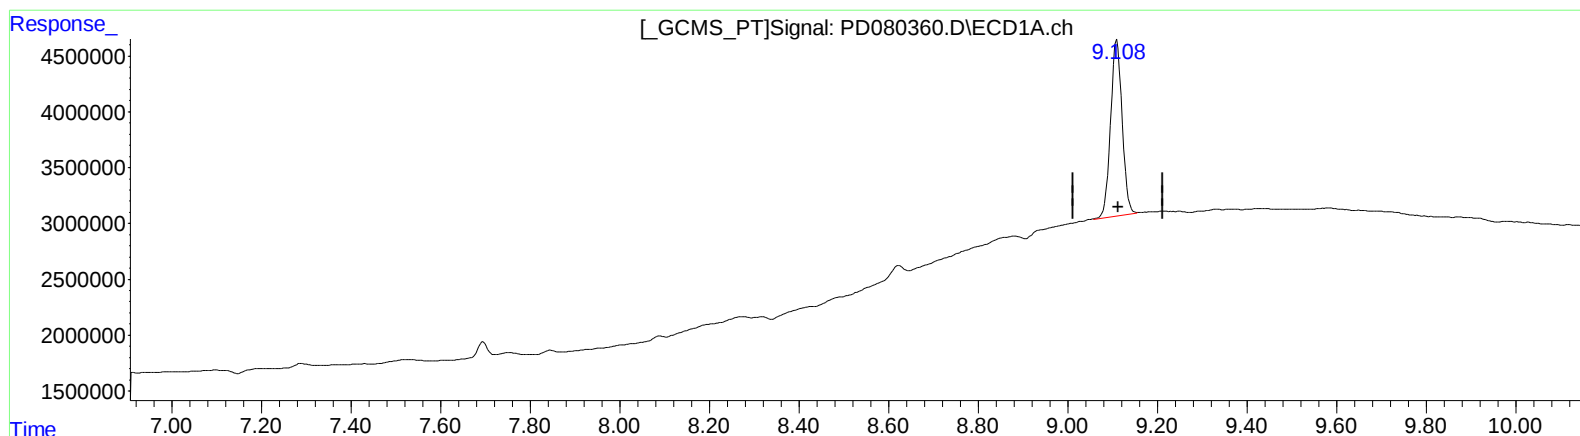

QEdit

(27) Decachlorobiphenyl (SA)

9.108min 17.554 ng/ml m

response 28222401

(27) Decachlorobiphenyl #2 (SA)

7.938min 18.982 ng/ml

response 45560793

(+) = Expected Retention Time

PD121623CLP.M Sat Dec 23 01:52:56 2023

Page: 1