

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
 Data File : PD080340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 19:52
 Operator : AR\AJ
 Sample : 05861-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSC5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 20:53:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.798	21522337	38756583	16.857	17.430
2)	SA Decachlor...	9.109	7.940	24288147	43015560	15.107m	17.921
Target Compounds							
13)	MA Dieldrin	6.379	5.385	2823489	5534472	1.517m	1.847m
19)	B Endosulfa...	7.188	6.385	5588560	4309803	3.047m	1.537m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122423\
Data File : PD080340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 19:52
Operator : AR\AJ
Sample : 05861-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 20:53:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

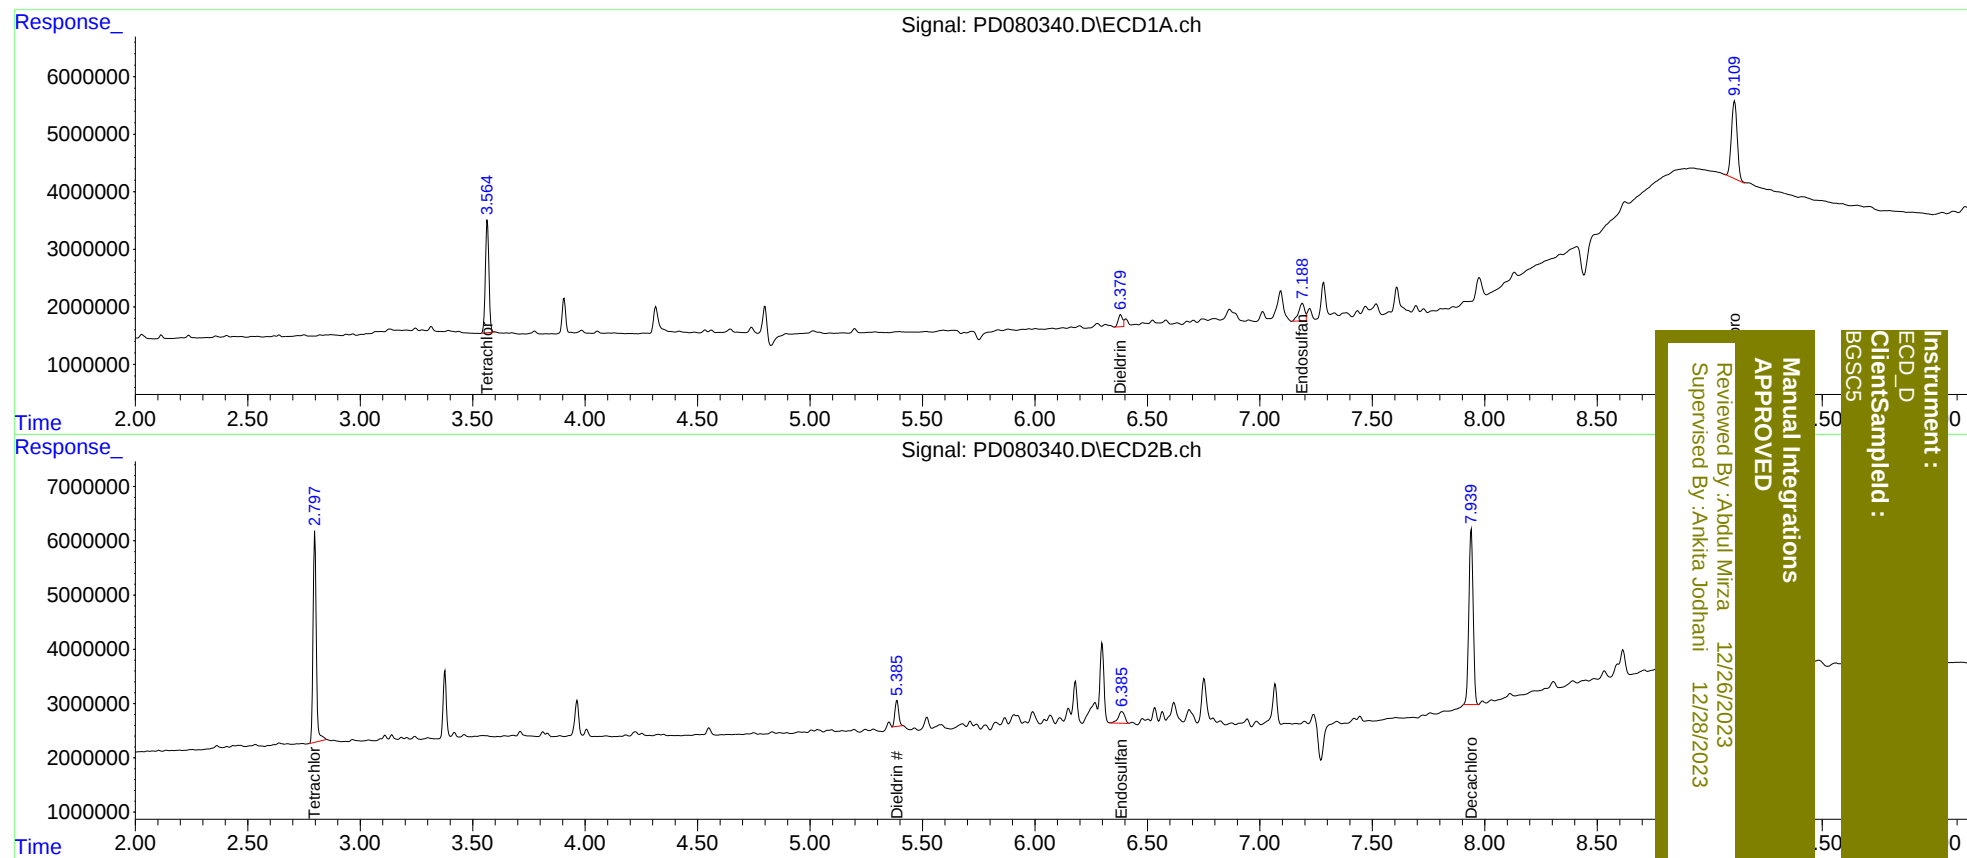

Reviewed By: Abdul Mirza 12/26/2023
Supervised By: Ankita Jodhani 12/28/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGSC5