

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122523\
 Data File : PD080438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2023 15:19
 Operator : AR\AJ
 Sample : 05982-13MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGR63MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 11:47:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.798	26702043	48568592	20.913	21.843
27)	SA Decachlor...	9.110	7.939	38377331	58930683	23.870	24.552
Target Compounds							
2)	A alpha-BHC	4.022	3.300	112.9E6	195.6E6	54.783	57.373
3)	MA gamma-BHC...	4.356	3.630	105.7E6	188.0E6	53.234	58.392
4)	MA Heptachlor	4.948	3.971	108.1E6	179.9E6	51.775	56.184
5)	MB Aldrin	5.292	4.252	104.7E6	176.7E6	46.794	50.021
6)	B beta-BHC	4.548	3.925	46407892	78479793	44.709m	45.707
7)	B delta-BHC	4.799	4.156	110.9E6	187.8E6	48.269	48.311
8)	B Heptachlo...	5.718	4.753	97237503	162.9E6	45.265	48.053
9)	A Endosulfan I	6.104	5.123	91771573	150.0E6	51.517	54.699
10)	B trans-Chl...	5.974	5.003	94551699	159.7E6	46.073	48.506
11)	B cis-Chlor...	6.054	5.067	97746605	161.7E6	46.567	48.111
12)	B 4,4'-DDE	6.224	5.257	182.8E6	313.4E6	94.644	99.779
13)	MA Dieldrin	6.380	5.388	200.2E6	337.0E6	107.584	112.456
14)	MA Endrin	6.610	5.663	167.6E6	298.2E6	106.993	113.328
15)	B Endosulfa...	6.828	5.956	169.3E6	283.1E6	90.307	97.656
16)	A 4,4'-DDD	6.741	5.810	149.3E6	253.6E6	107.624	110.290
17)	MA 4,4'-DDT	7.057	6.061	157.4E6	260.3E6	106.482	107.937
18)	B Endrin al...	6.958	6.134	121.4E6	199.4E6	81.359	86.458
19)	B Endosulfa...	7.192	6.357	163.7E6	267.9E6	89.228	95.500
20)	A Methoxychlor	7.531	6.636	404.7E6	627.0E6	511.106	498.089
21)	B Endrin ke...	7.679	6.863	183.3E6	306.5E6	94.191	95.797

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122523\
Data File : PD080438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2023 15:19
Operator : AR\AJ
Sample : 05982-13MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 11:47:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

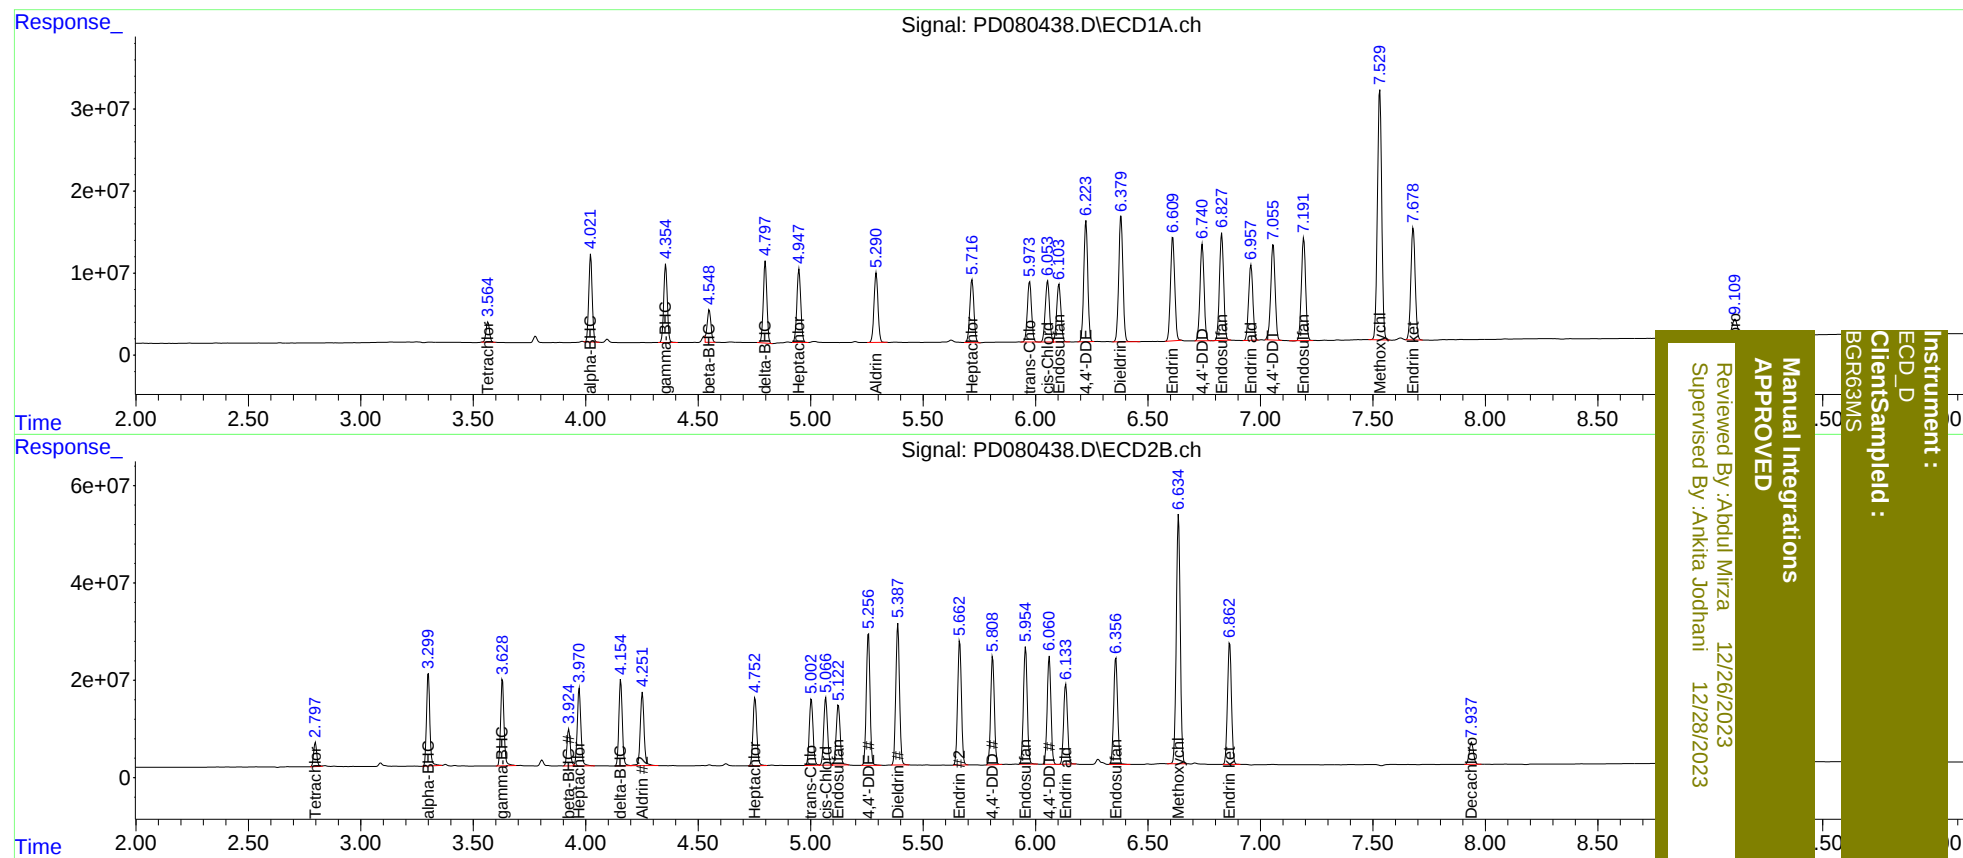

Instrument :
ECD_D
ClientSampled :
BGR63MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 12/26/2023
Supervised By: Ankita Jodhani 12/28/2023