

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
 Data File : PD056773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2019 11:15
 Operator : SG\AJ
 Sample : K6238-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFPZ7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 03:21:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	9025562	17996152	10.898	14.969 #
27)	SA Decachlor...	7.956	8.994	11000611	14783226	12.183	12.287
Target Compounds							
2)	A alpha-BHC	0.000	4.318f	0	229329	N.D.	0.137
4)	MA Heptachlor	0.000	5.091f	0	5735281	N.D.	3.519
7)	B delta-BHC	0.000	4.988f	0	3026149	N.D.	1.817
9)	A Endosulfan I	0.000	6.215	0	415954	N.D.	0.287
10)	B trans-Chl...	0.000	6.051	0	2958493	N.D.	1.789
11)	B cis-Chlor...	0.000	6.129	0	3105272	N.D.	1.927
12)	B 4,4'-DDE	0.000	6.281	0	2303839	N.D.	1.467
20)	A Methoxychlor	0.000	7.582f	0	1432663	N.D.	2.365
22)	Toxaphene-1	0.000	6.281	0	2303839	N.D.	205.207
26)	Toxaphene-5	0.000	7.582	0	1432663	N.D.	56.053


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
Data File : PD056773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2019 11:15
Operator : SG\AJ
Sample : K6238-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFPZ7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 03:21:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

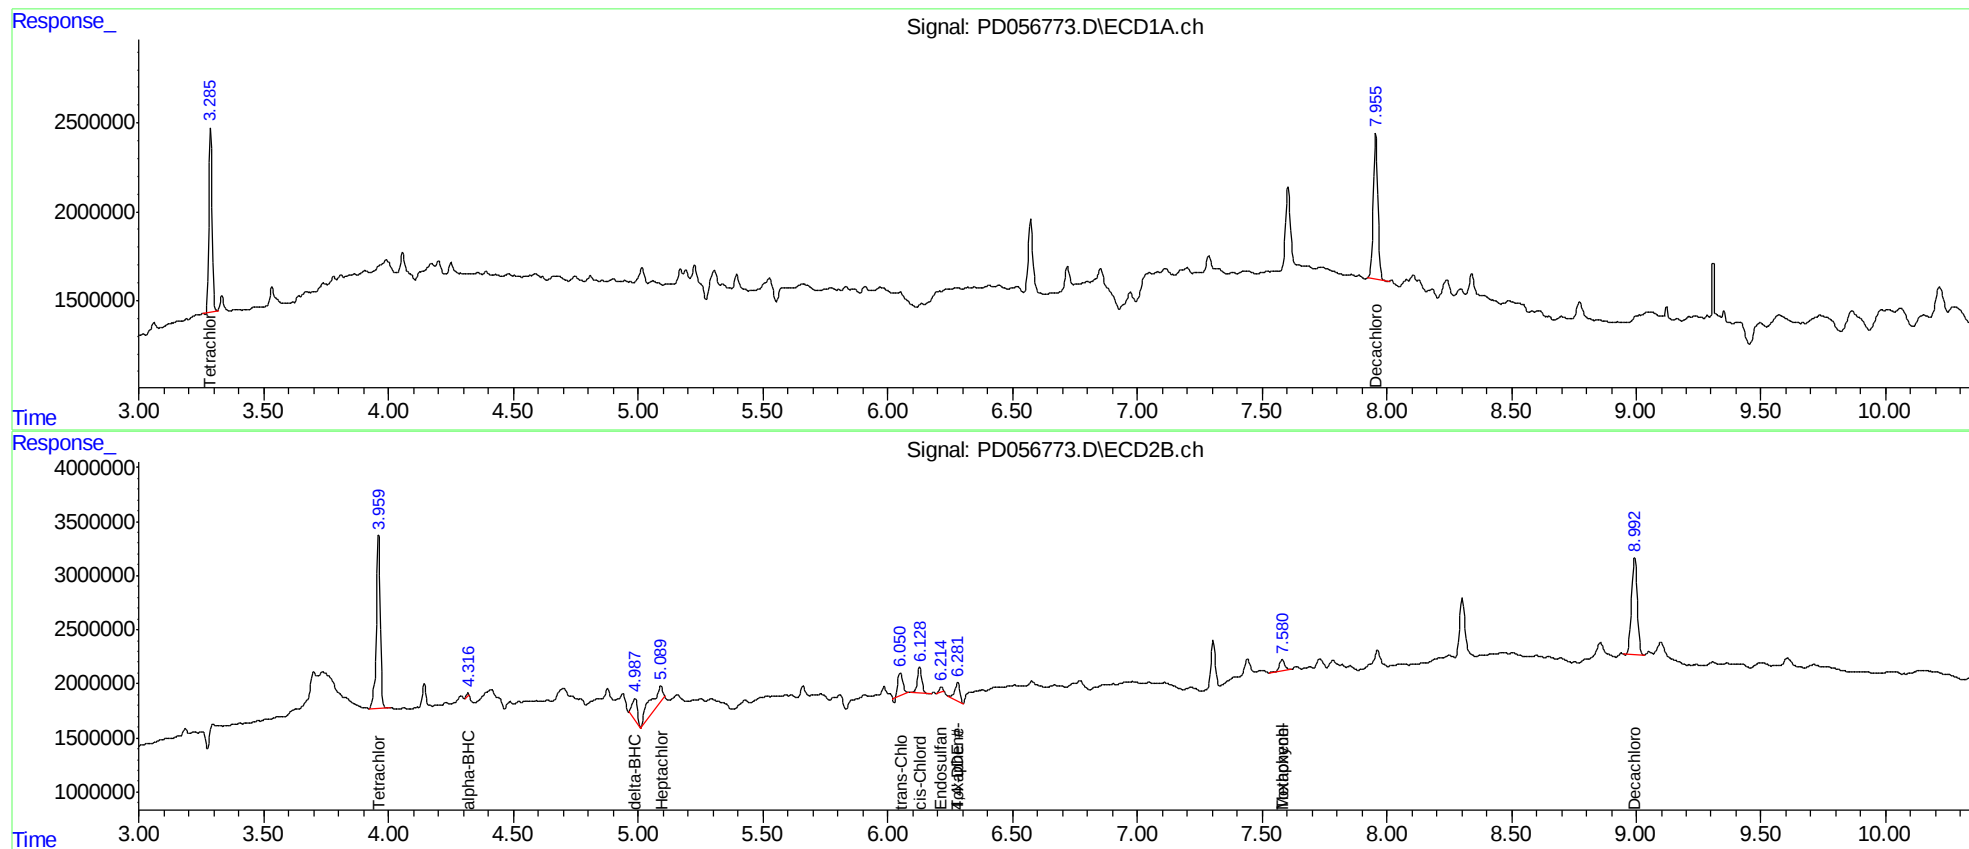


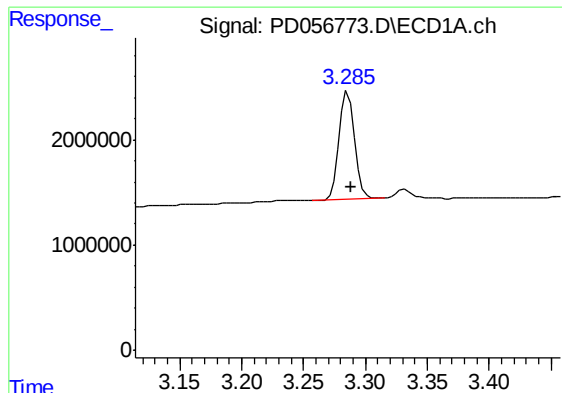

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 9025562
Conc: 10.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFPZ7

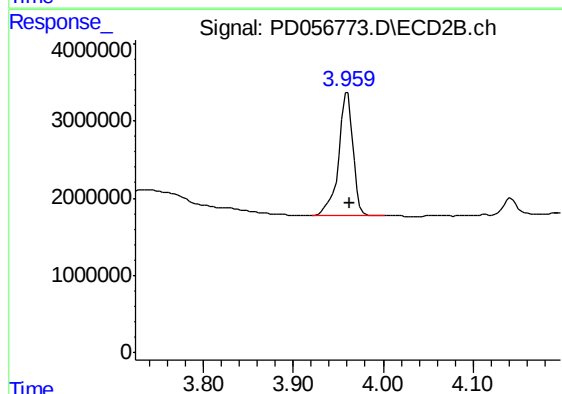


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 17996152
Conc: 14.97 ng/ml

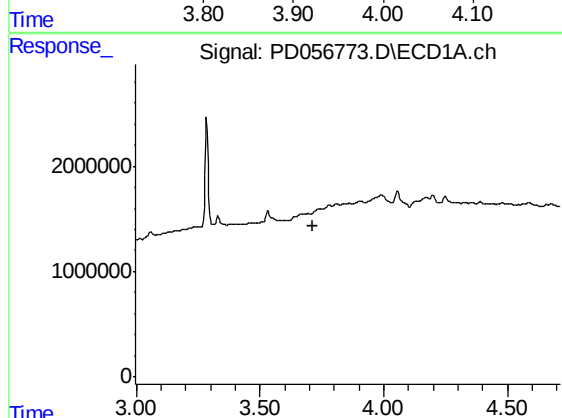


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.715 min
Response: 0
Conc: N.D.

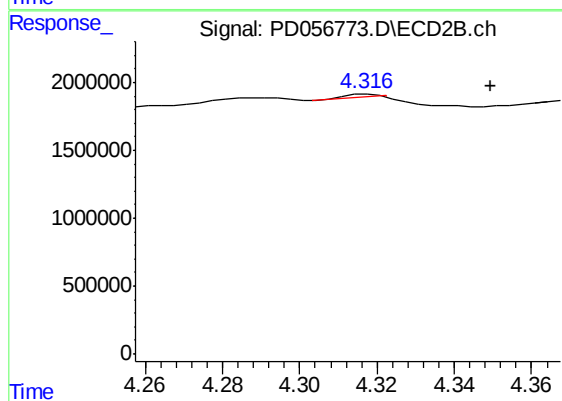

#2 alpha-BHC


R.T.: 4.318 min
Delta R.T.: -0.032 min
Response: 229329
Conc: 0.14 ng/ml

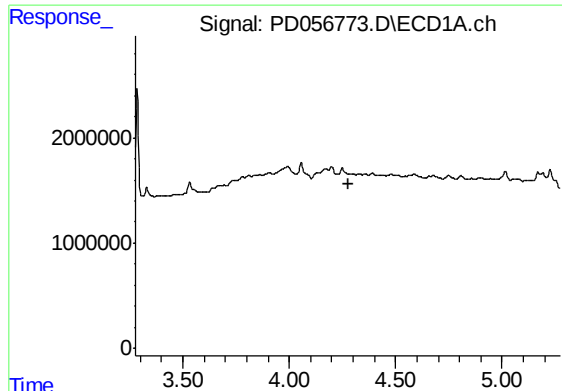

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ7

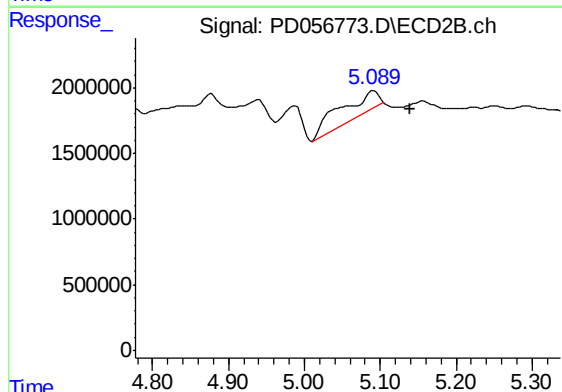


#4 Heptachlor

R.T.: 5.091 min
Delta R.T.: -0.048 min
Response: 5735281
Conc: 3.52 ng/ml

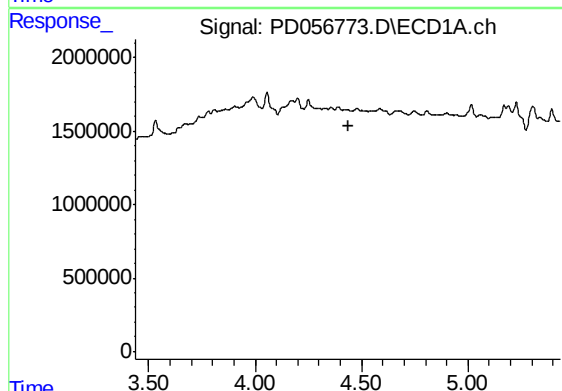


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

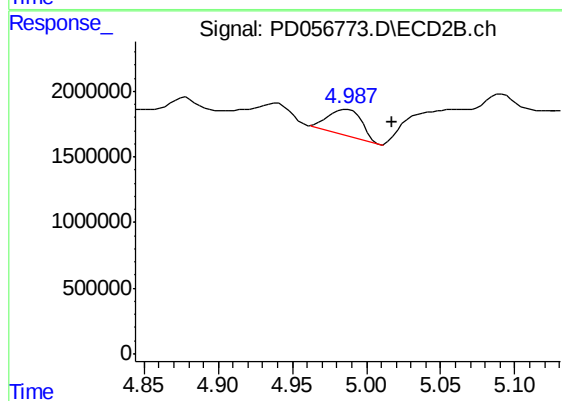

#7 delta-BHC


R.T.: 4.988 min
Delta R.T.: -0.029 min
Response: 3026149
Conc: 1.82 ng/ml

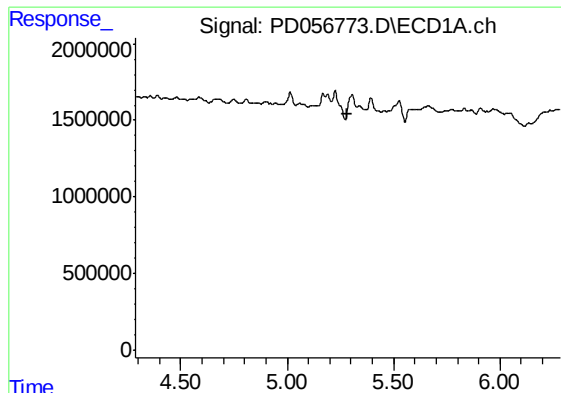

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ7

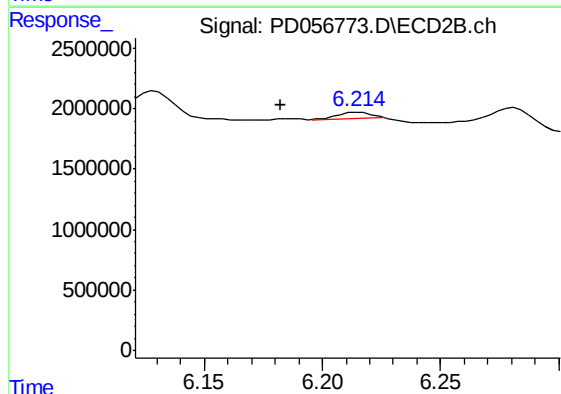


#9 Endosulfan I

R.T.: 6.215 min
Delta R.T.: 0.033 min
Response: 415954
Conc: 0.29 ng/ml

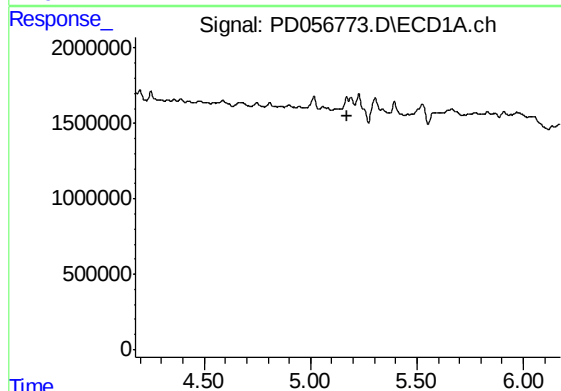


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

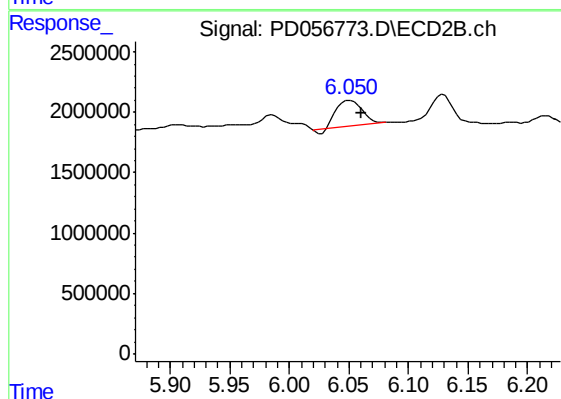

#10 trans-Chlordane


R.T.: 6.051 min
Delta R.T.: -0.009 min
Response: 2958493
Conc: 1.79 ng/ml

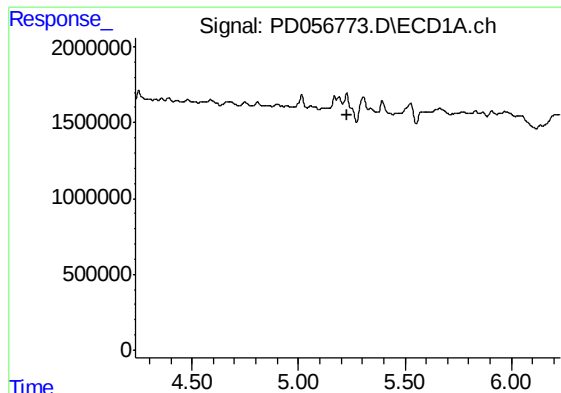

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ7

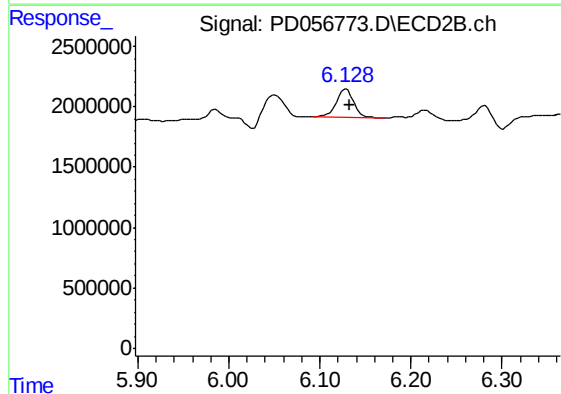


#11 cis-Chlordane

R.T.: 6.129 min
Delta R.T.: -0.003 min
Response: 3105272
Conc: 1.93 ng/ml

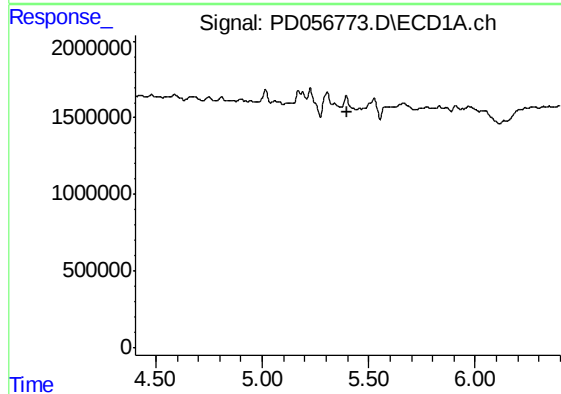


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

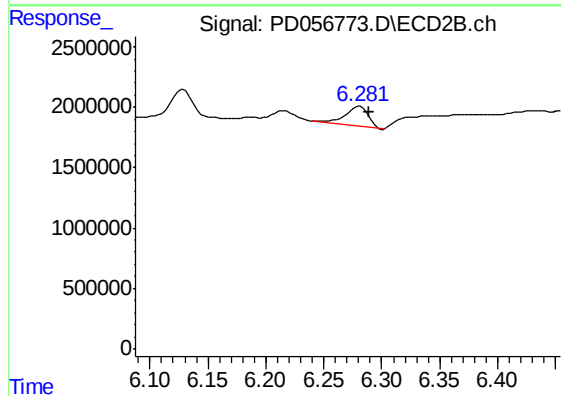

#12 4,4'-DDE


R.T.: 6.281 min
Delta R.T.: -0.008 min
Response: 2303839
Conc: 1.47 ng/ml

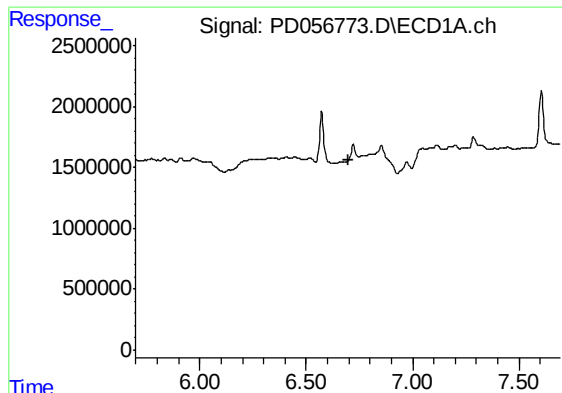

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.696 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ7

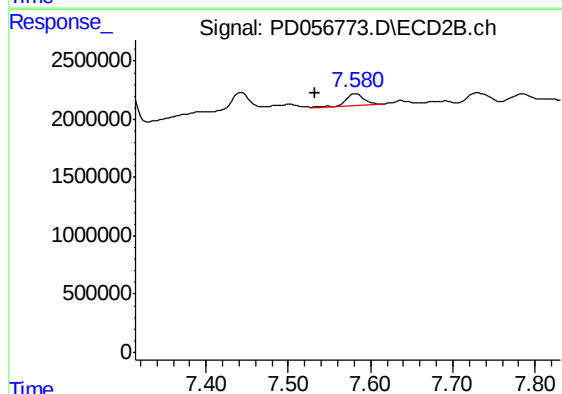


#20 Methoxychlor

R.T.: 7.582 min
Delta R.T.: 0.049 min
Response: 1432663
Conc: 2.36 ng/ml

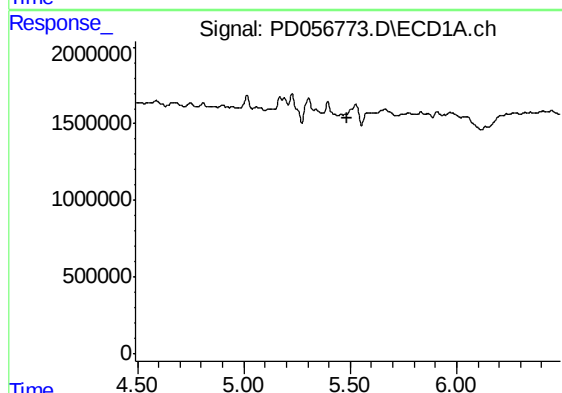


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.489 min
Response: 0
Conc: N.D.

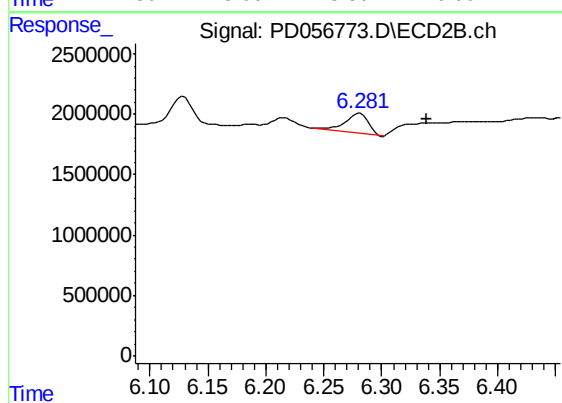

#22 Toxaphene-1


R.T.: 6.281 min
Delta R.T.: -0.058 min
Response: 2303839
Conc: 205.21 ng/ml

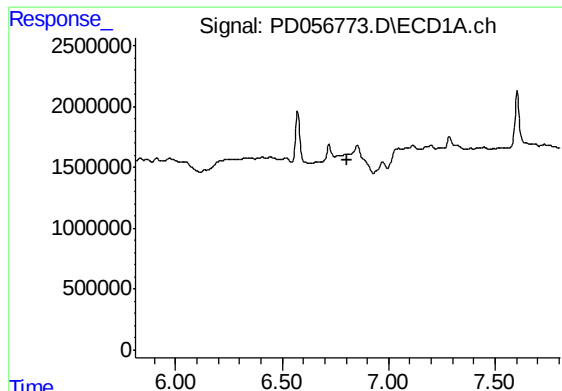

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 6.808 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ7

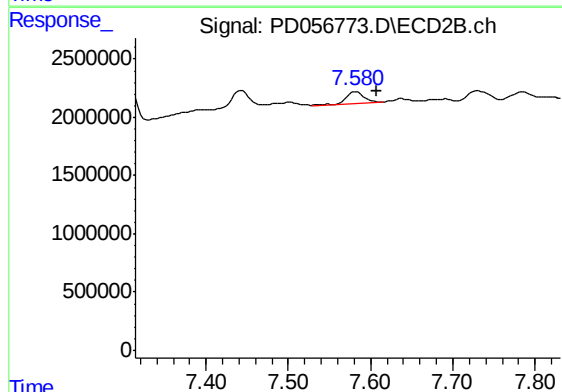


#26 Toxaphene-5

R.T.: 7.582 min
Delta R.T.: -0.026 min
Response: 1432663
Conc: 56.05 ng/ml

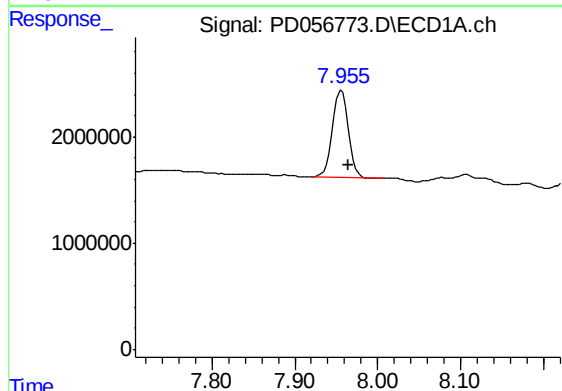

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.009 min
Response: 11000611
Conc: 12.18 ng/ml

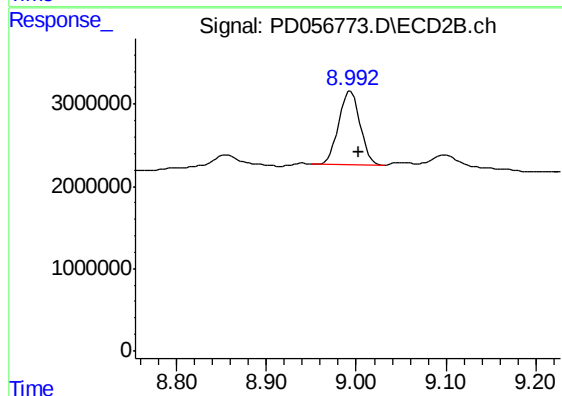

#27 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: -0.009 min
Response: 14783226
Conc: 12.29 ng/ml