

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
 Data File : PD056788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 08:46
 Operator : SG\AJ
 Sample : PB125564BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 10:13:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.959	19390345	35324440	23.413	29.382 #
27)	SA Decachlor...	7.962	8.996	38662101	54614376	42.817	45.393
Target Compounds							
3)	MA gamma-BHC...	0.000	4.644	0	2201784	N.D.	1.364
7)	B delta-BHC	0.000	4.990f	0	1733383	N.D.	1.041
19)	B Endosulfa...	0.000	7.236	0	3533231	N.D.	2.643


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
Data File : PD056788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 08:46
Operator : SG\AJ
Sample : PB125564BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 10:13:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

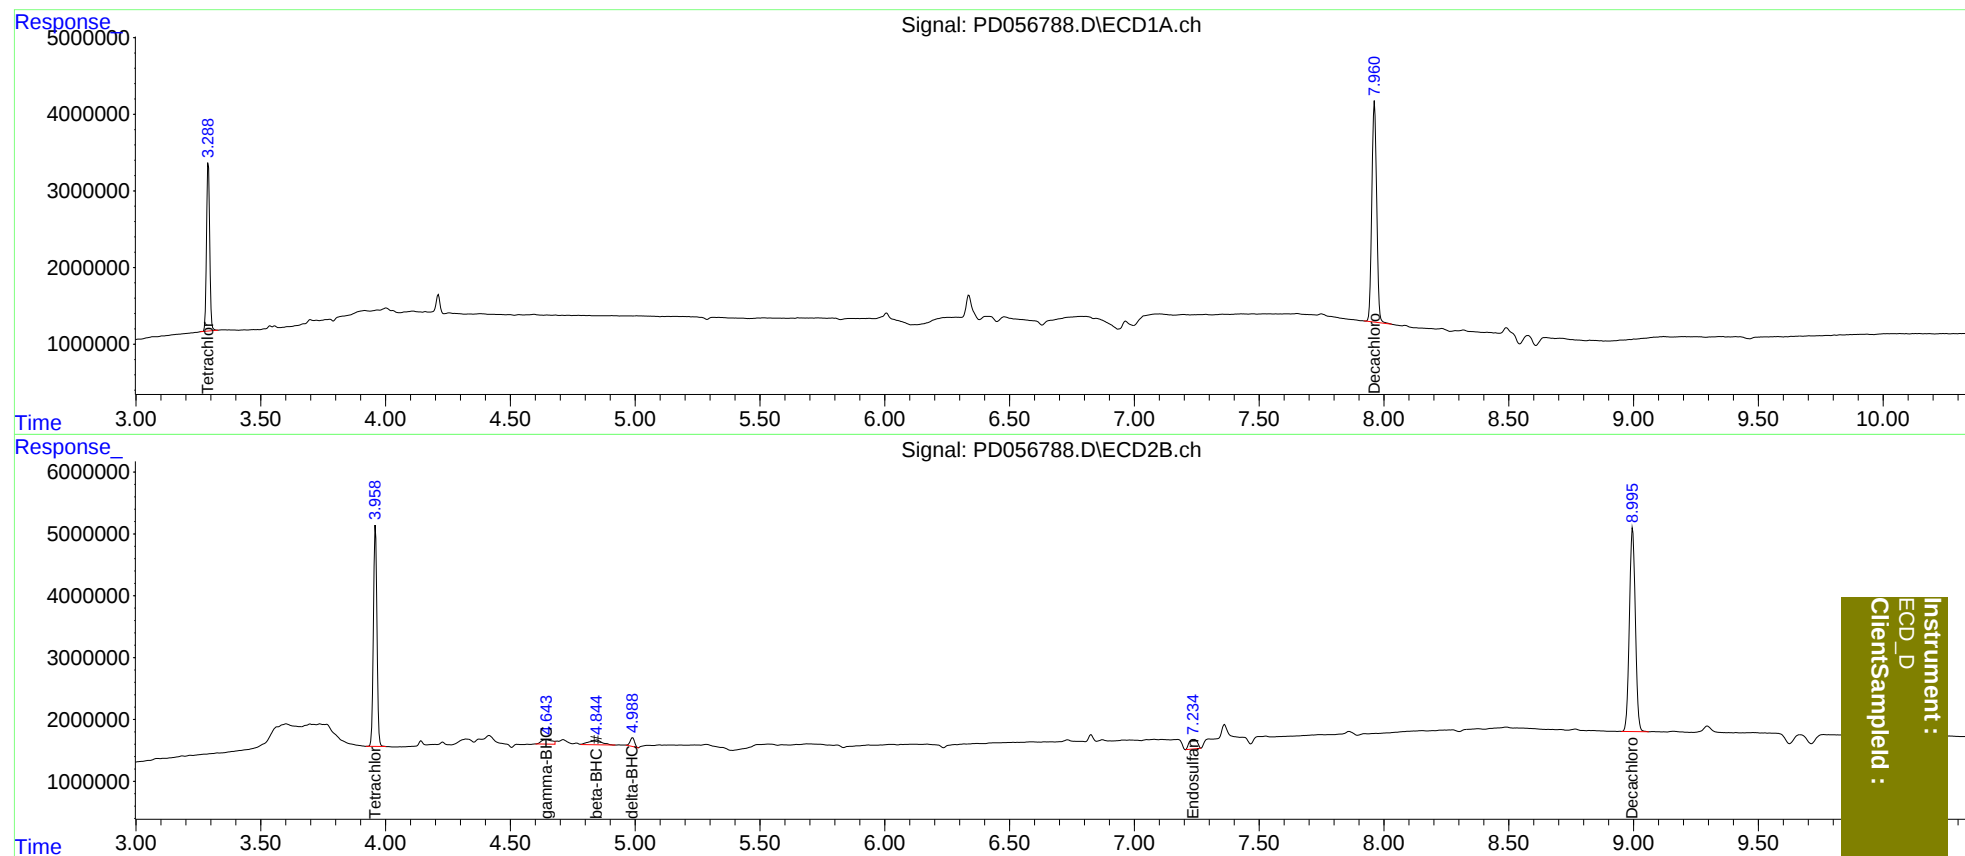


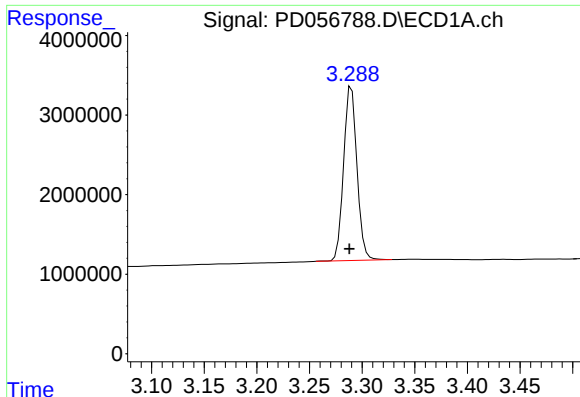

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.002 min
Response: 19390345
Conc: 23.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

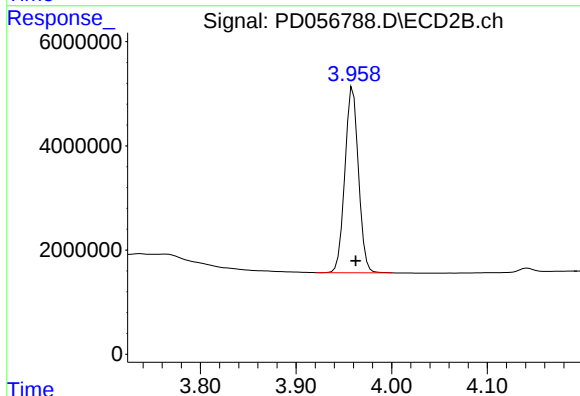


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.003 min
Response: 35324440
Conc: 29.38 ng/ml

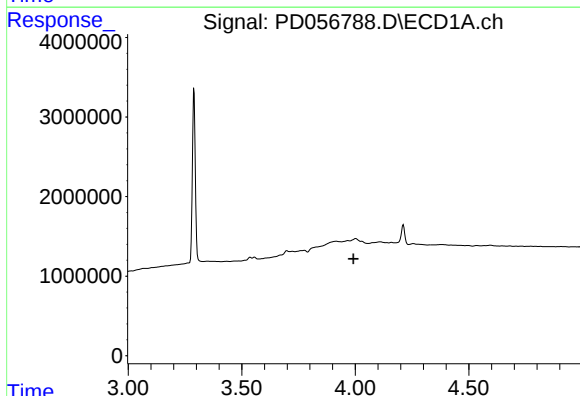


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

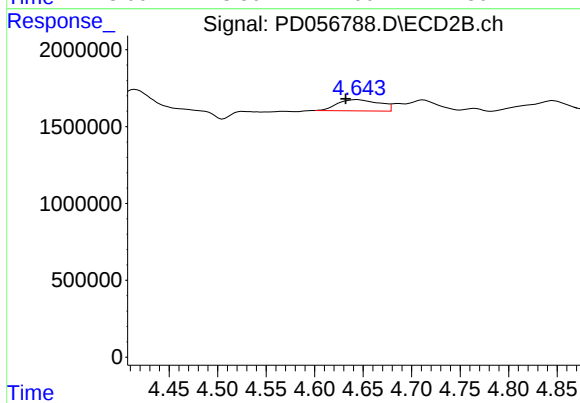

#3 gamma-BHC (Lindane)


R.T.: 4.644 min
Delta R.T.: 0.012 min
Response: 2201784
Conc: 1.36 ng/ml

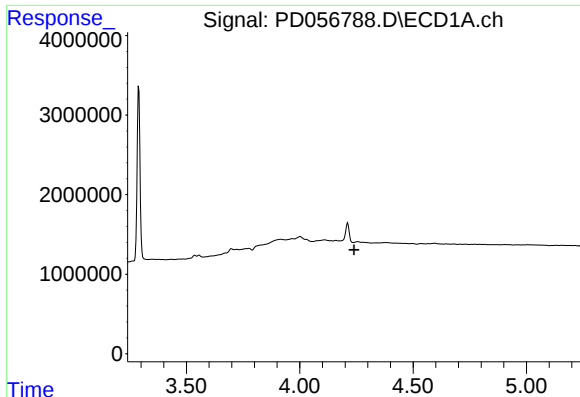

#6 beta-BHC


R.T.: 4.211 min
Delta R.T.: -0.029 min
Response: -2060950
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

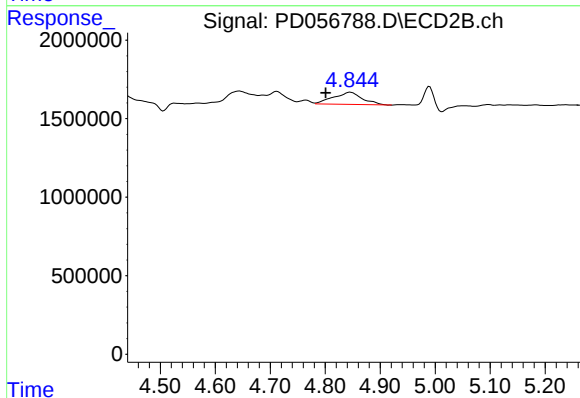


#6 beta-BHC

R.T.: 4.846 min
Delta R.T.: 0.045 min
Response: 2822876
Conc: 3.43 ng/ml

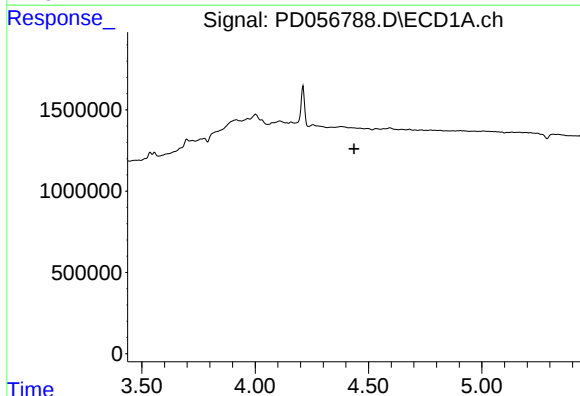


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.436 min
Response: 0
Conc: N.D.

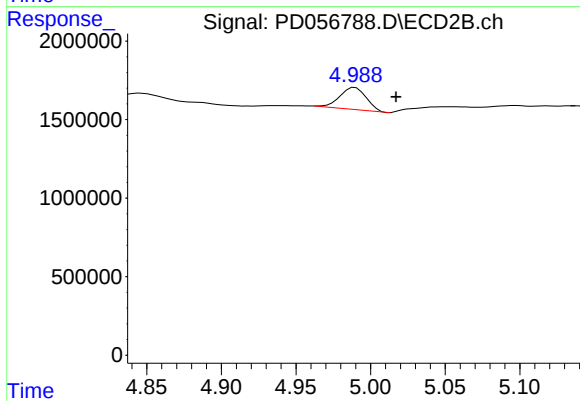

#7 delta-BHC


R.T.: 4.990 min
Delta R.T.: -0.027 min
Response: 1733383
Conc: 1.04 ng/ml

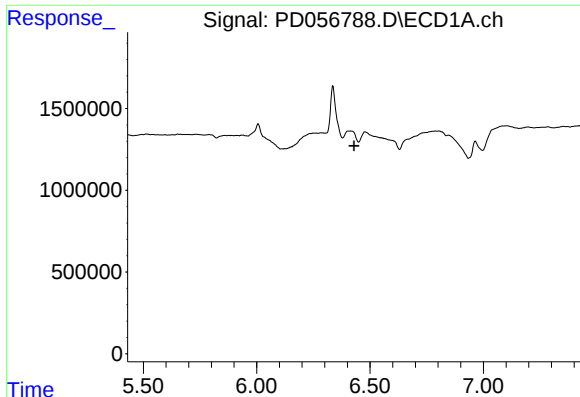

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

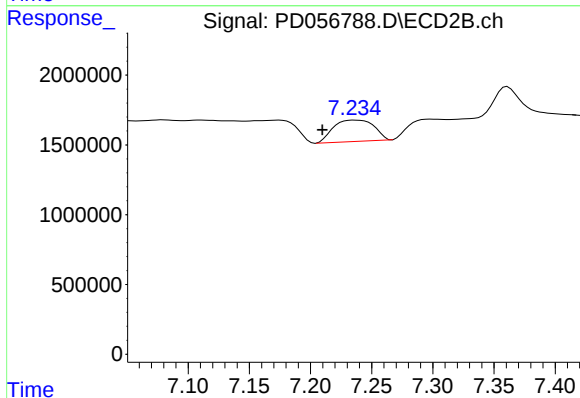


#19 Endosulfan Sulfate

R.T.: 7.236 min
Delta R.T.: 0.026 min
Response: 3533231
Conc: 2.64 ng/ml

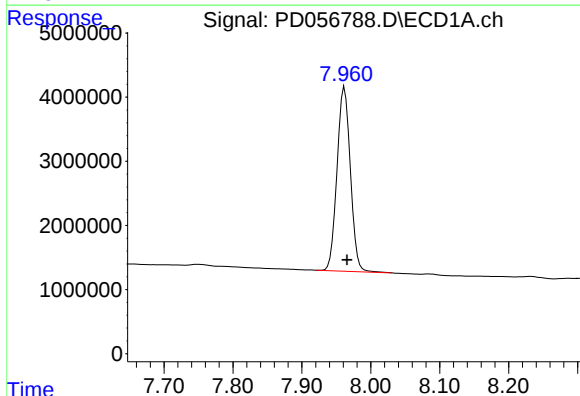

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.004 min
Response: 38662101
Conc: 42.82 ng/ml

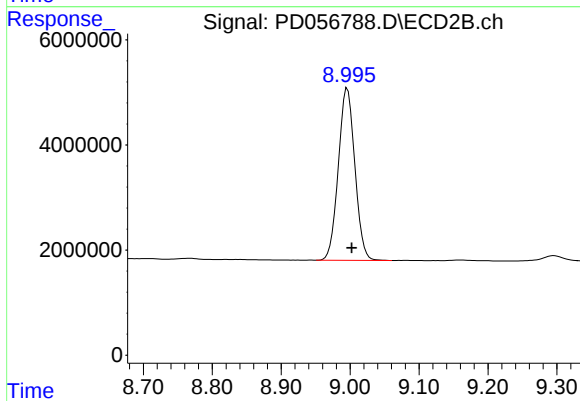

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.006 min
Response: 54614376
Conc: 45.39 ng/ml