

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
 Data File : PD056768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2019 09:45
 Operator : SG\AJ
 Sample : PB125564BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS64

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 03:19:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	17400342	30604766	21.010	25.456
27)	SA Decachlor...	7.956	8.995	32575768	45464284	36.076	37.788
Target Compounds							
3)	MA gamma-BHC...	3.987	4.629	55061527	94318197	49.033	58.444
8)	B Heptachlo...	4.948	5.822	54149381	93595922	52.942	60.413
10)	B trans-Chl...	5.170	6.055	55331974	94731626	52.780	57.294
12)	B 4,4'-DDE	5.395	6.284	110.8E6	181.8E6	109.680	115.790
13)	MA Dieldrin	5.518	6.433	113.7E6	192.7E6	111.914	122.649
14)	MA Endrin	5.772	6.650	89012820	142.9E6	106.514	112.921
19)	B Endosulfa...	6.424	7.203	59859289	100.3E6	68.914	74.978

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
Data File : PD056768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2019 09:45
Operator : SG\AJ
Sample : PB125564BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 03:19:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

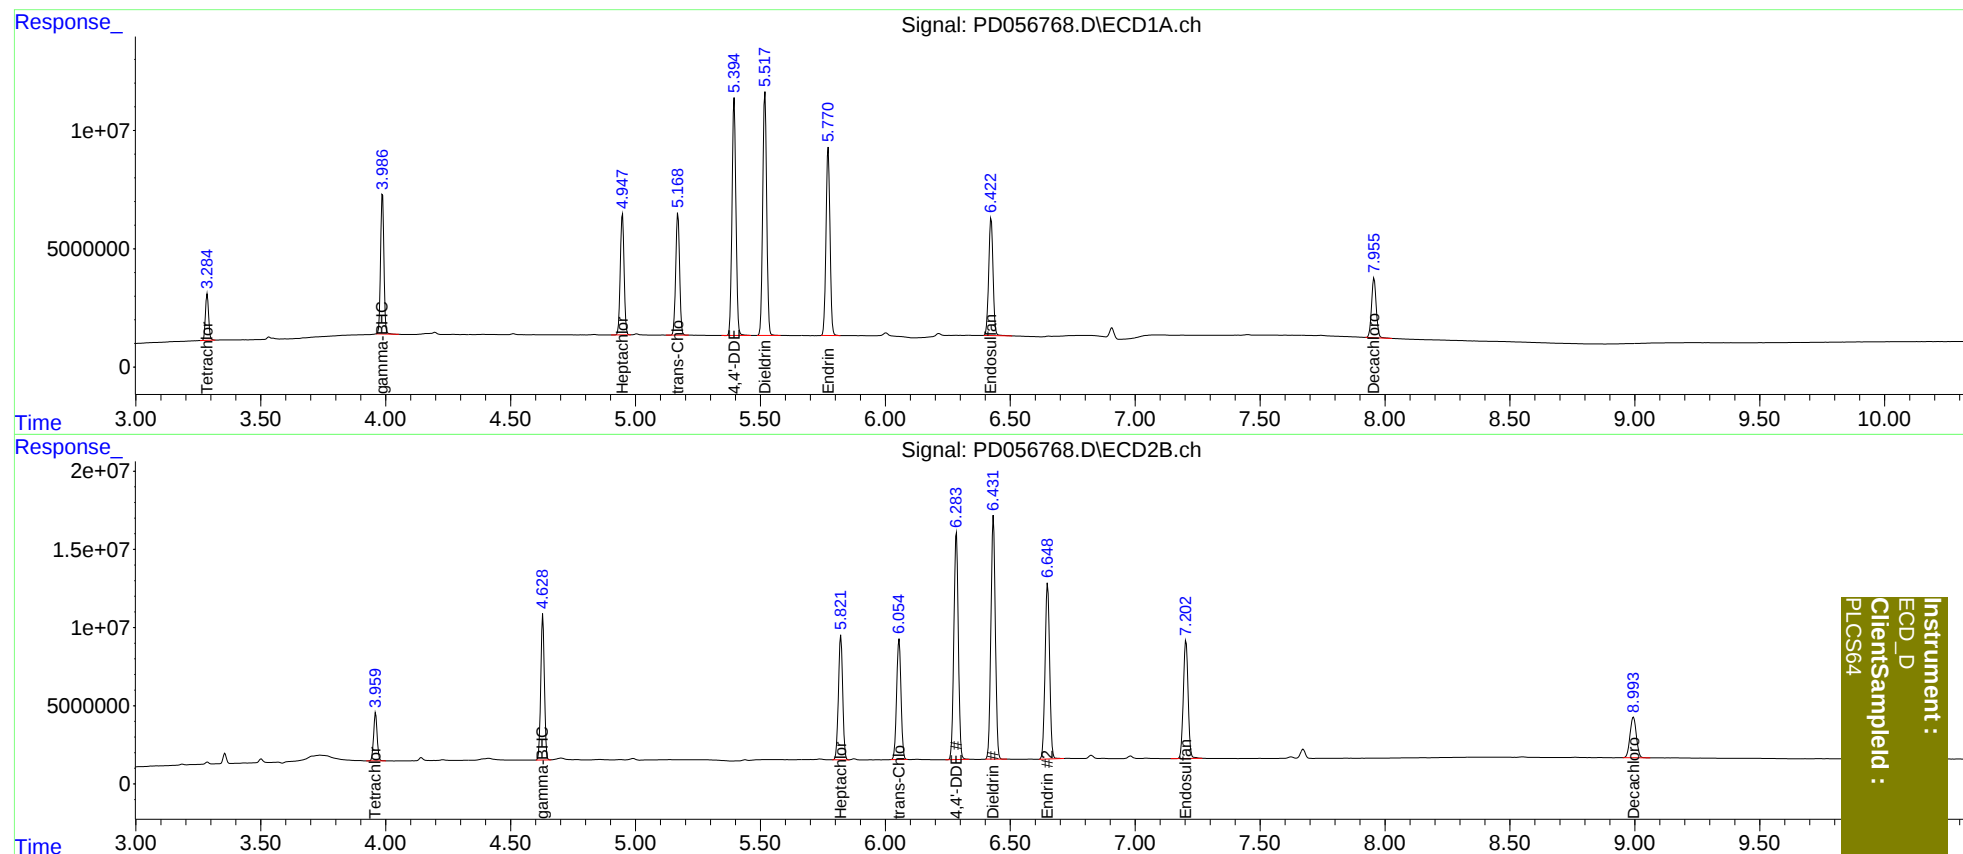

Instrument :
ECD_D
ClientSampled :
PLCS64