

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
 Data File : PD056781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2019 13:07
 Operator : SG\AJ
 Sample : K6254-18MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C05MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 03:24:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	15296120	29894489	18.469	24.865 #
27)	SA Decachlor...	7.956	8.995	28225614	40066638	31.259	33.302
Target Compounds							
3)	MA gamma-BHC...	3.987	4.629	54655217	93260739	48.672	57.788
4)	MA Heptachlor	4.272	5.135	53127816	91831995	52.710	56.346
5)	MB Aldrin	4.511	5.439	50857330	89291747	46.830	54.341
13)	MA Dieldrin	5.518	6.433	100.5E6	169.9E6	98.950	108.127
14)	MA Endrin	5.771	6.650	83936719	135.6E6	100.440	107.157
17)	MA 4,4'-DDT	6.140	7.070	70134707	119.5E6	99.674	101.095

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122619\
Data File : PD056781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2019 13:07
Operator : SG\AJ
Sample : K6254-18MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 03:24:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

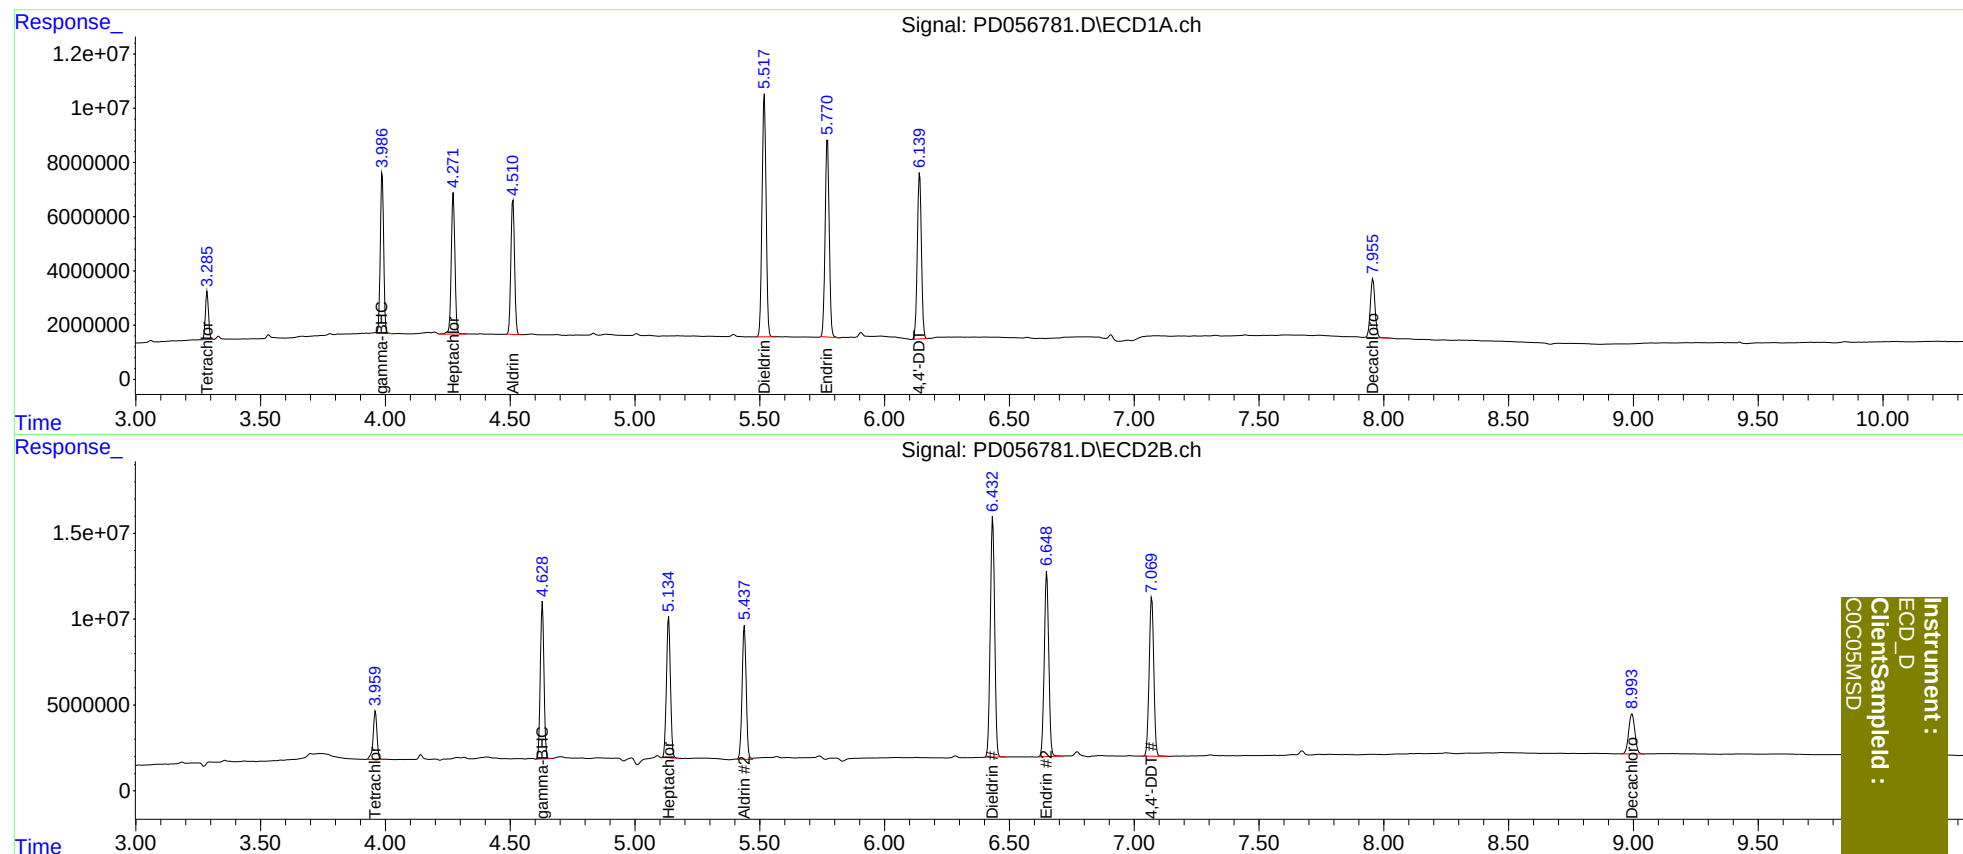

Instrument :
ECD_D
ClientSampled :
C0C05MSD