

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 15:18
 Operator : AR\AJ
 Sample : PB158058BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:19:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.797	26665171	45324700	17.692	18.030
28)	SA Decachlor...	9.114	7.939	33452471	49105356	16.526	17.420
Target Compounds							
2)	A alpha-BHC	4.010	3.290	48770	237556	0.019	0.062 #
3)	MA gamma-BHC...	0.000	3.647	0	197533	N.D.	0.054 #
7)	B delta-BHC	4.799	0.000	1536425	0	0.627	N.D. #
8)	B Heptachlo...	5.717	0.000	440641	0	0.200	N.D. #
13)	MA Dieldrin	6.393	0.000	200367	0	0.092	N.D. #
15)	B Endosulfa...	6.826	0.000	745938	0	0.392	N.D. #
18)	B Endrin al...	0.000	6.138	0	230294	N.D.	0.112 #
21)	B Endrin ke...	7.666f	0.000	14056	0	0.007	N.D. #
27)	Chlordane-5	6.910	0.000	152176	0	2.249	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 15:18
Operator : AR\AJ
Sample : PB158058BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:19:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

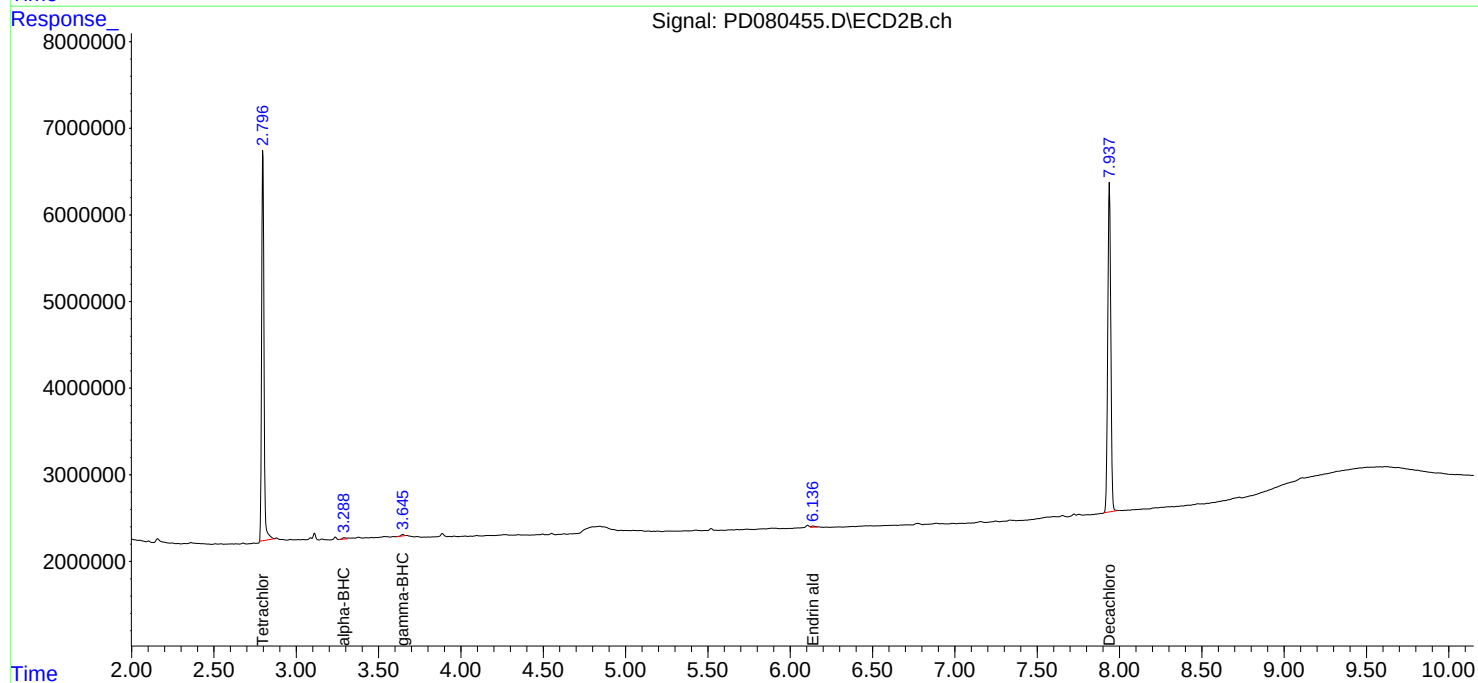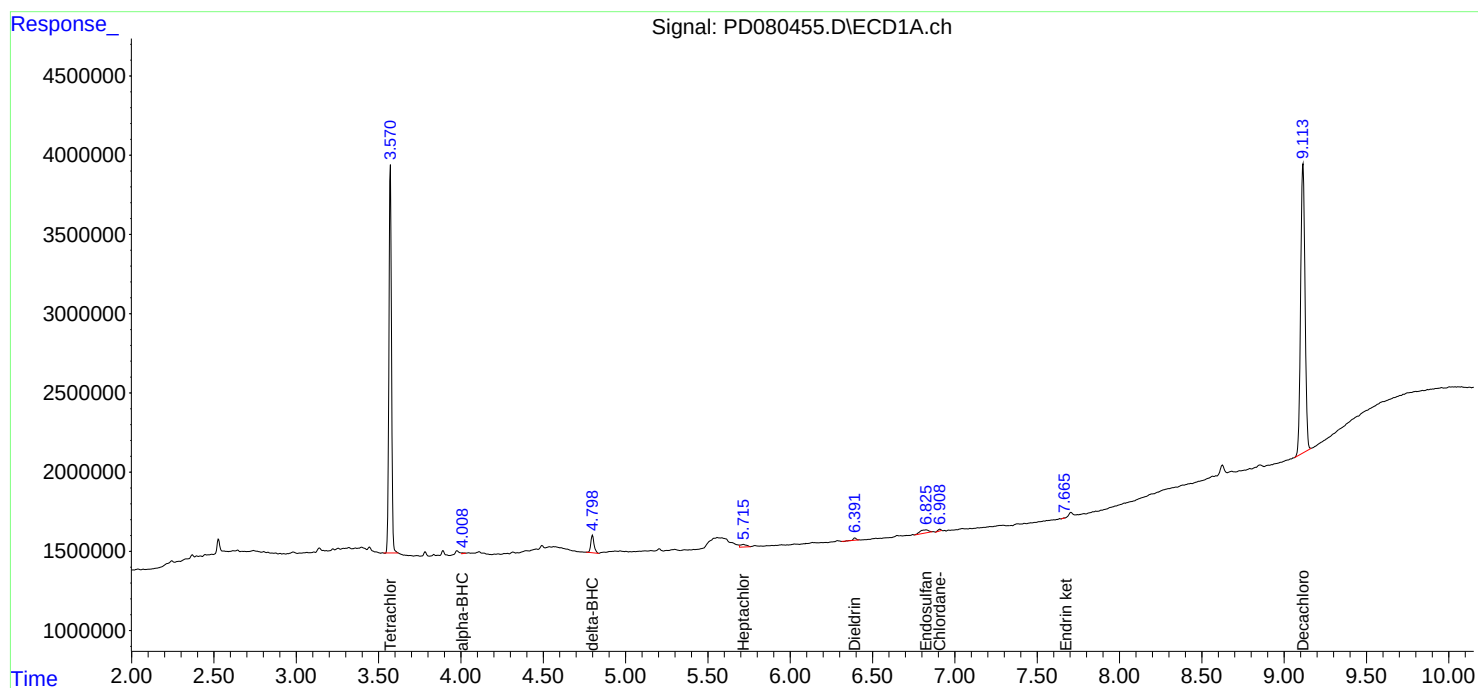

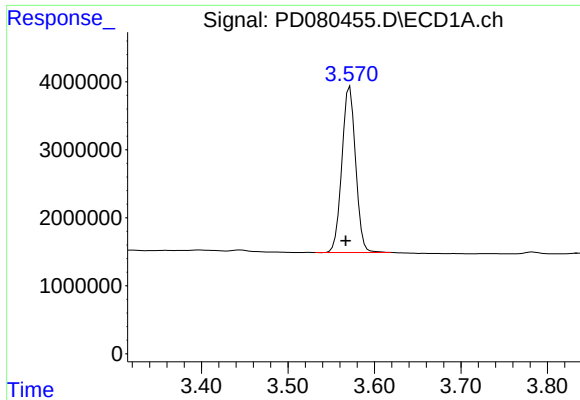


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: 0.005 min
Response: 26665171
Conc: 17.69 ng/ml

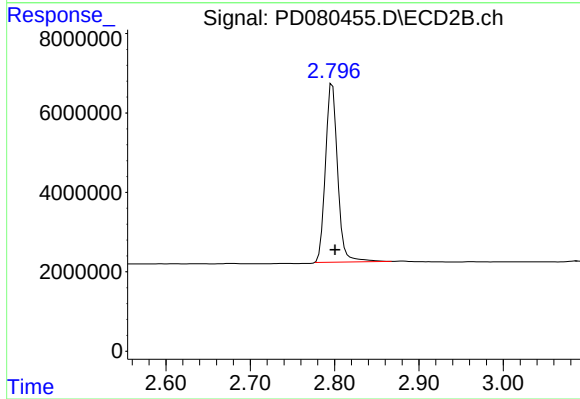


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: -0.003 min
Response: 45324700
Conc: 18.03 ng/ml

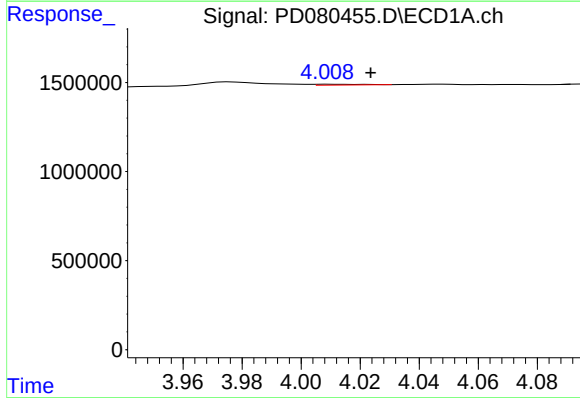


#2 alpha-BHC

R.T.: 4.010 min
Delta R.T.: -0.014 min
Response: 48770
Conc: 0.02 ng/ml

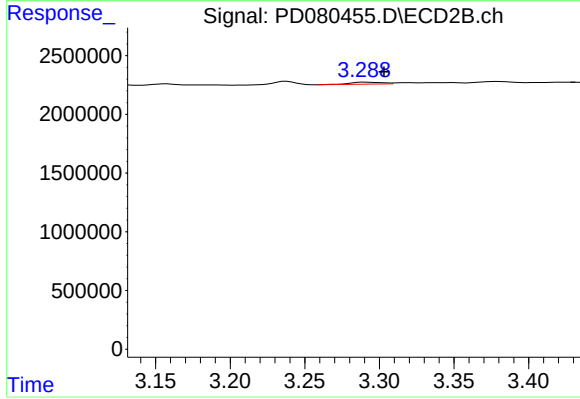


#2 alpha-BHC

R.T.: 3.290 min
Delta R.T.: -0.013 min
Response: 237556
Conc: 0.06 ng/ml

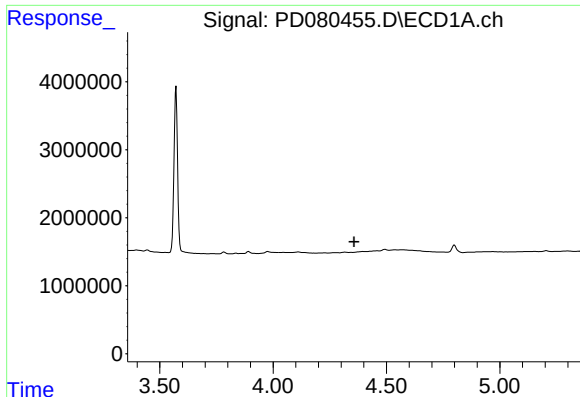


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

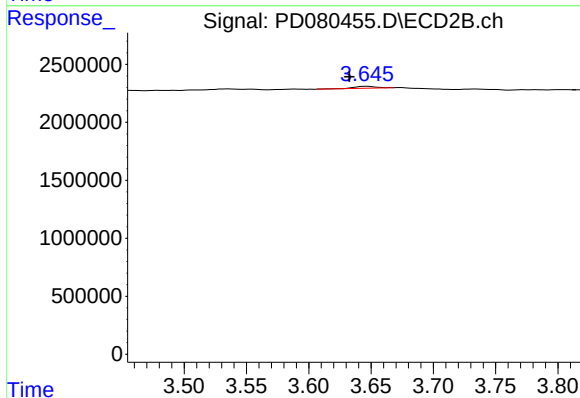


#3 gamma-BHC (Lindane)

R.T.: 3.647 min
Delta R.T.: 0.014 min
Response: 197533
Conc: 0.05 ng/ml

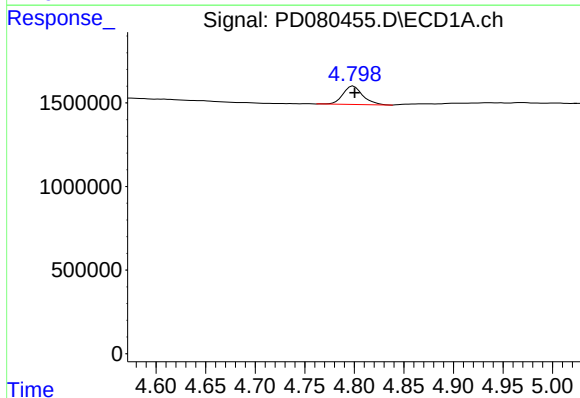


#7 delta-BHC

R.T.: 4.799 min
Delta R.T.: -0.001 min
Response: 1536425
Conc: 0.63 ng/ml

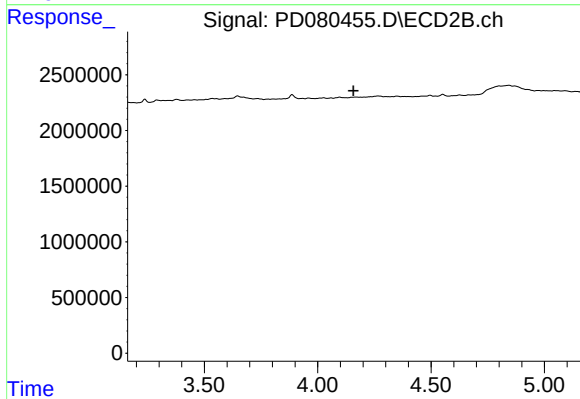


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.158 min
Response: 0
Conc: N.D.

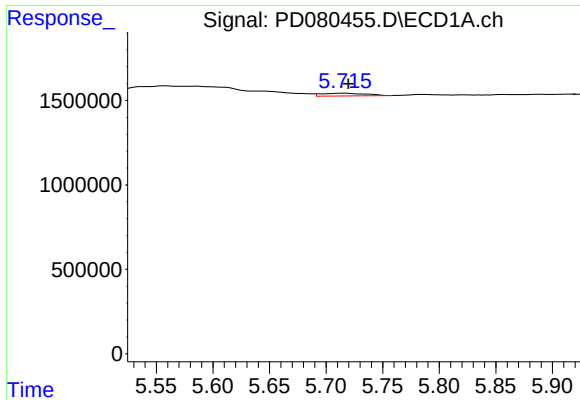


#8 Heptachlor epoxide

R.T.: 5.717 min
Delta R.T.: -0.003 min
Response: 440641
Conc: 0.20 ng/ml

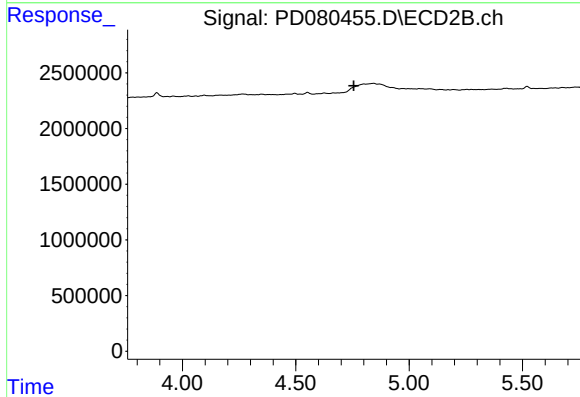


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

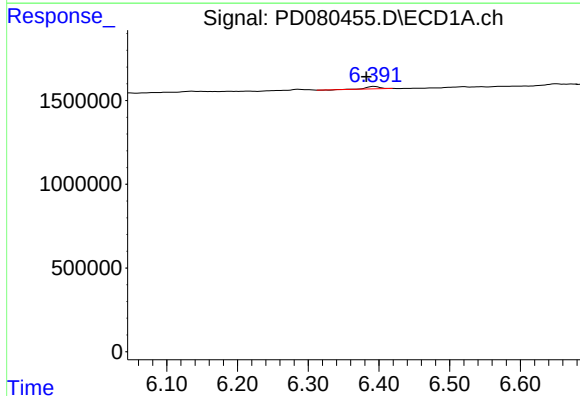


#13 Dieldrin

R.T.: 6.393 min
Delta R.T.: 0.010 min
Response: 200367
Conc: 0.09 ng/ml

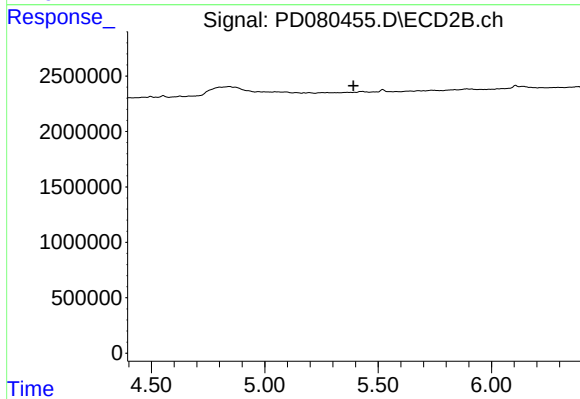


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.392 min
Response: 0
Conc: N.D.

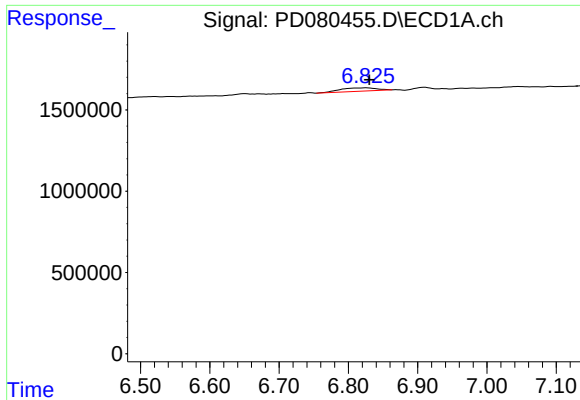


#15 Endosulfan II

R.T.: 6.826 min
Delta R.T.: -0.004 min
Response: 745938
Conc: 0.39 ng/ml

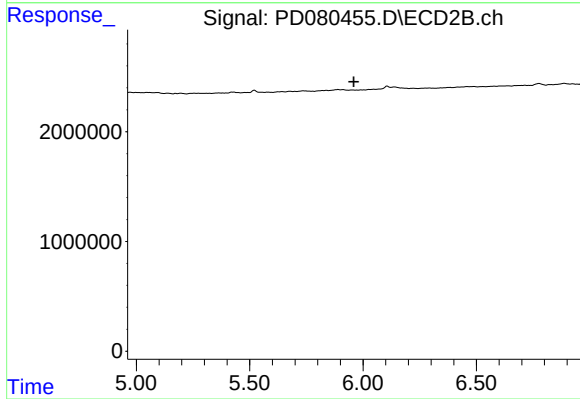


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

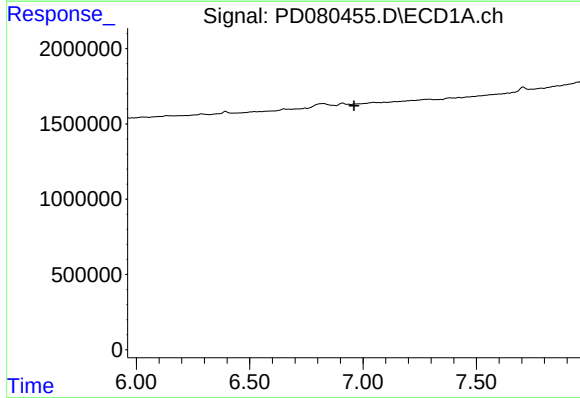


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.960 min
Response: 0
Conc: N.D.

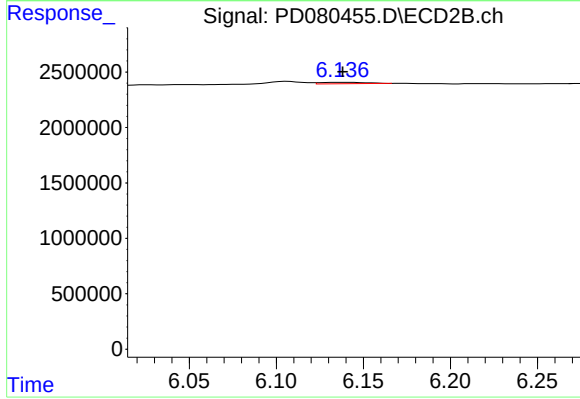


#18 Endrin aldehyde

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 230294
Conc: 0.11 ng/ml

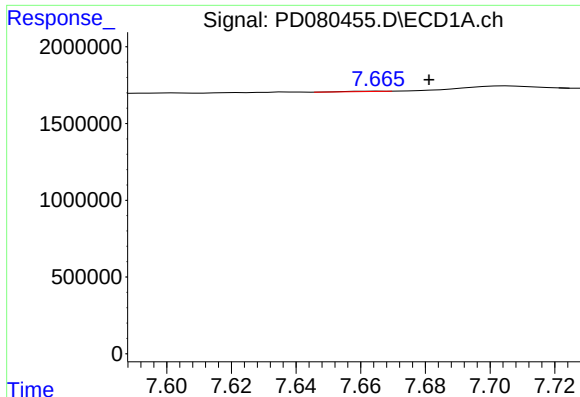


#21 Endrin ketone

R.T.: 7.666 min
Delta R.T.: -0.015 min
Response: 14056
Conc: 0.01 ng/ml

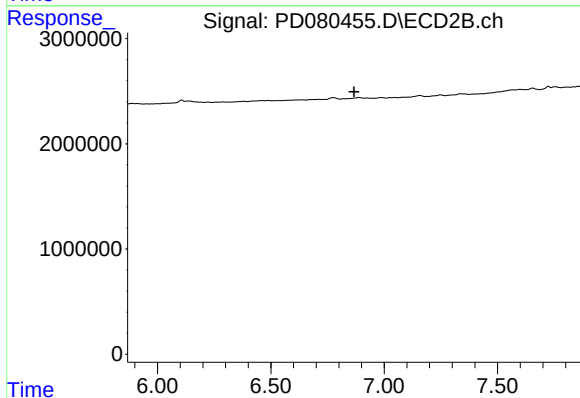


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.867 min
Response: 0
Conc: N.D.

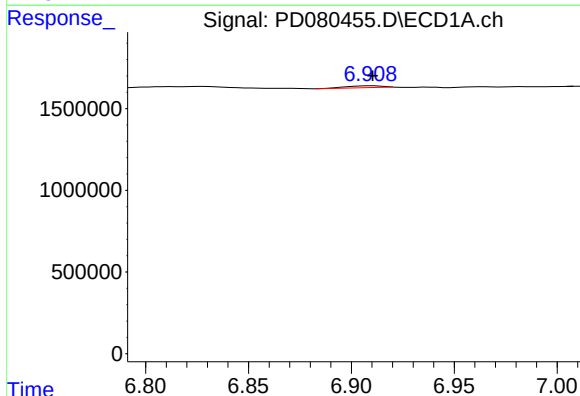


#27 Chlordane-5

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 152176
Conc: 2.25 ng/ml

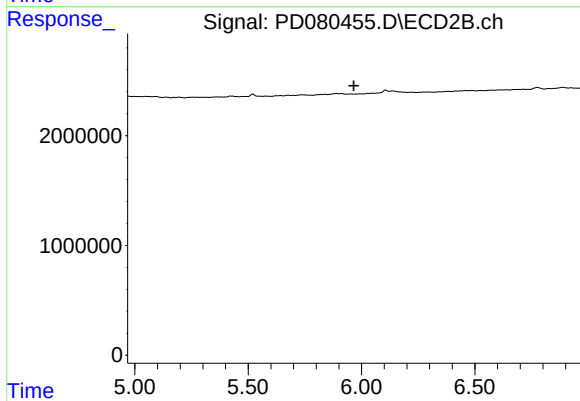


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.966 min
Response: 0
Conc: N.D.

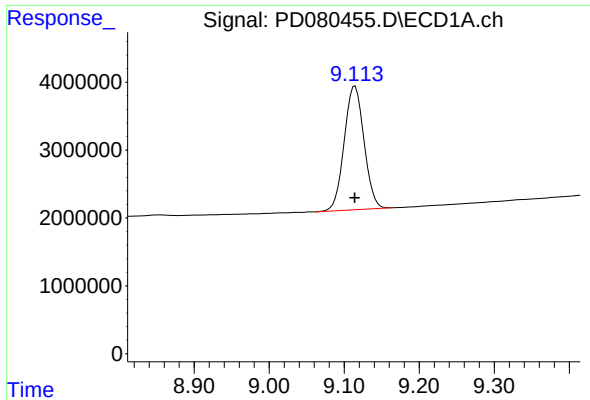

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 33452471
Conc: 16.53 ng/ml

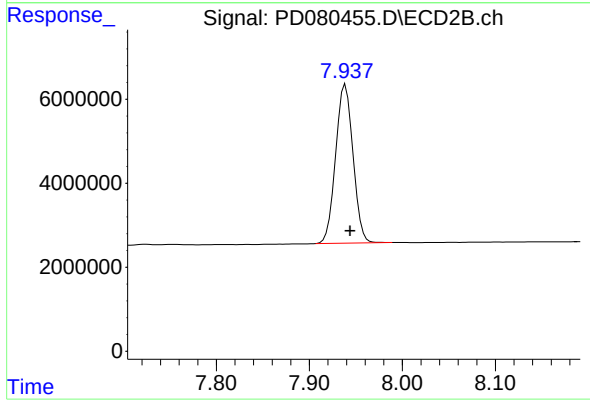

#28 Decachlorobiphenyl

R.T.: 7.939 min
Delta R.T.: -0.005 min
Response: 49105356
Conc: 17.42 ng/ml