

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 18:11
 Operator : AR\AJ
 Sample : 05926-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:23:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.799	26346585	44184527	17.480	17.577
28)	SA Decachlor...	9.109	7.938	32023946	45956609	15.821	16.303
Target Compounds							
6)	B beta-BHC	4.541	0.000	250172	0	0.250	N.D. #
7)	B delta-BHC	4.793	0.000	8455902	0	3.453	N.D. #
8)	B Heptachlo...	5.709	0.000	694911	0	0.315	N.D. #
10)	B gamma-Chl...	5.941f	0.000	434501	0	0.200	N.D. #
13)	MA Dieldrin	6.388	0.000	741829	0	0.340	N.D. #
15)	B Endosulfa...	6.815f	0.000	385537	0	0.202	N.D. #
21)	B Endrin ke...	7.705f	0.000	88404	0	0.043	N.D. #
22)	Mirex	8.152	0.000	21948	0	0.013	N.D. #
27)	Chlordane-5	6.904	0.000	437022	0	6.460	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 18:11
Operator : AR\AJ
Sample : 05926-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:23:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

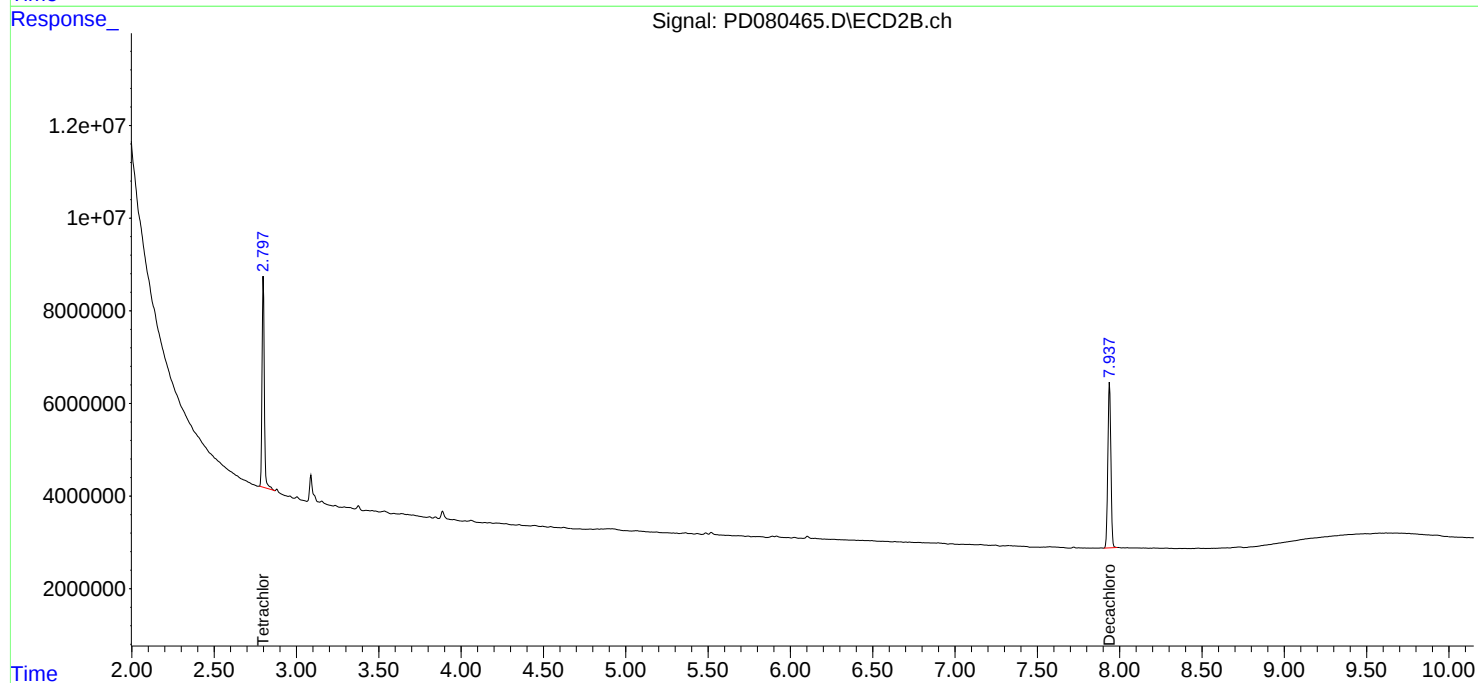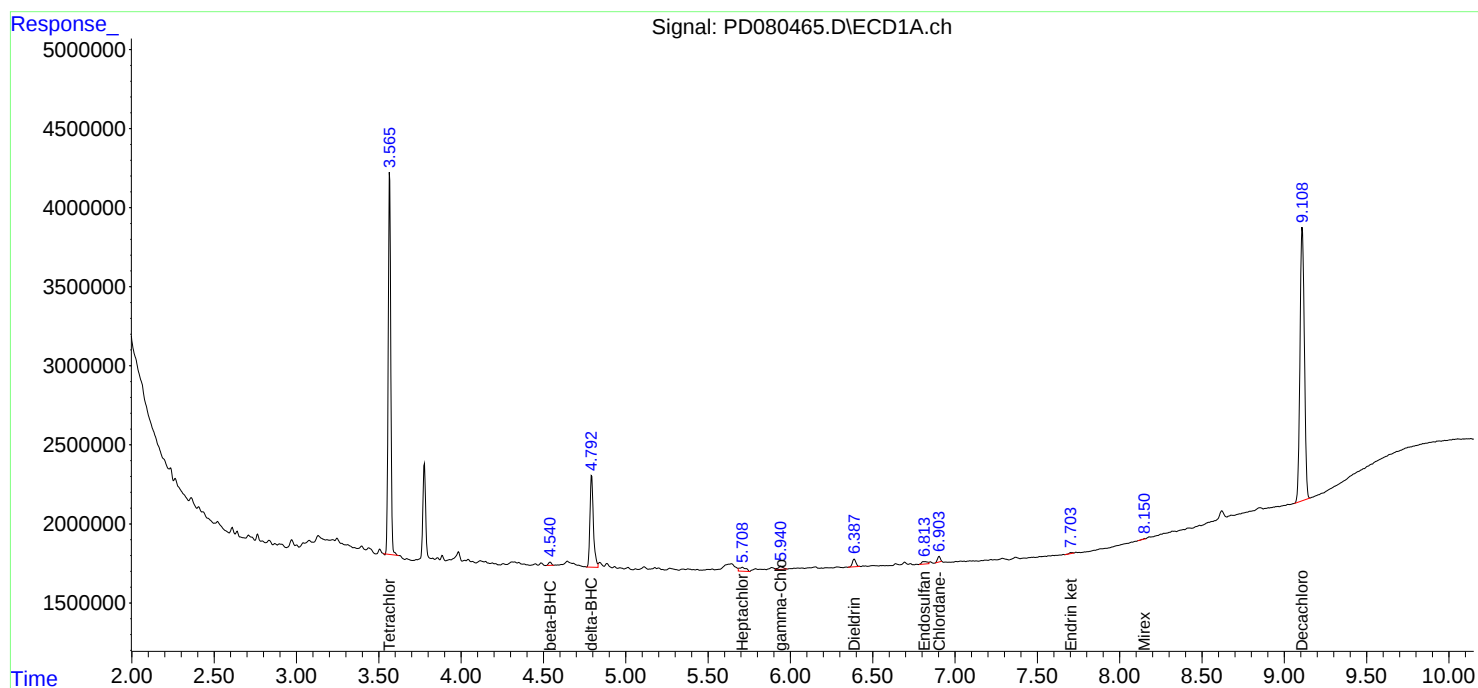

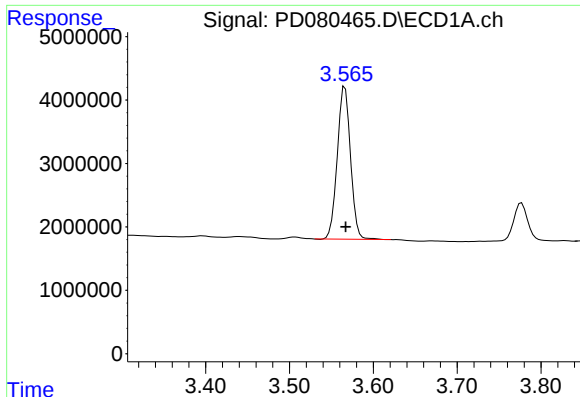


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 26346585
Conc: 17.48 ng/ml

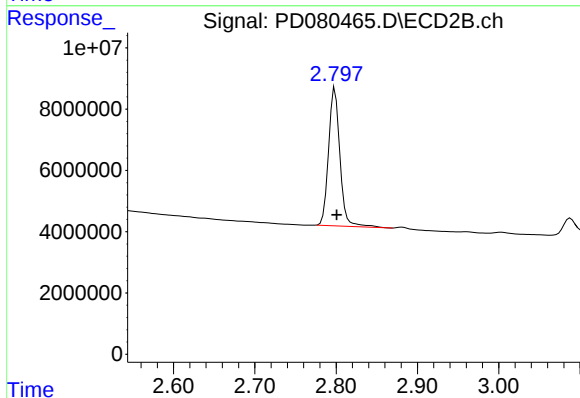


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: -0.002 min
Response: 44184527
Conc: 17.58 ng/ml

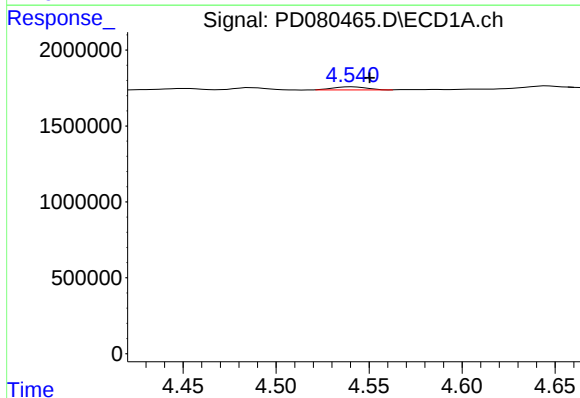


#6 beta-BHC

R.T.: 4.541 min
Delta R.T.: -0.010 min
Response: 250172
Conc: 0.25 ng/ml

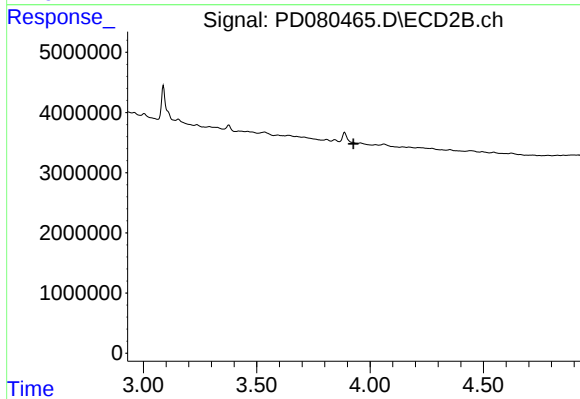


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 3.927 min
Response: 0
Conc: N.D.

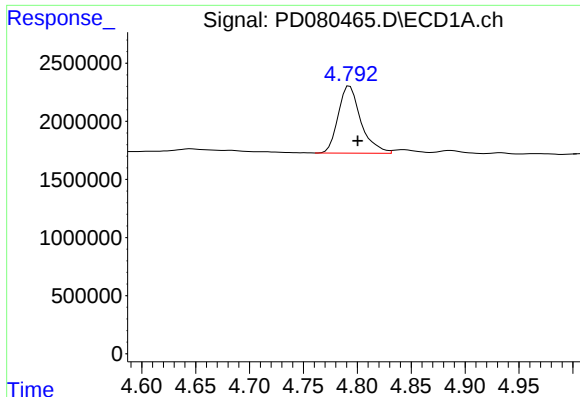


#7 delta-BHC

R.T.: 4.793 min
Delta R.T.: -0.007 min
Response: 8455902
Conc: 3.45 ng/ml

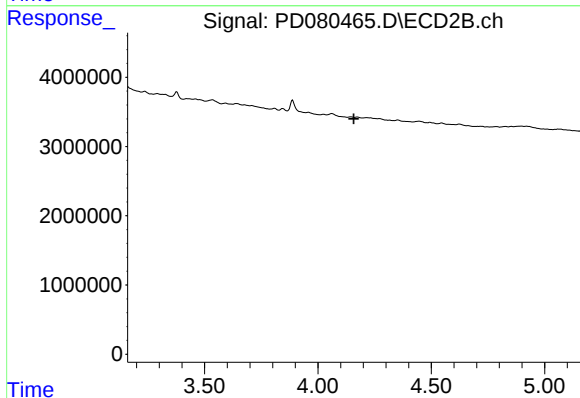


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.158 min
Response: 0
Conc: N.D.

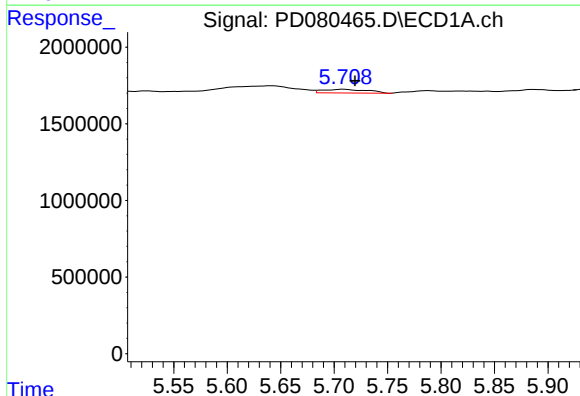


#8 Heptachlor epoxide

R.T.: 5.709 min
Delta R.T.: -0.010 min
Response: 694911
Conc: 0.32 ng/ml

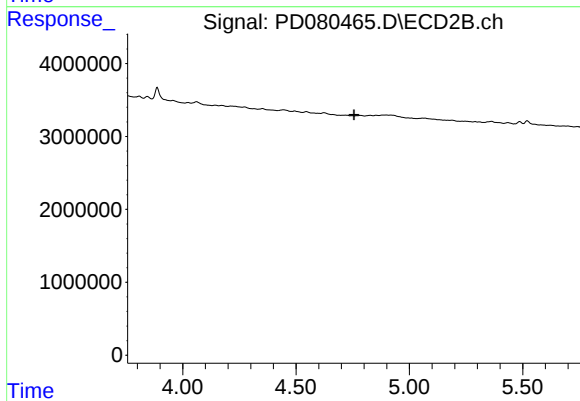


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.756 min
Response: 0
Conc: N.D.

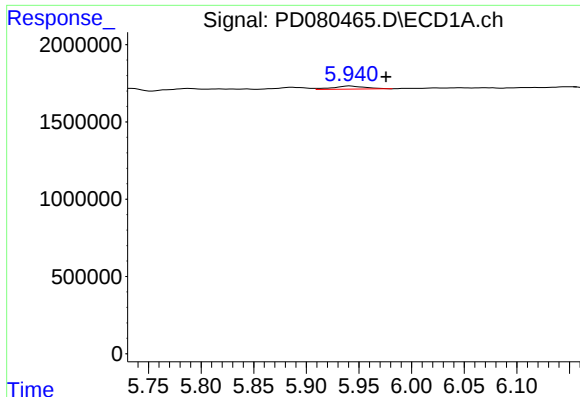


#10 gamma-Chlordane

R.T.: 5.941 min
Delta R.T.: -0.034 min
Response: 434501
Conc: 0.20 ng/ml

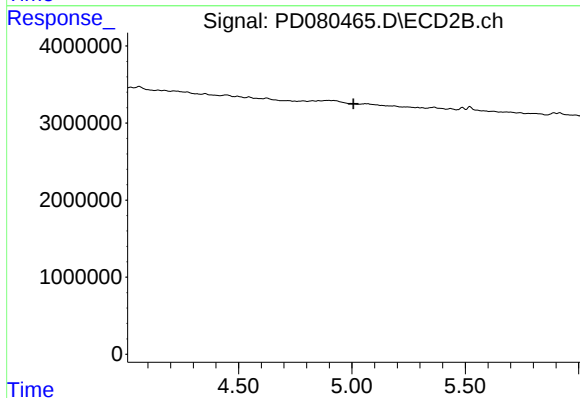


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.007 min
Response: 0
Conc: N.D.

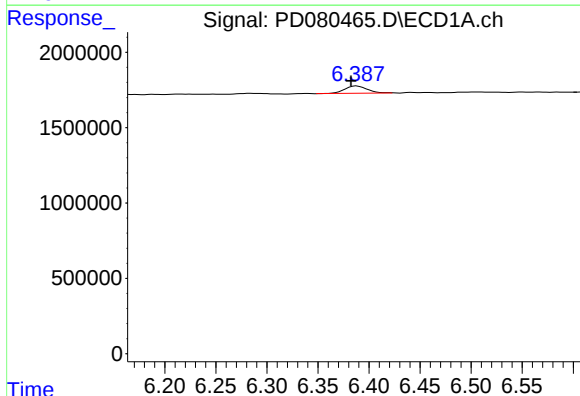


#13 Dieldrin

R.T.: 6.388 min
Delta R.T.: 0.006 min
Response: 741829
Conc: 0.34 ng/ml

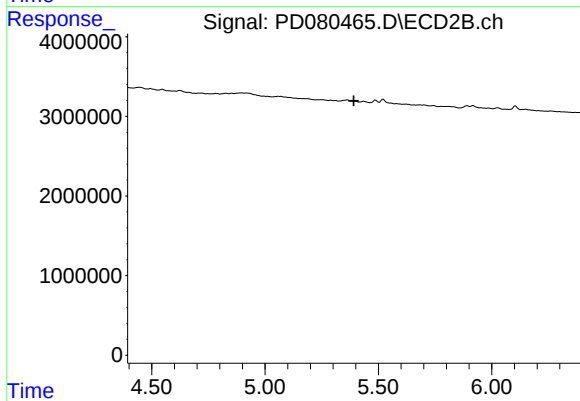


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.392 min
Response: 0
Conc: N.D.

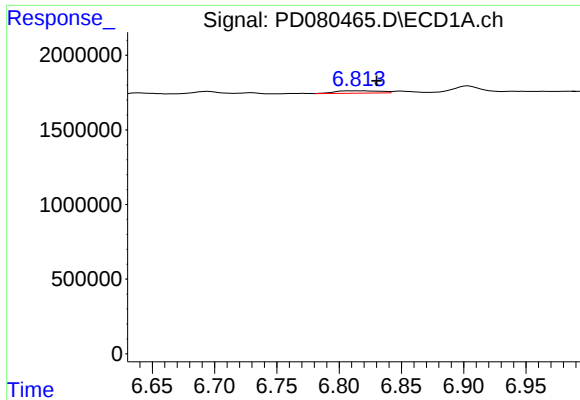


#15 Endosulfan II

R.T.: 6.815 min
Delta R.T.: -0.015 min
Response: 385537
Conc: 0.20 ng/ml

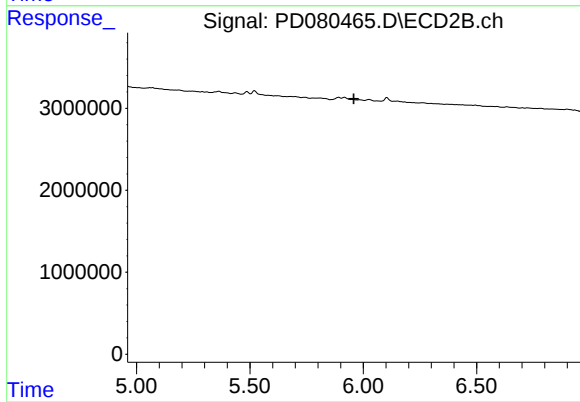


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

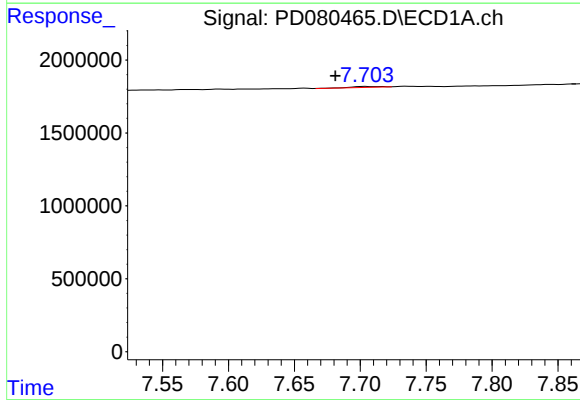


#21 Endrin ketone

R.T.: 7.705 min
Delta R.T.: 0.024 min
Response: 88404
Conc: 0.04 ng/ml

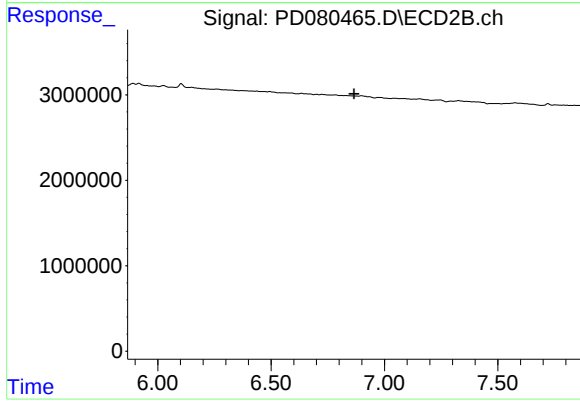


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.867 min
Response: 0
Conc: N.D.

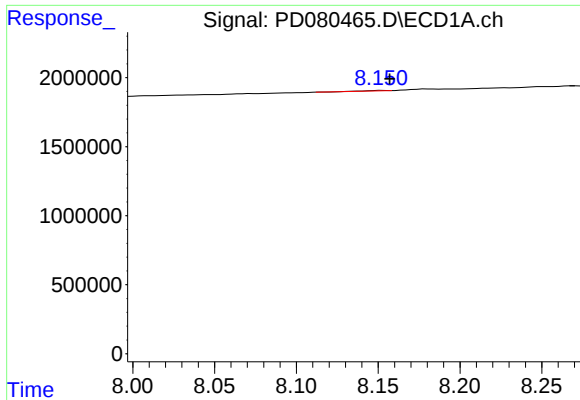


#22 Mirex

R.T.: 8.152 min
Delta R.T.: -0.006 min
Response: 21948
Conc: 0.01 ng/ml

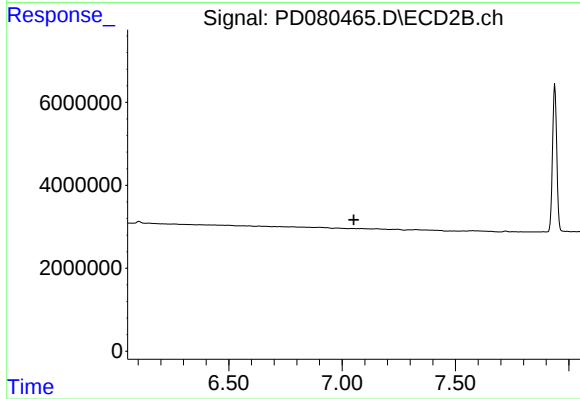


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.051 min
Response: 0
Conc: N.D.

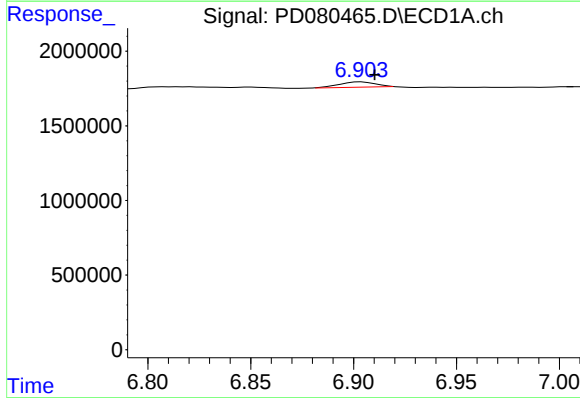


#27 Chlordane-5

R.T.: 6.904 min
Delta R.T.: -0.007 min
Response: 437022
Conc: 6.46 ng/ml

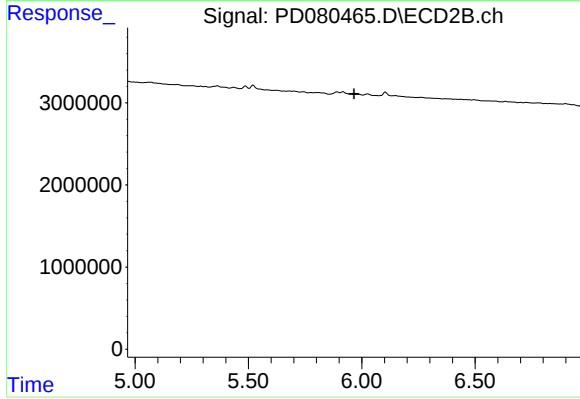


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.966 min
Response: 0
Conc: N.D.

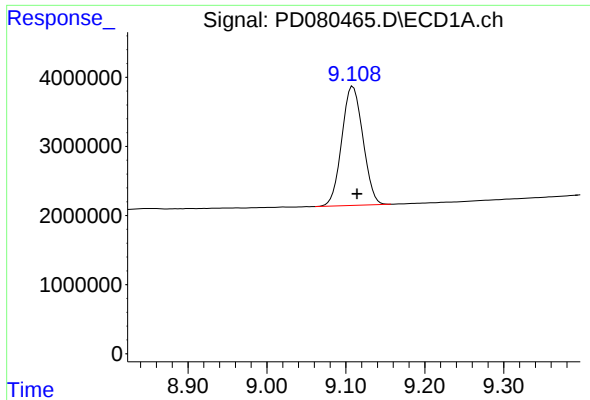

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.005 min
Response: 32023946
Conc: 15.82 ng/ml

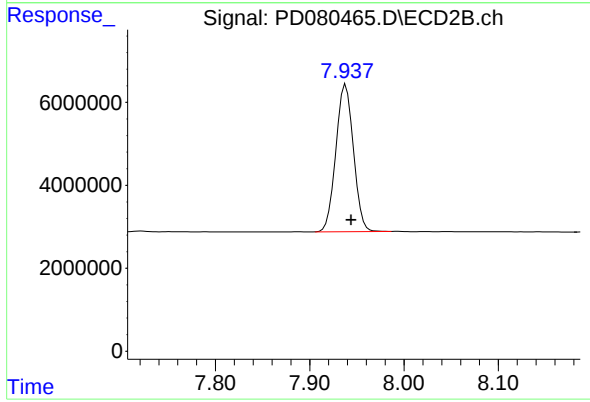

#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.005 min
Response: 45956609
Conc: 16.30 ng/ml