

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 18:38
 Operator : AR\AJ
 Sample : 05980-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:24:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.799	28669503	49091952	19.022	19.529
28)	SA Decachlor...	9.109	7.938	25499702	38393878	12.597	13.620
Target Compounds							
4)	MA Heptachlor	4.968f	0.000	118416	0	0.048	N.D. #
6)	B beta-BHC	4.542	0.000	248647	0	0.248	N.D. #
7)	B delta-BHC	4.793	0.000	3476133	0	1.419	N.D. #
8)	B Heptachlo...	5.710	0.000	438669	0	0.199	N.D. #
12)	B 4,4'-DDE	6.214	0.000	453529	0	0.226	N.D. #
13)	MA Dieldrin	6.388	0.000	787297	0	0.361	N.D. #
14)	MA Endrin	6.641f	0.000	154183	0	0.085	N.D. #
15)	B Endosulfa...	6.828	0.000	270625	0	0.142	N.D. #
19)	B Endosulfa...	7.224f	6.332f	-381052	3242995	N.D.	1.210
20)	A Methoxychlor	0.000	6.627	0	148420	N.D.	0.101 #
21)	B Endrin ke...	7.711f	0.000	59902	0	0.029	N.D. #
27)	Chlordane-5	6.904	0.000	487412	0	7.205	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 18:38
Operator : AR\AJ
Sample : 05980-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:24:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

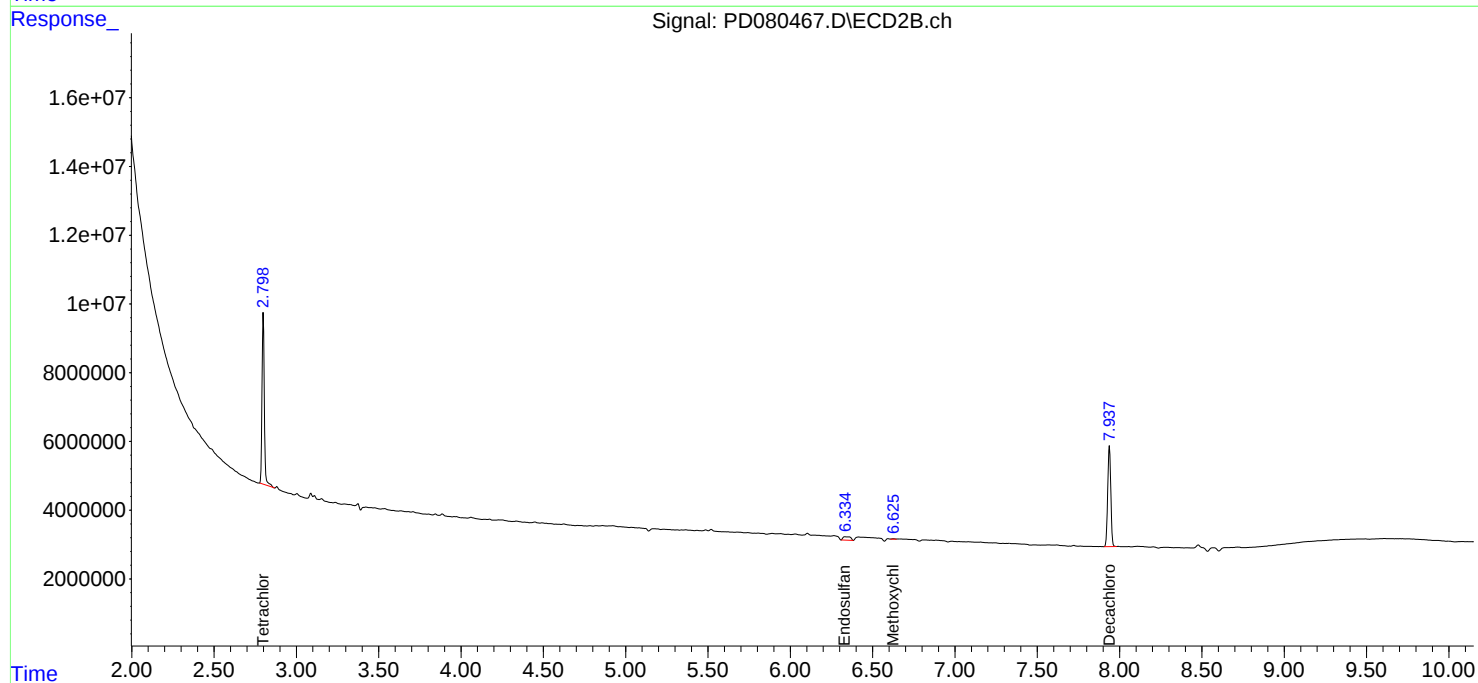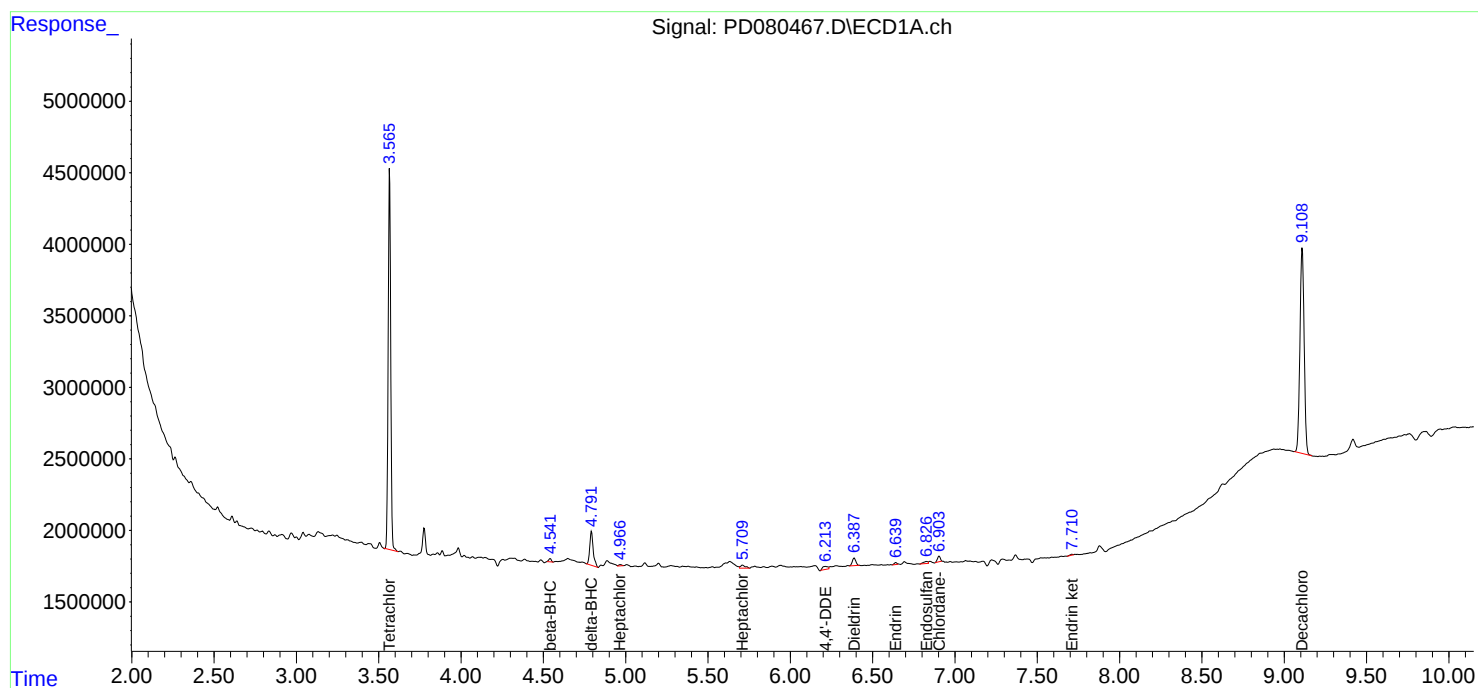

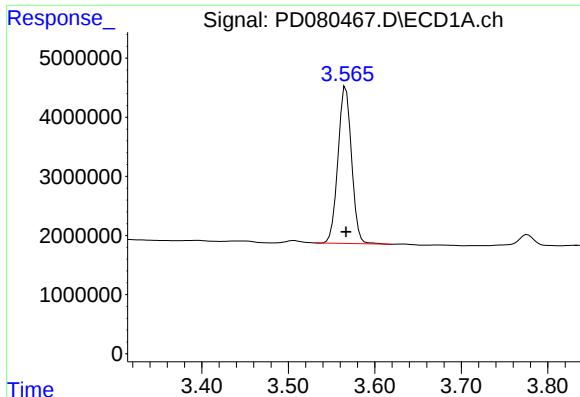


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 28669503
Conc: 19.02 ng/ml

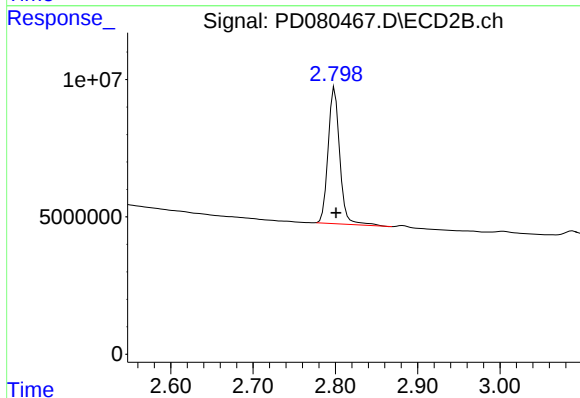


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: -0.001 min
Response: 49091952
Conc: 19.53 ng/ml

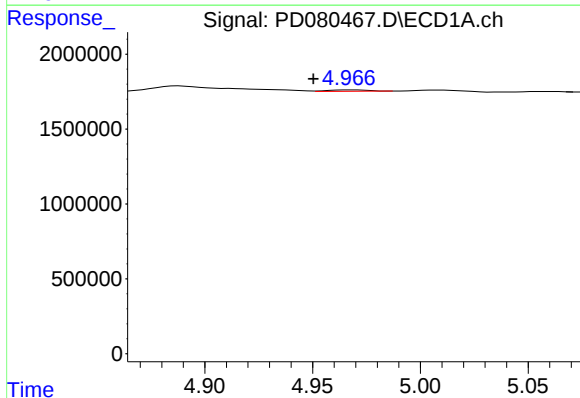


#4 Heptachlor

R.T.: 4.968 min
Delta R.T.: 0.018 min
Response: 118416
Conc: 0.05 ng/ml

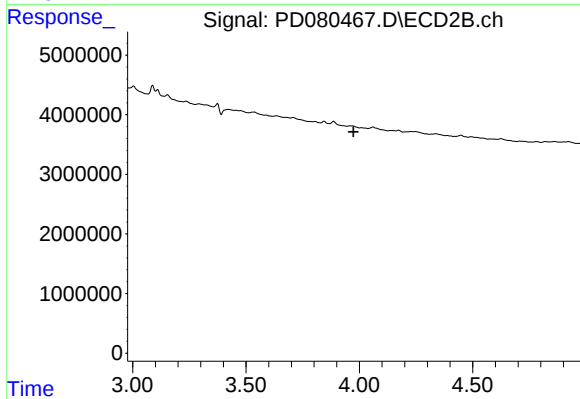


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.975 min
Response: 0
Conc: N.D.

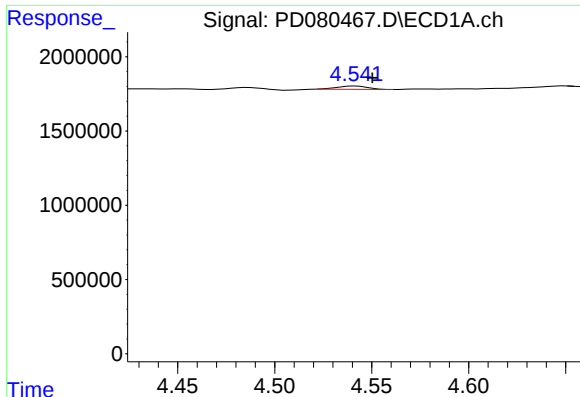


#6 beta-BHC

R.T.: 4.542 min
Delta R.T.: -0.008 min
Response: 248647
Conc: 0.25 ng/ml

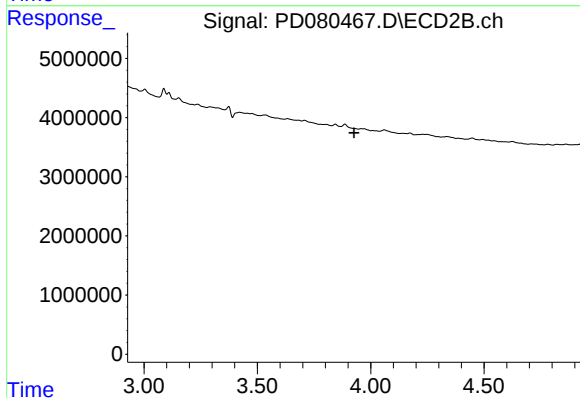


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.927 min
Response: 0
Conc: N.D.

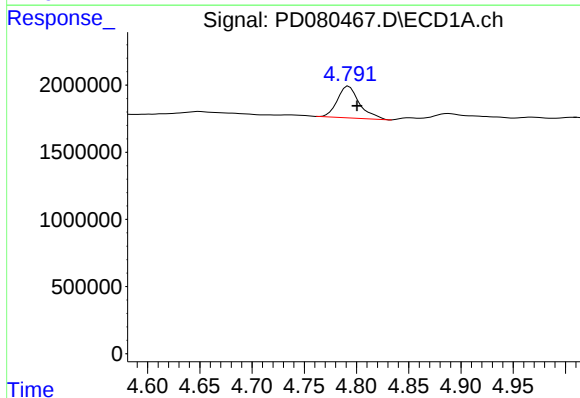


#7 delta-BHC

R.T.: 4.793 min
Delta R.T.: -0.008 min
Response: 3476133
Conc: 1.42 ng/ml

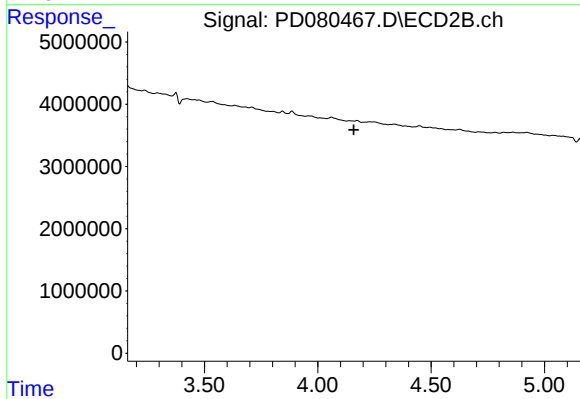


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.158 min
Response: 0
Conc: N.D.

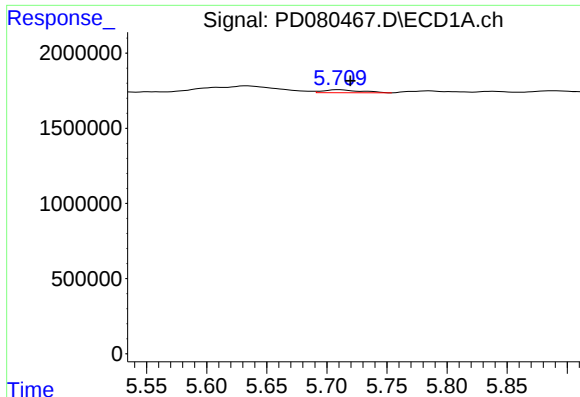


#8 Heptachlor epoxide

R.T.: 5.710 min
Delta R.T.: -0.010 min
Response: 438669
Conc: 0.20 ng/ml

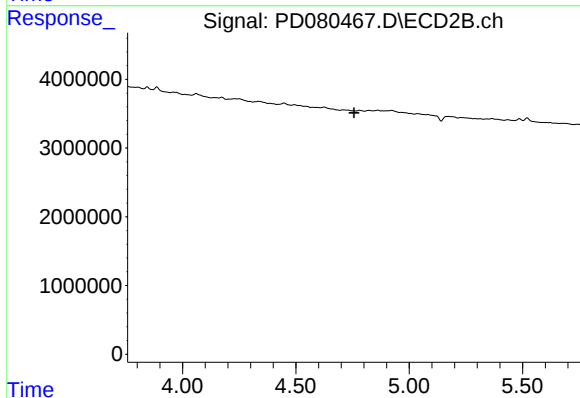


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

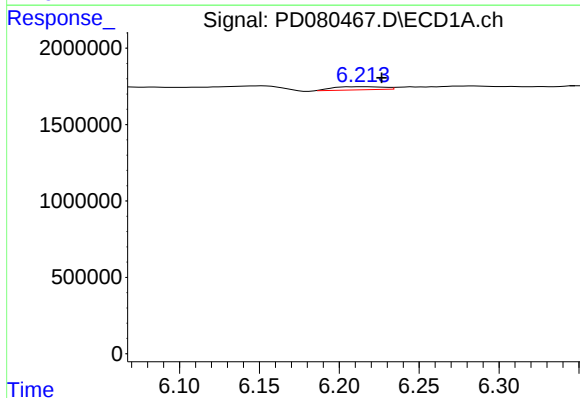


#12 4,4'-DDE

R.T.: 6.214 min
Delta R.T.: -0.012 min
Response: 453529
Conc: 0.23 ng/ml

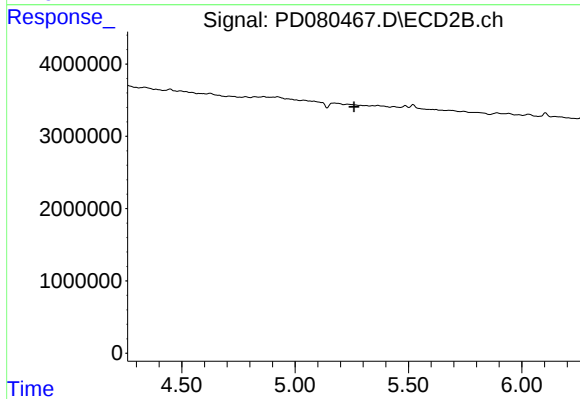


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.260 min
Response: 0
Conc: N.D.

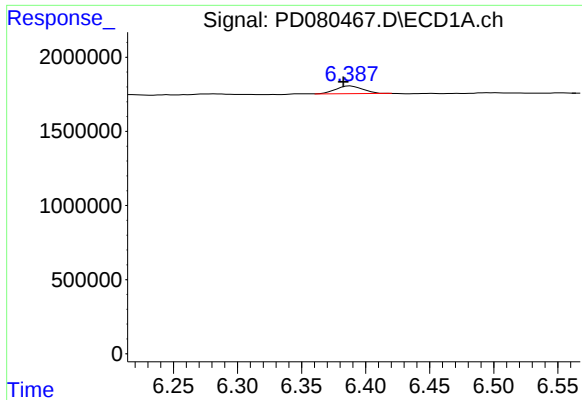


#13 Dieldrin

R.T.: 6.388 min
Delta R.T.: 0.006 min
Response: 787297
Conc: 0.36 ng/ml

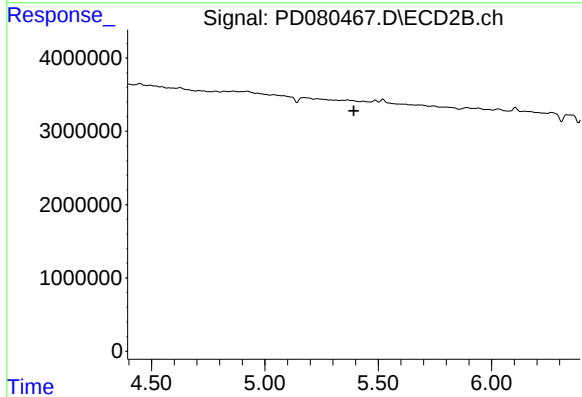


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.392 min
Response: 0
Conc: N.D.

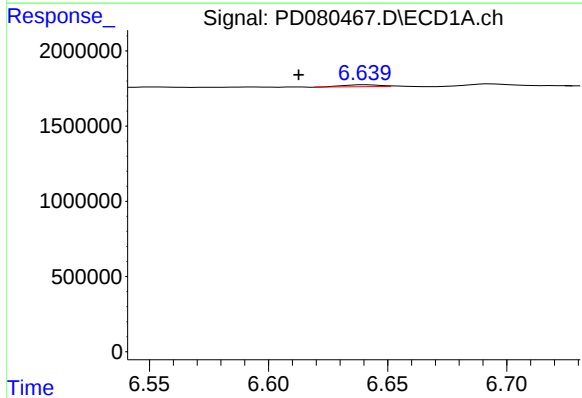


#14 Endrin

R.T.: 6.641 min
Delta R.T.: 0.028 min
Response: 154183
Conc: 0.09 ng/ml

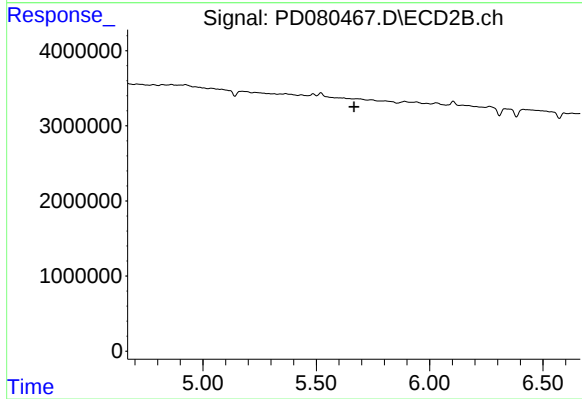


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.666 min
Response: 0
Conc: N.D.

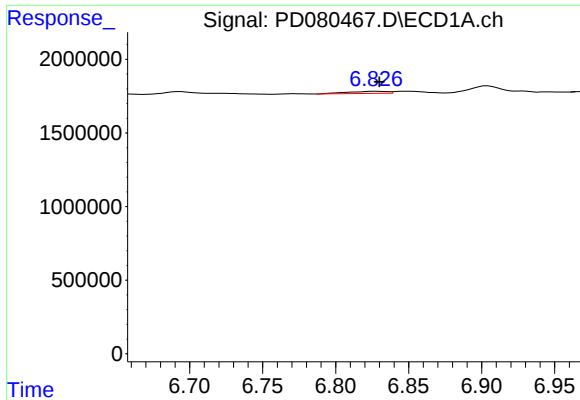


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: -0.003 min
Response: 270625
Conc: 0.14 ng/ml

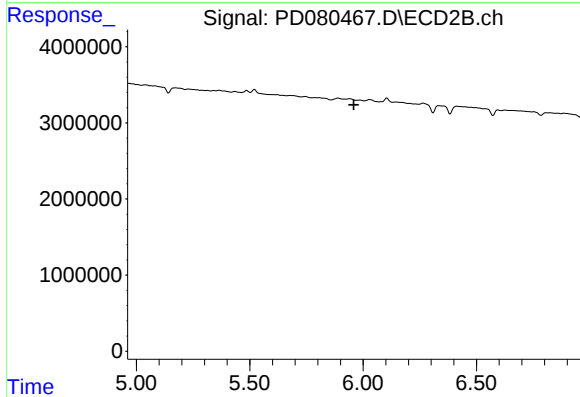


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.959 min
Response: 0
Conc: N.D.

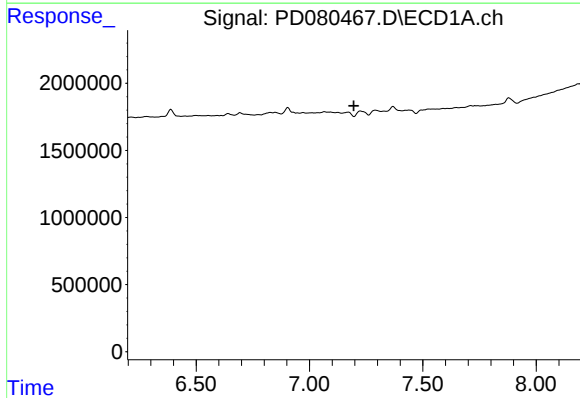


#19 Endosulfan Sulfate

R.T.: 7.224 min
Delta R.T.: 0.029 min
Response: -381052
Conc: N.D.

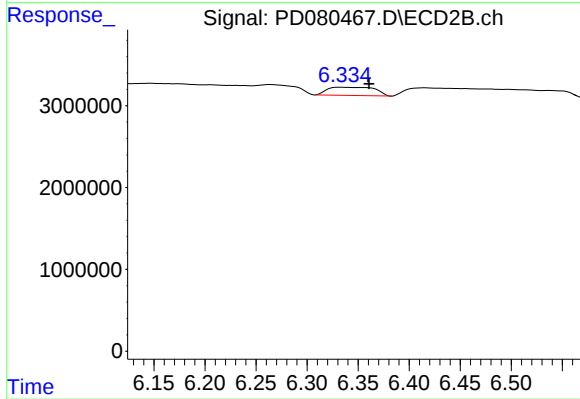


#19 Endosulfan Sulfate

R.T.: 6.332 min
Delta R.T.: -0.028 min
Response: 3242995
Conc: 1.21 ng/ml

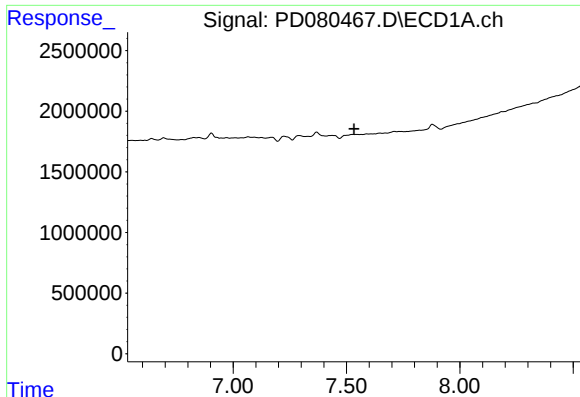


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.533 min
Response: 0
Conc: N.D.

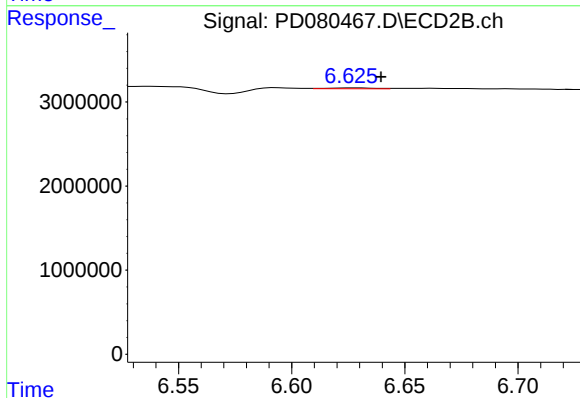


#20 Methoxychlor

R.T.: 6.627 min
Delta R.T.: -0.013 min
Response: 148420
Conc: 0.10 ng/ml

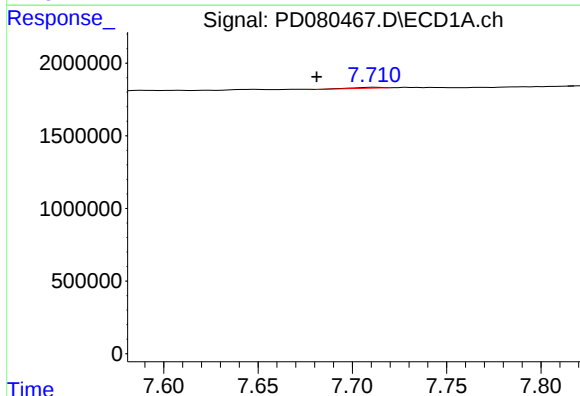


#21 Endrin ketone

R.T.: 7.711 min
Delta R.T.: 0.030 min
Response: 59902
Conc: 0.03 ng/ml

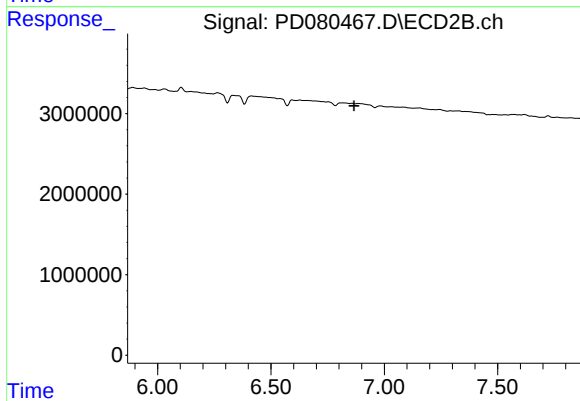


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.867 min
Response: 0
Conc: N.D.

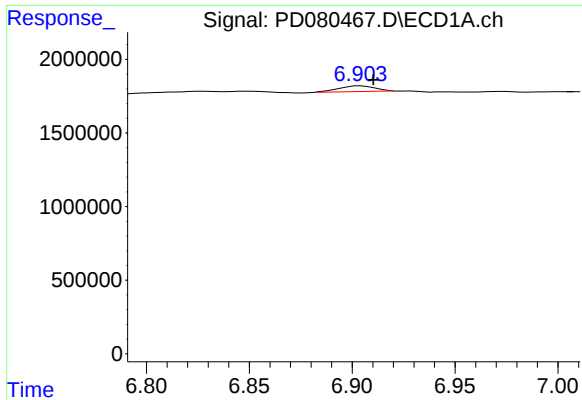


#27 Chlordane-5

R.T.: 6.904 min
Delta R.T.: -0.006 min
Response: 487412
Conc: 7.20 ng/ml

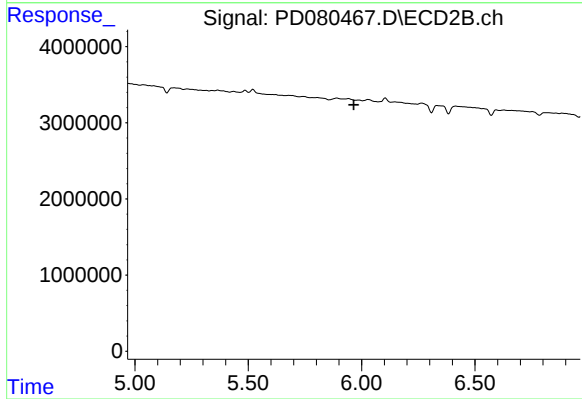


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.966 min
Response: 0
Conc: N.D.

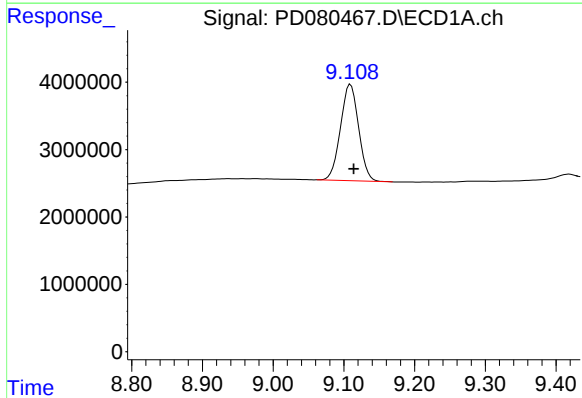

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.005 min
Response: 25499702
Conc: 12.60 ng/ml

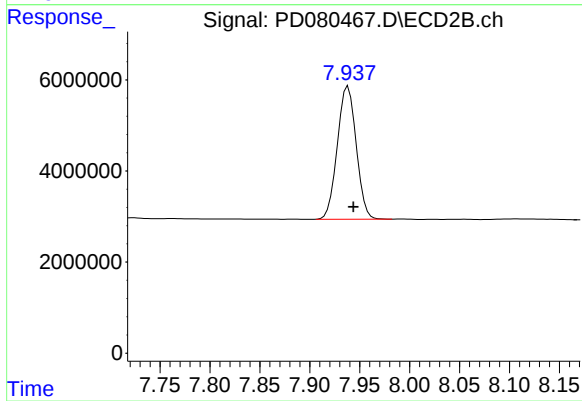

#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.005 min
Response: 38393878
Conc: 13.62 ng/ml