

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 19:18
 Operator : AR\AJ
 Sample : PB1578982TB
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:25:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.798	25169166	44448441	16.699	17.682
28)	SA Decachlor...	9.110	7.938	30793438	47046030	15.213	16.689
Target Compounds							
2)	A alpha-BHC	0.000	3.289	0	166869	N.D.	0.044 #
4)	MA Heptachlor	4.938	0.000	212197	0	0.086	N.D. #
7)	B delta-BHC	4.793	0.000	1011206	0	0.413	N.D. #
8)	B Heptachlo...	5.712	0.000	165242	0	0.075	N.D. #
27)	Chlordane-5	6.900	0.000	314544	0	4.650	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 19:18
Operator : AR\AJ
Sample : PB1578982TB
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:25:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

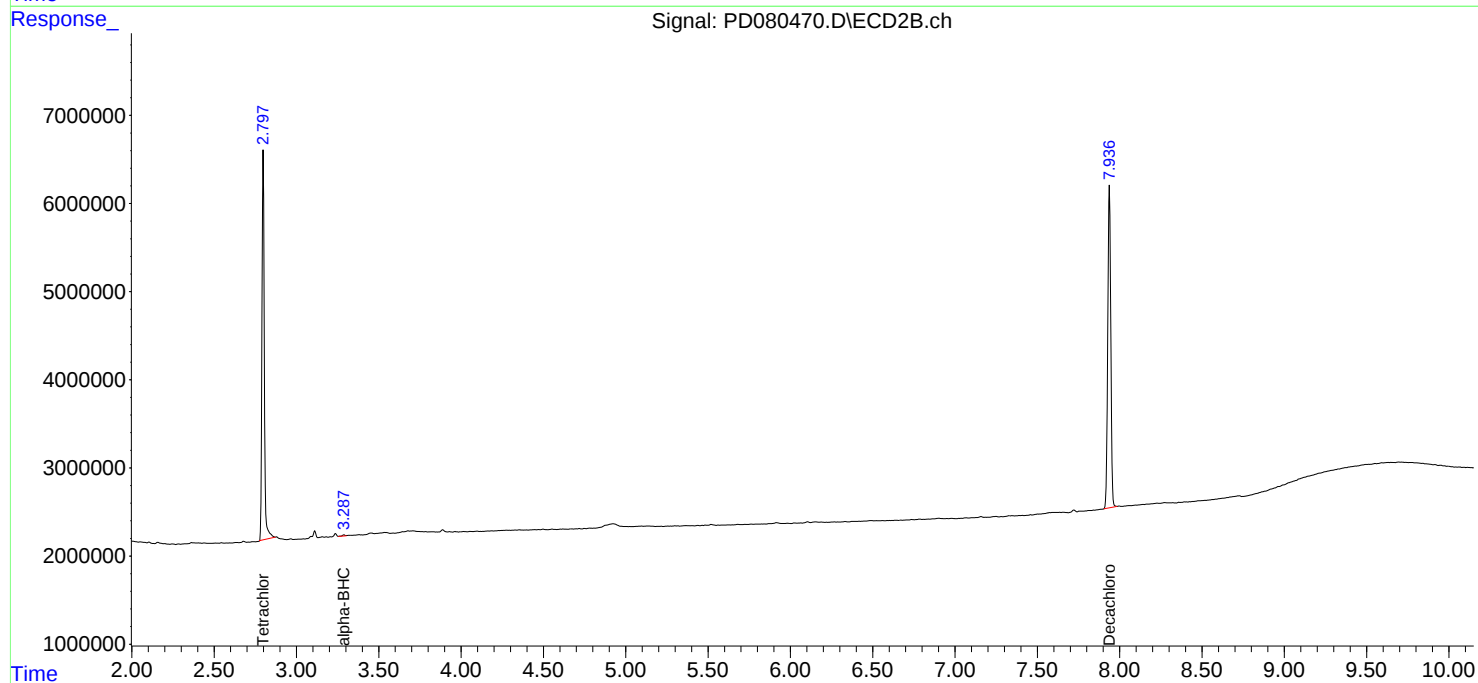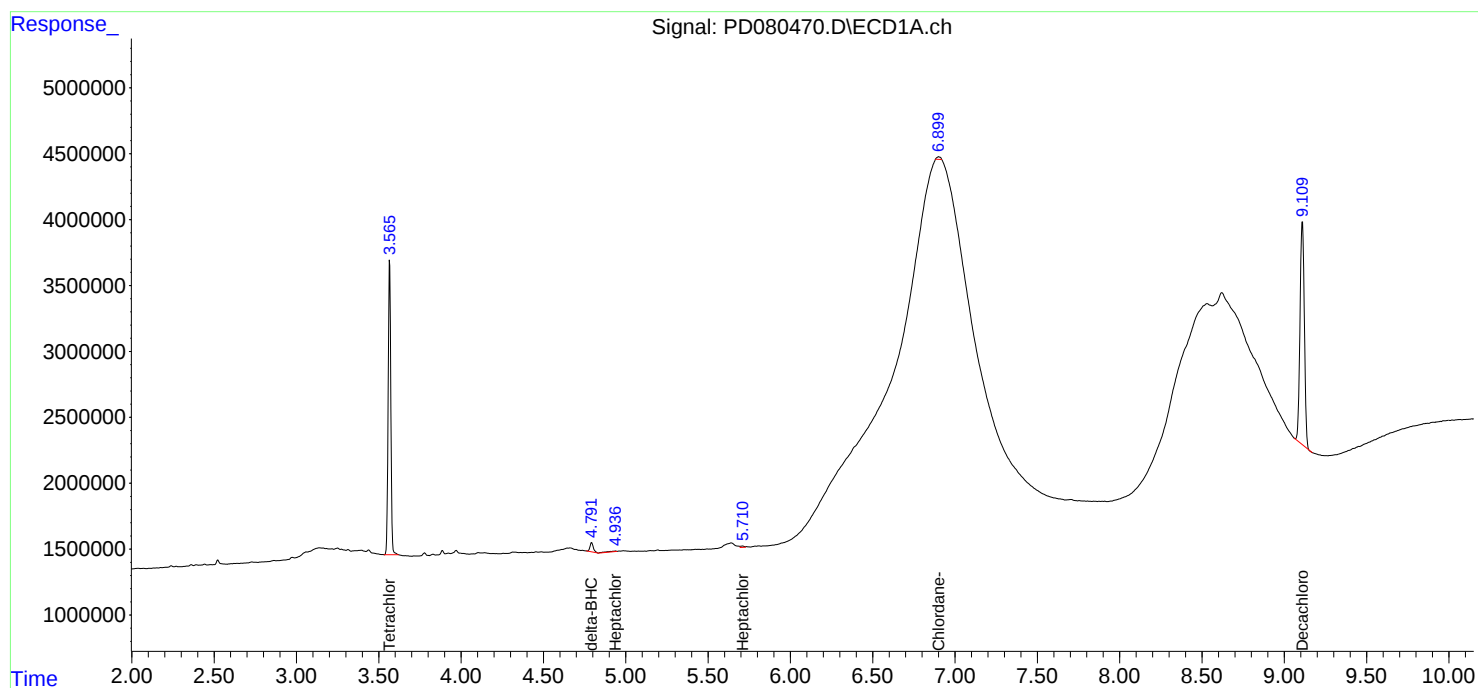

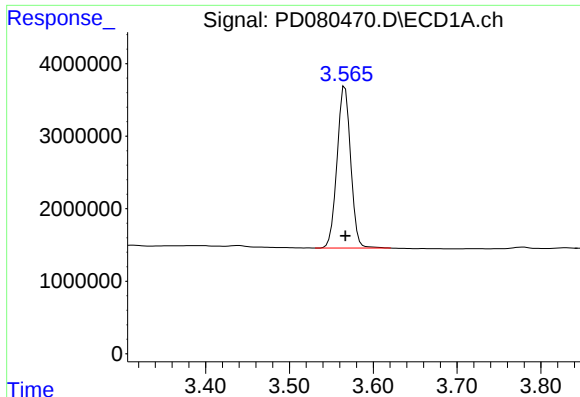


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 25169166
Conc: 16.70 ng/ml

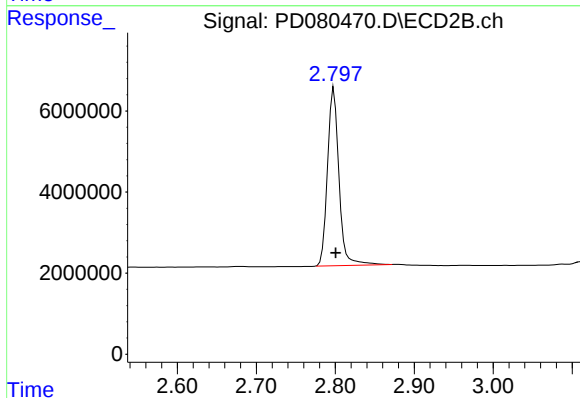


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: -0.002 min
Response: 44448441
Conc: 17.68 ng/ml

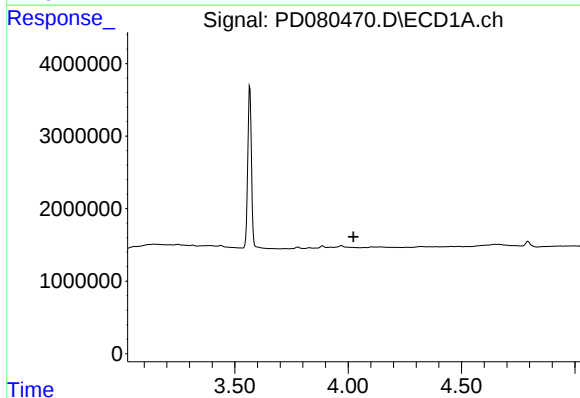


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

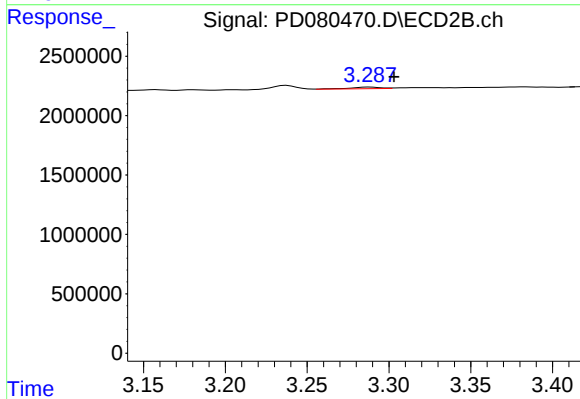


#2 alpha-BHC

R.T.: 3.289 min
Delta R.T.: -0.014 min
Response: 166869
Conc: 0.04 ng/ml

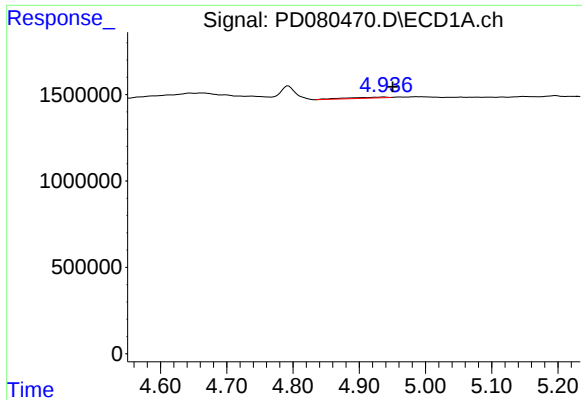


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: -0.013 min
Response: 212197
Conc: 0.09 ng/ml

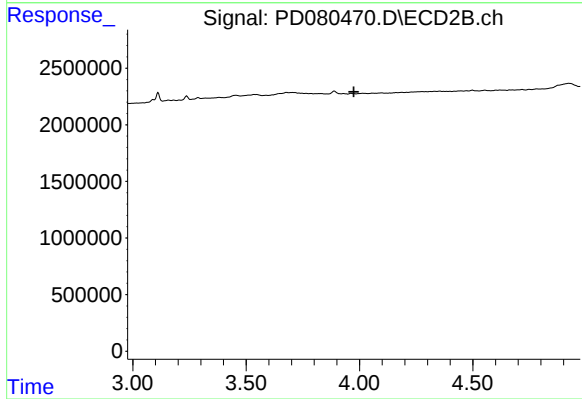


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.975 min
Response: 0
Conc: N.D.

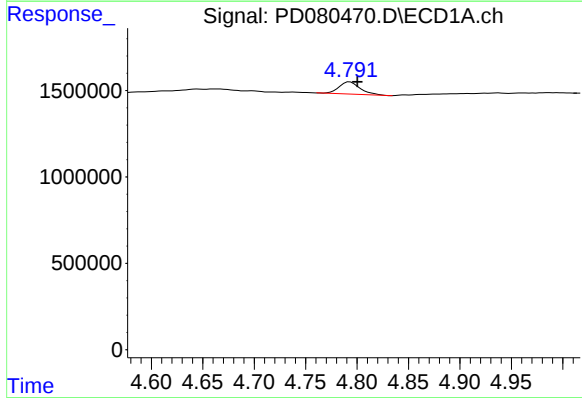


#7 delta-BHC

R.T.: 4.793 min
Delta R.T.: -0.007 min
Response: 1011206
Conc: 0.41 ng/ml

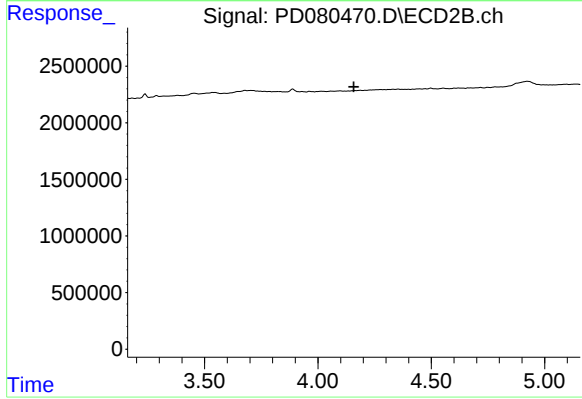


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.158 min
Response: 0
Conc: N.D.

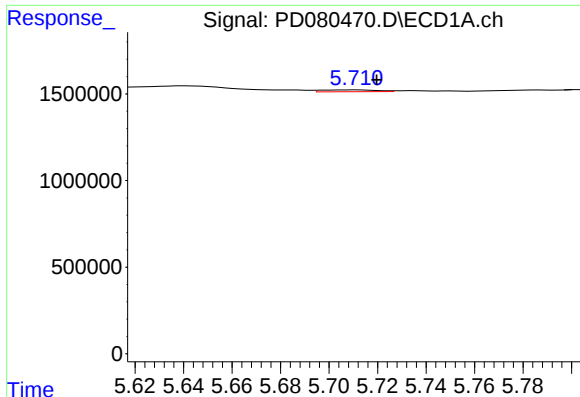


#8 Heptachlor epoxide

R.T.: 5.712 min
Delta R.T.: -0.008 min
Response: 165242
Conc: 0.08 ng/ml

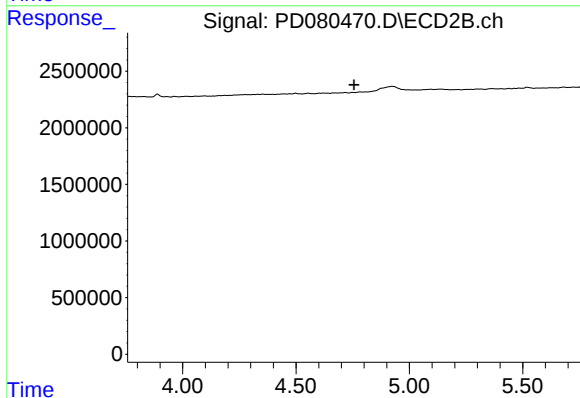


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

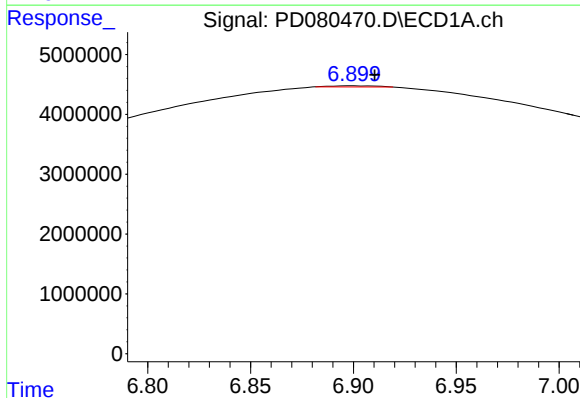


#27 Chlordane-5

R.T.: 6.900 min
Delta R.T.: -0.010 min
Response: 314544
Conc: 4.65 ng/ml

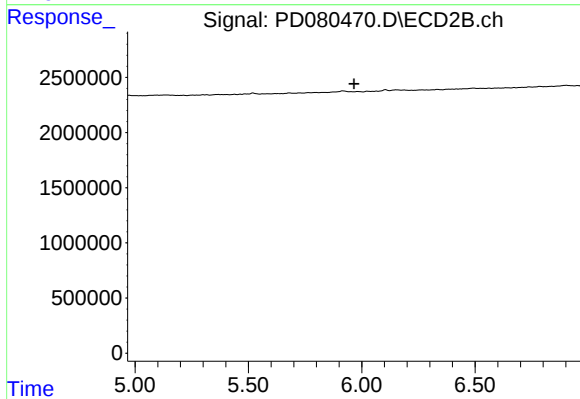


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.966 min
Response: 0
Conc: N.D.

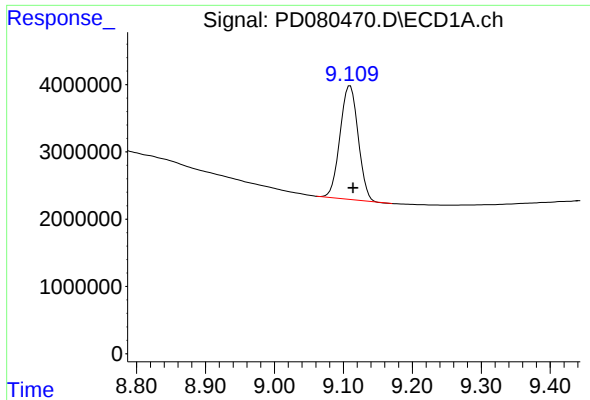

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.004 min
Response: 30793438
Conc: 15.21 ng/ml

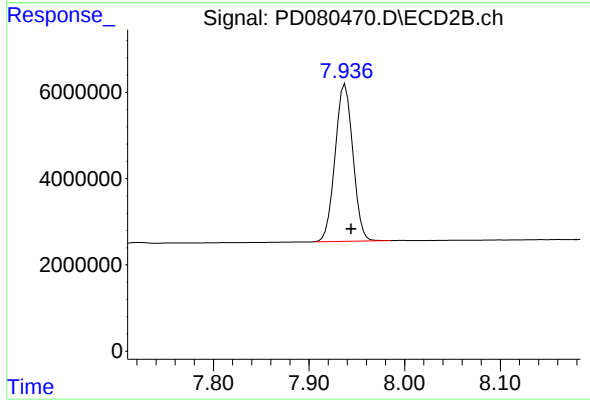

#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.006 min
Response: 47046030
Conc: 16.69 ng/ml