

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 16:52
 Operator : AR\AJ
 Sample : 05862-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-LIQUIDS-20231213-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2023
 Supervised By : Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:21:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.565	2.800	29602481	50494728	19.641m	20.087
2) SA Decachlor...	9.111	7.938	28934340	42682084	14.294	15.141

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 16:52
Operator : AR\AJ
Sample : 05862-13
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-LIQUIDS-20231213-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:21:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

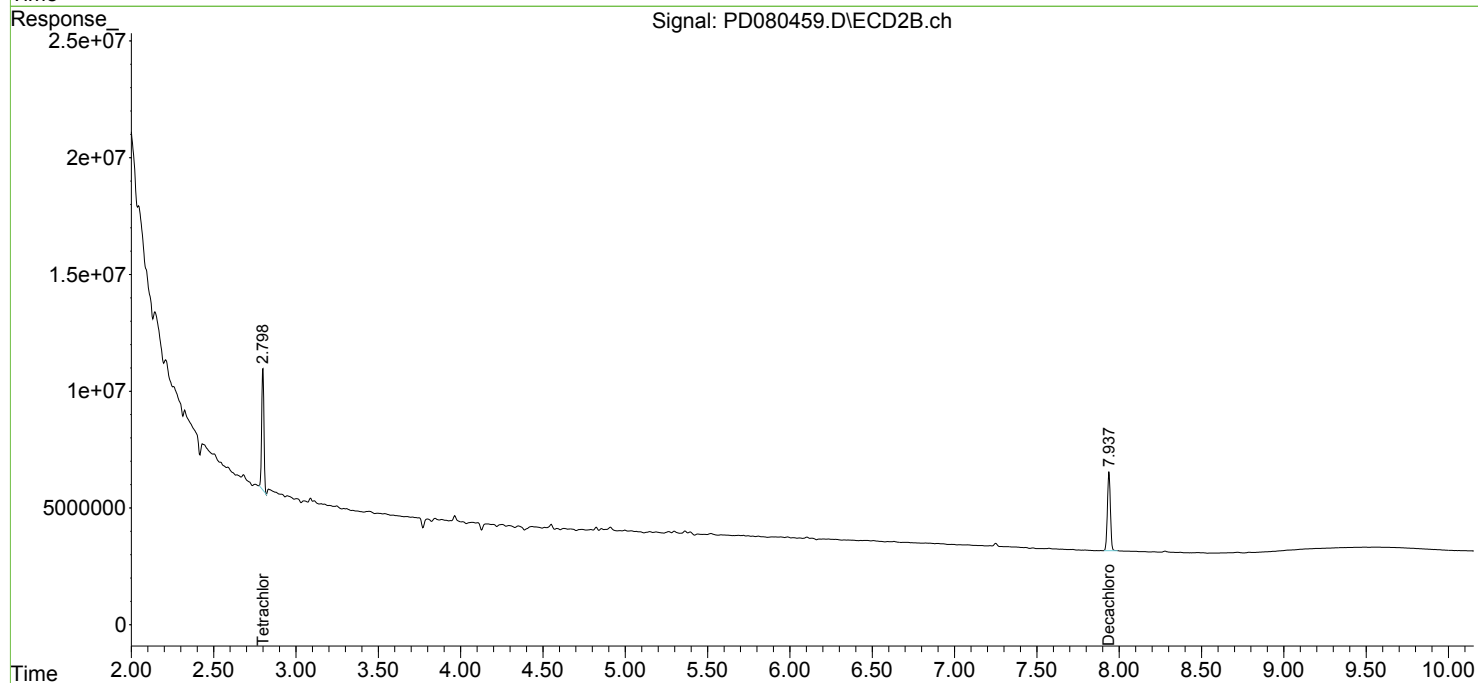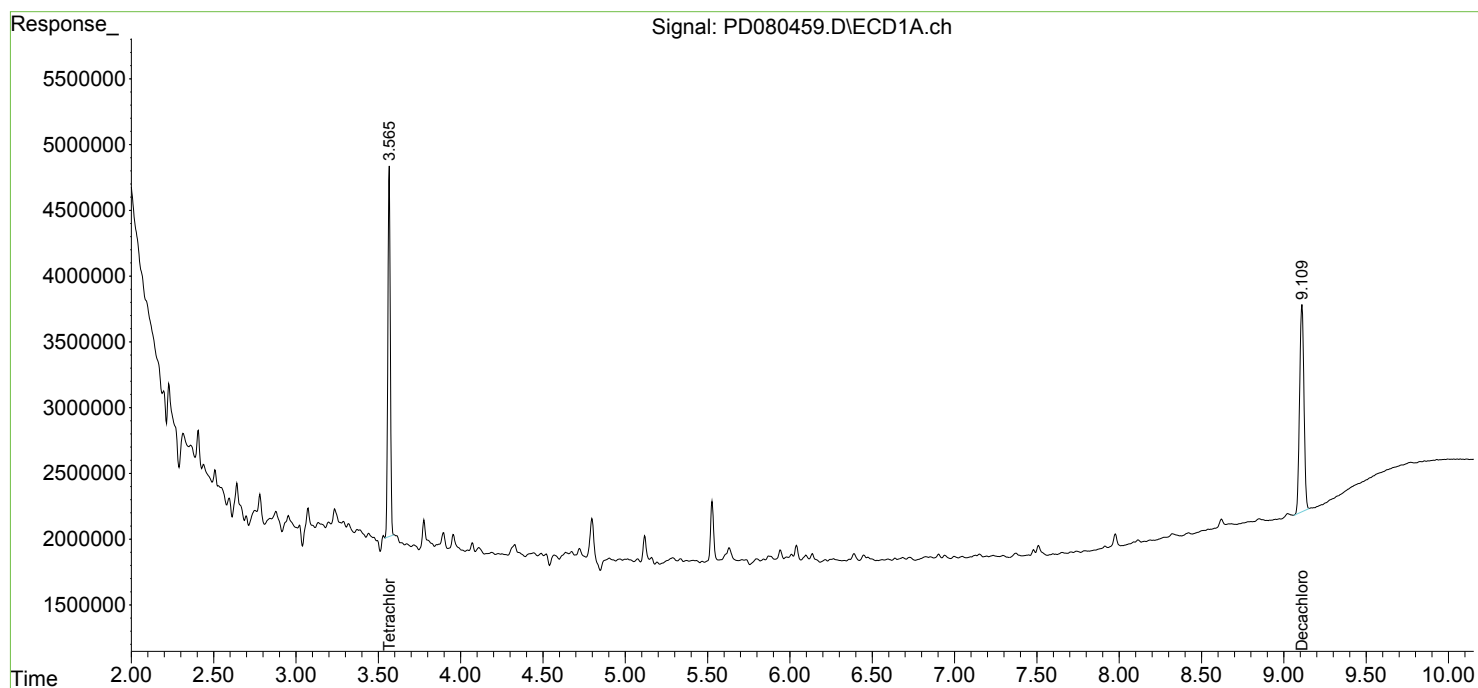

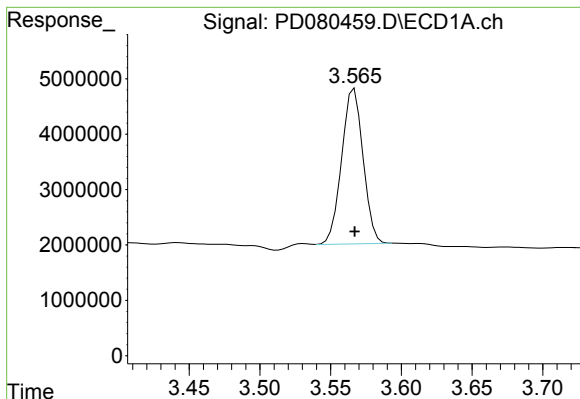


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.002 min
Response: 29602481
Conc: 19.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-LIQUIDS-20231213-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/28/2023

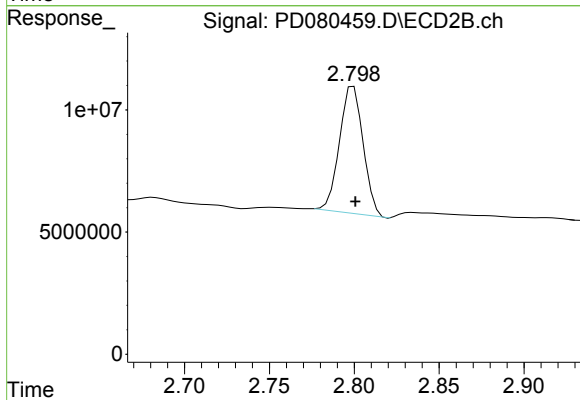


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: -0.001 min
Response: 50494728
Conc: 20.09 ng/ml

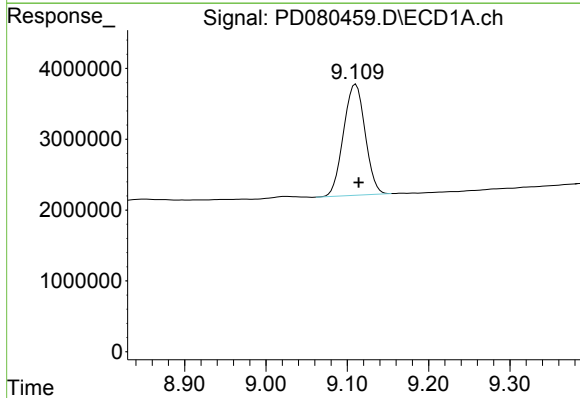

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.004 min
Response: 28934340
Conc: 14.29 ng/ml

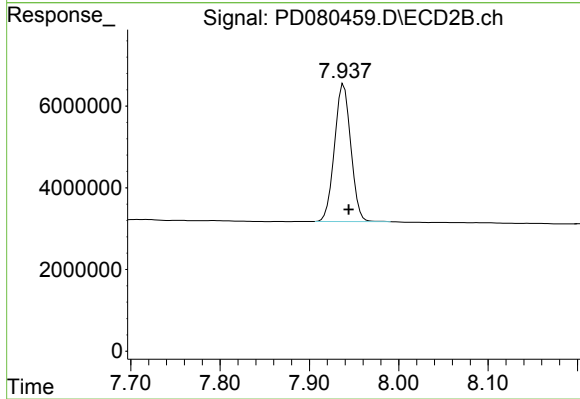

#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.005 min
Response: 42682084
Conc: 15.14 ng/ml