

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
 Data File : PD080466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Dec 2023 18:25
 Operator : AR\AJ
 Sample : 05926-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MR-319-3.7-4.7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 23:23:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.799	26634738	45598500	17.672	18.139
28)	SA Decachlor...	9.108	7.938	31056351	44603125	15.343	15.823

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122623\
Data File : PD080466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Dec 2023 18:25
Operator : AR\AJ
Sample : 05926-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MR-319-3.7-4.7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 23:23:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

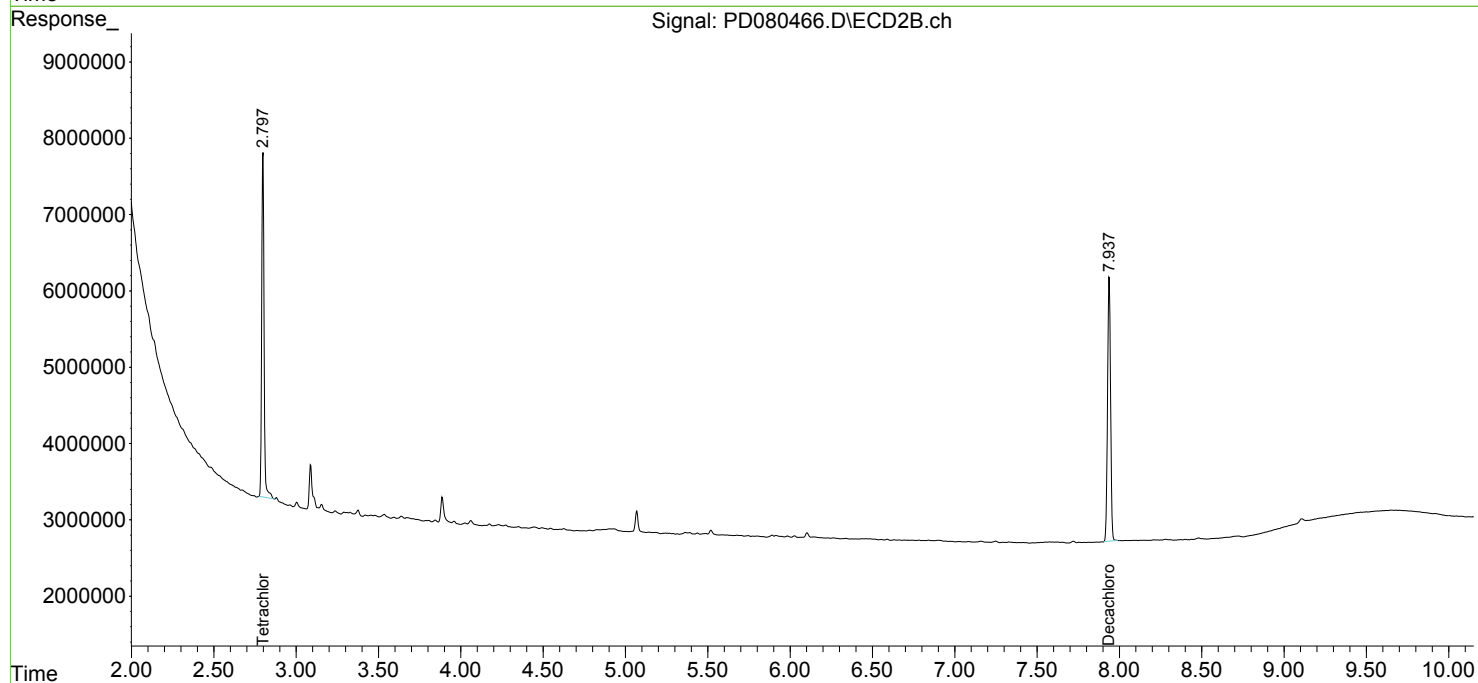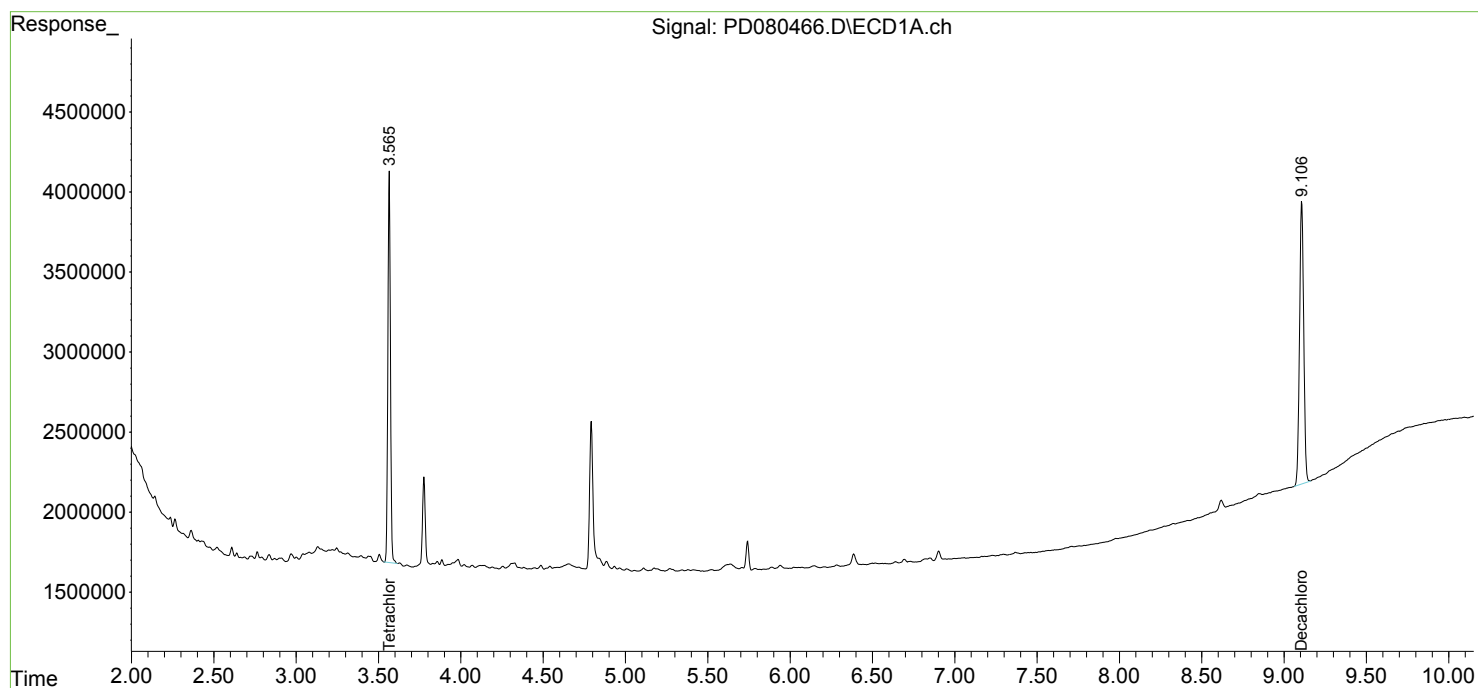


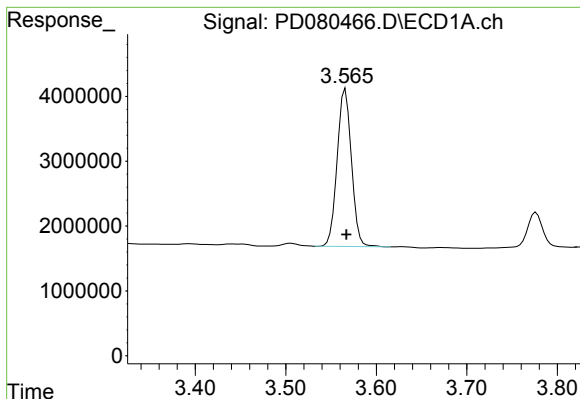

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: -0.001 min
Response: 26634738
Conc: 17.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
MR-319-3.7-4.7

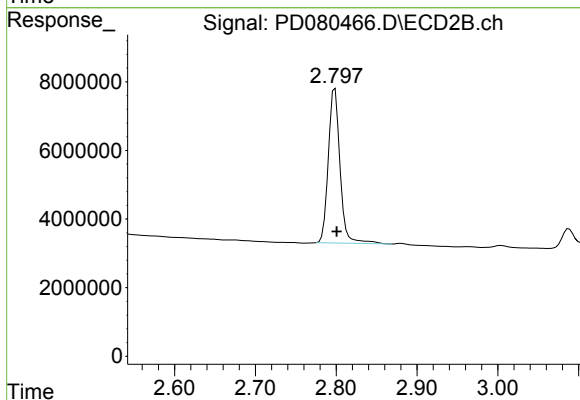


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: -0.002 min
Response: 45598500
Conc: 18.14 ng/ml

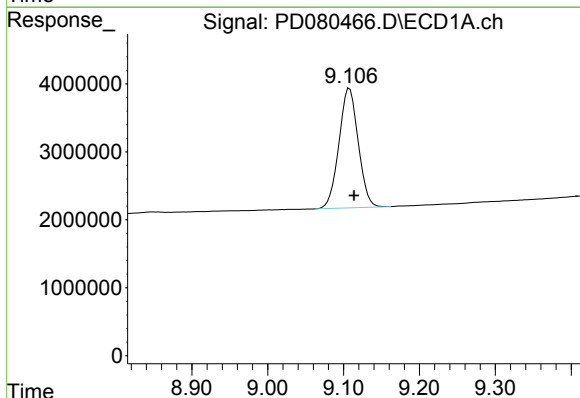

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.006 min
Response: 31056351
Conc: 15.34 ng/ml

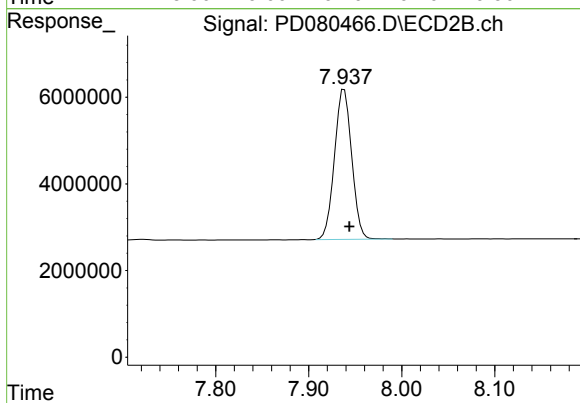

#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.006 min
Response: 44603125
Conc: 15.82 ng/ml