

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122624\
 Data File : PD087353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 16:46
 Operator : AR\AJ
 Sample : P5334-05MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2921MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 21:50:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 23:32:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.882	30845611	197.6E6	15.066m	16.982
27)	SA Decachlor...	9.079	8.082	47494876	211.9E6	15.551m	16.087
Target Compounds							
2)	A alpha-BHC	4.004	3.396	220.0E6	906.9E6	54.519	49.751
3)	MA gamma-BHC...	4.334	3.732	213.1E6	856.8E6	54.570m	50.643
4)	MA Heptachlor	4.934	4.087	202.3E6	813.0E6	50.990m	47.021
5)	MB Aldrin	5.278	4.373	196.7E6	805.8E6	50.502	48.146
6)	B beta-BHC	4.520	4.028	66761282	340.4E6	38.178	43.497
7)	B delta-BHC	4.766	4.265	208.5E6	855.5E6	52.454m	49.274
8)	B Heptachlo...	5.697	4.877	176.5E6	720.2E6	48.886	45.938
9)	A Endosulfan I	6.079	5.252	169.7E6	678.2E6	50.802m	46.793m
10)	B trans-Chl...	5.952	5.131	168.2E6	755.8E6	48.121	46.447
11)	B cis-Chlor...	6.031	5.194	175.6E6	775.0E6	49.460m	49.334m
12)	B 4,4'-DDE	6.202	5.381	316.2E6	1442.3E6	95.564	96.814
13)	MA Dieldrin	6.352	5.517	380.6E6	1444.5E6	105.229m	94.356m
14)	MA Endrin	6.580	5.795	304.1E6	1263.8E6	101.779	90.460
15)	B Endosulfa...	6.791	6.087	269.4E6	1098.5E6	90.130	80.902
16)	A 4,4'-DDD	6.710	5.936	256.4E6	998.0E6	98.916	81.961
17)	MA 4,4'-DDT	7.027	6.191	262.5E6	1136.5E6	97.925	90.140
18)	B Endrin al...	6.920	6.265	191.0E6	801.9E6	81.394	76.750
19)	B Endosulfa...	7.154	6.489	281.9E6	1147.4E6	97.256	86.791
20)	A Methoxychlor	7.497	6.761	737.8E6	2400.9E6	495.948m	411.825m
21)	B Endrin ke...	7.635	6.997	300.3E6	1031.7E6	93.595	71.374

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122624\
Data File : PD087353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 16:46
Operator : AR\AJ
Sample : P5334-05MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 21:50:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 23:32:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

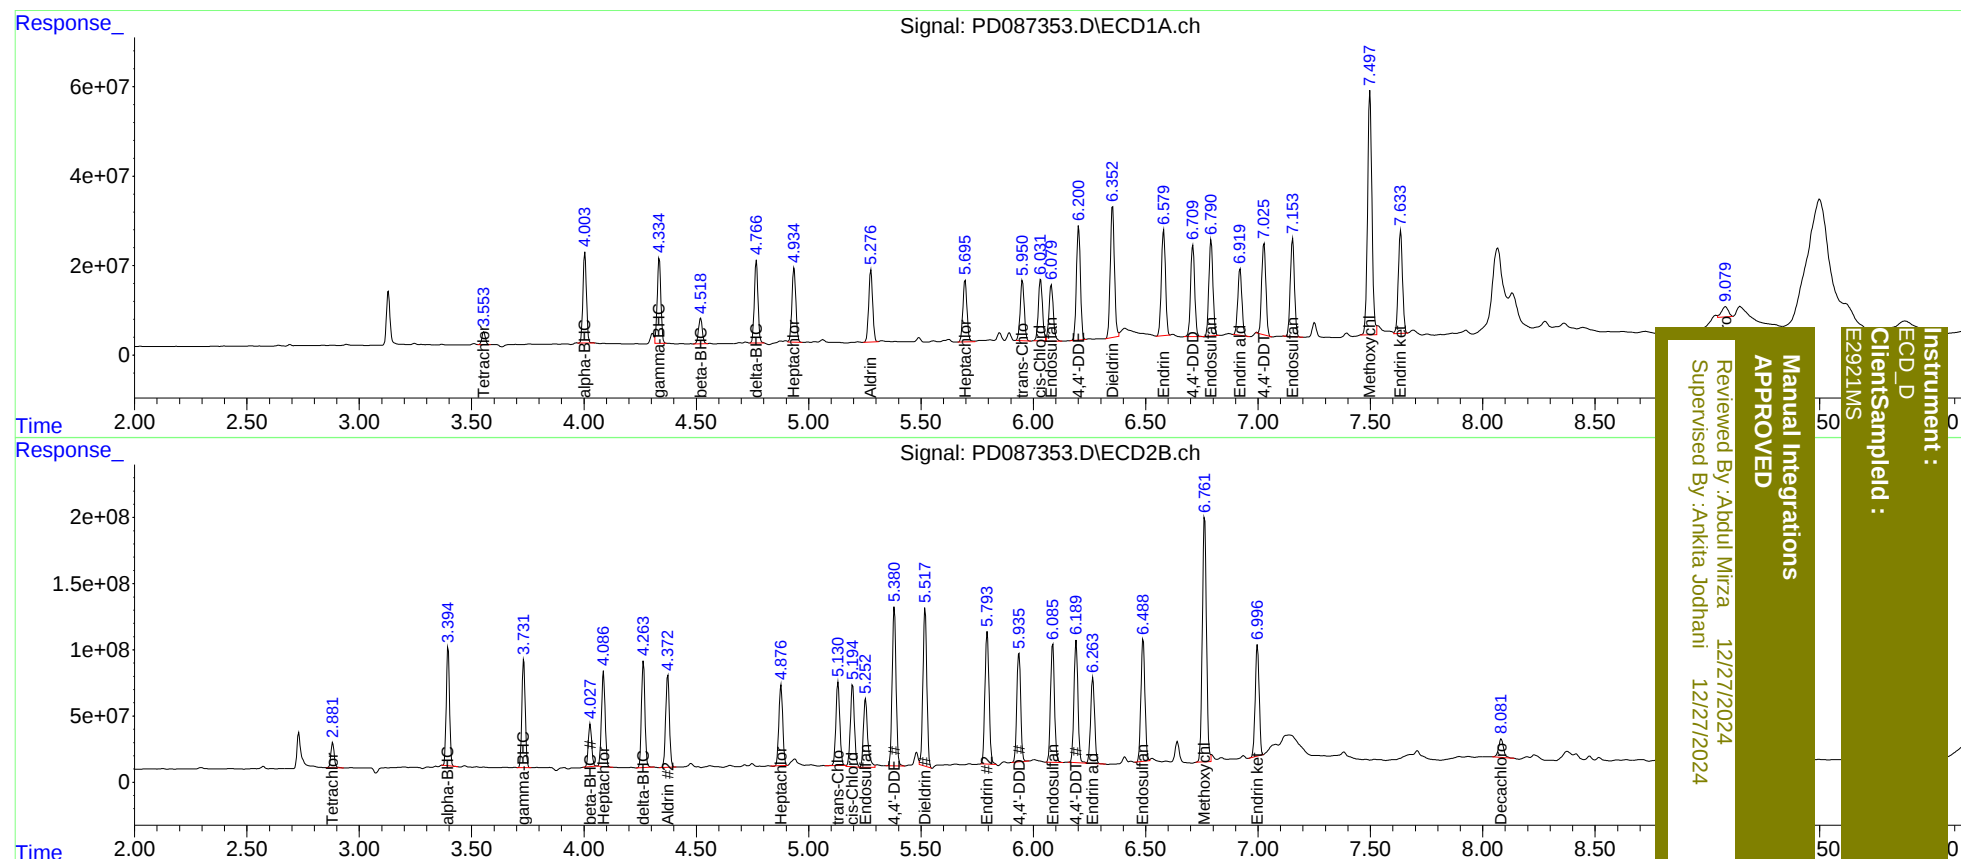

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 12/27/2024
Supervised By: Ankita Jodhani 12/27/2024

Instrument :
ECD_D
Client Sampled :
EZ921MS