

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122718\
 Data File : PD050897.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Dec 2018 17:15
 Operator : AJ\SJ
 Sample : PIBLK26
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 07:04:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122718CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 27 14:51:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.226	4.045	28212520	471.8E6	18.287	17.498
27) SA Decachlor...	7.827	9.151	38304509	646.6E6	33.998	34.769
Target Compounds						
6) B beta-BHC	0.000	4.937f	0	40495707	N.D.	2.416


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122718\
Data File : PD050897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Dec 2018 17:15
Operator : AJ\SJ
Sample : PIBLK26
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 07:04:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122718CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 27 14:51:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

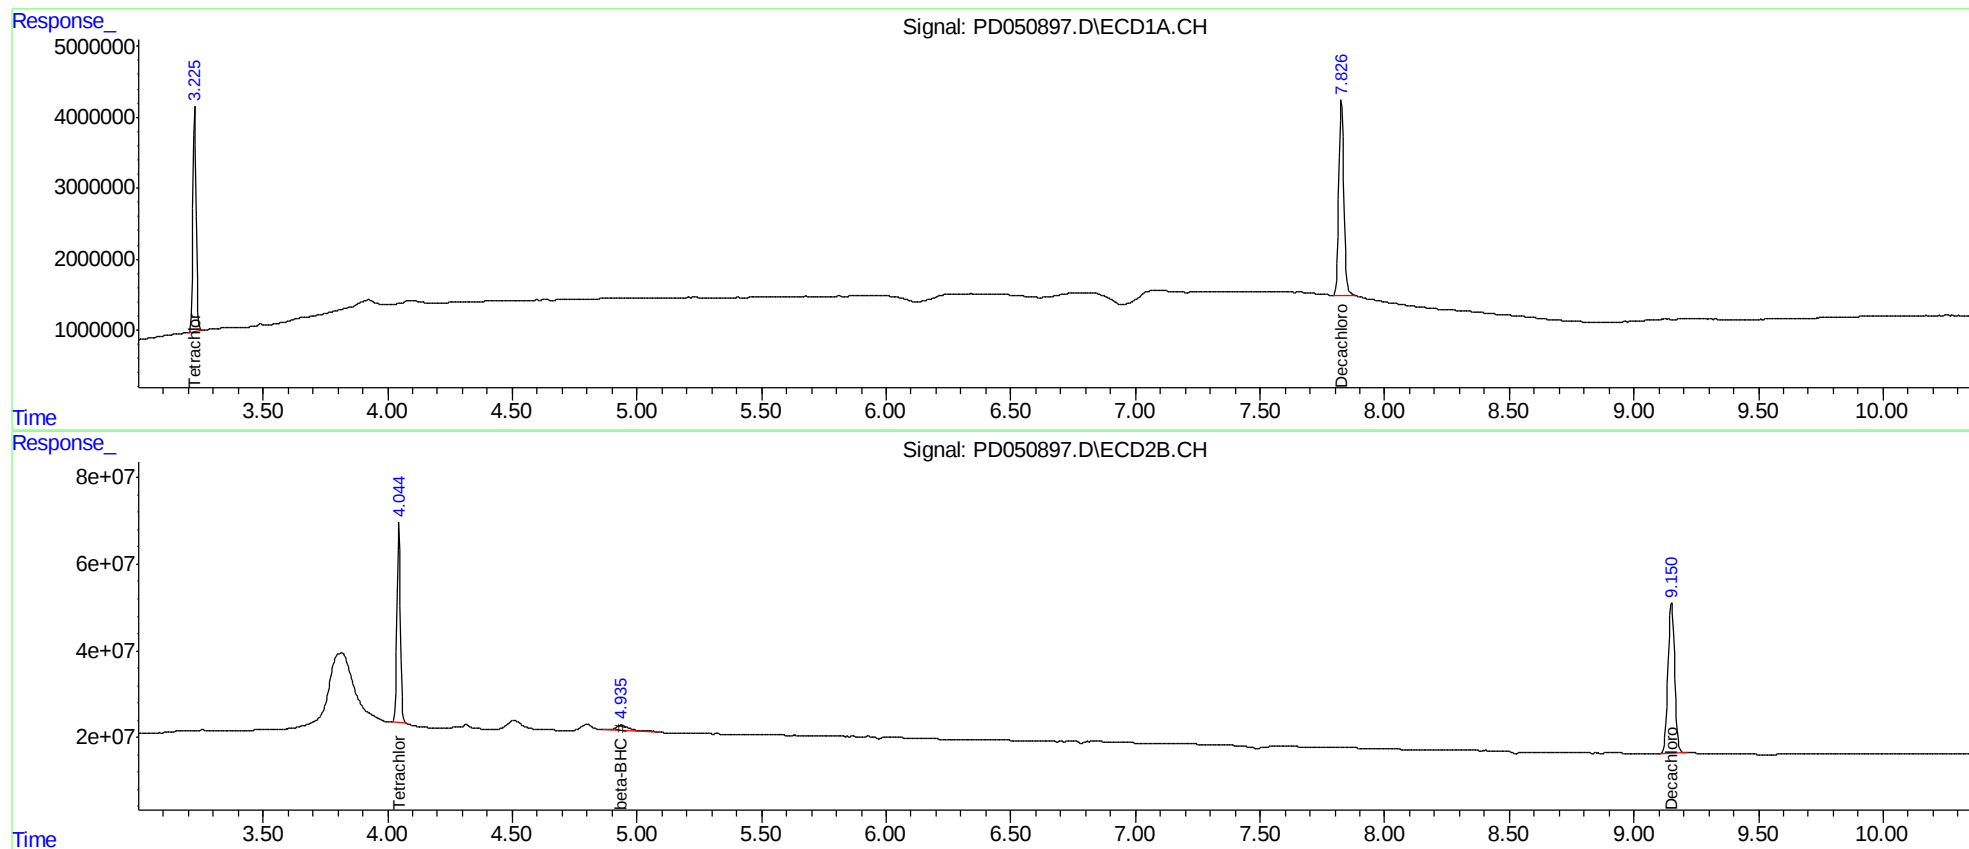


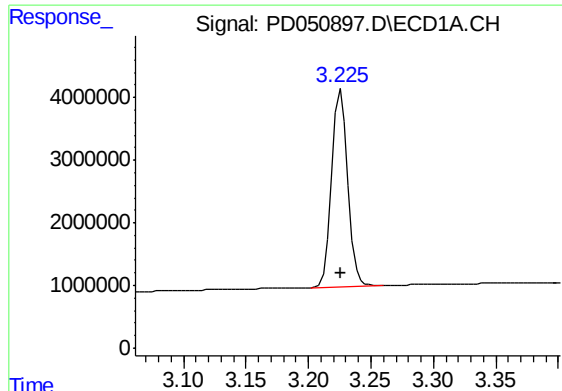

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 28212520
Conc: 18.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK26

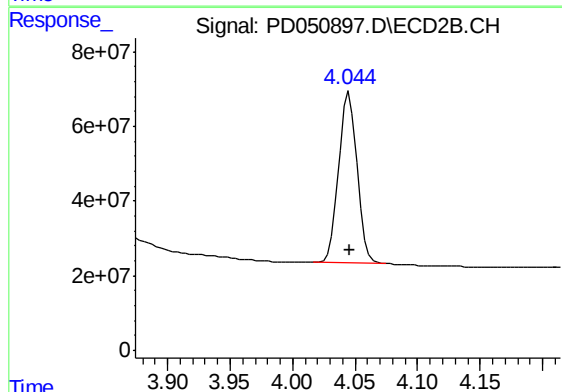


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 471796395
Conc: 17.50 ng/ml

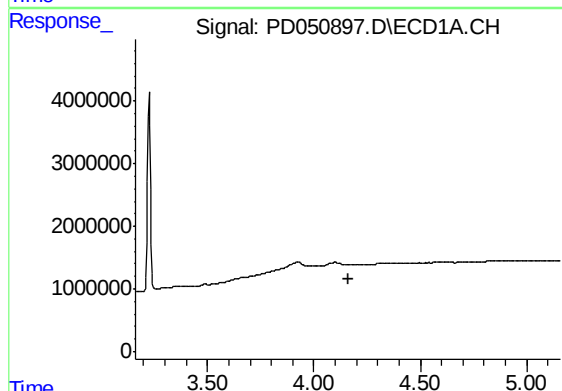


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

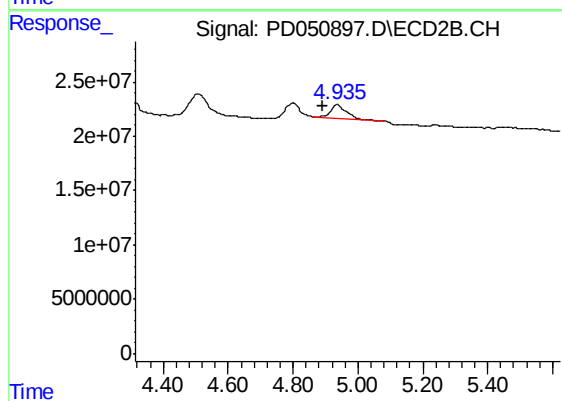

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.044 min
Response: 40495707
Conc: 2.42 ng/ml

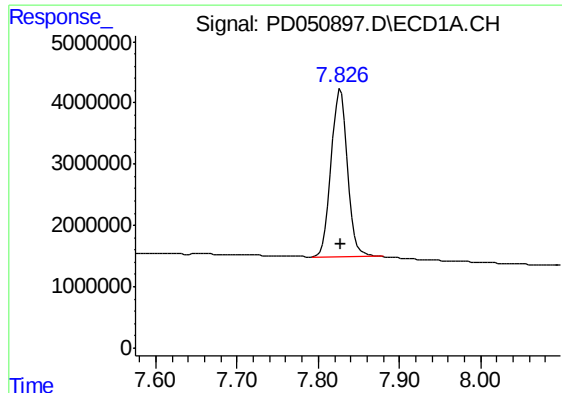

#27 Decachlorobiphenyl

R.T.: 7.827 min
Delta R.T.: 0.000 min
Response: 38304509
Conc: 34.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK26

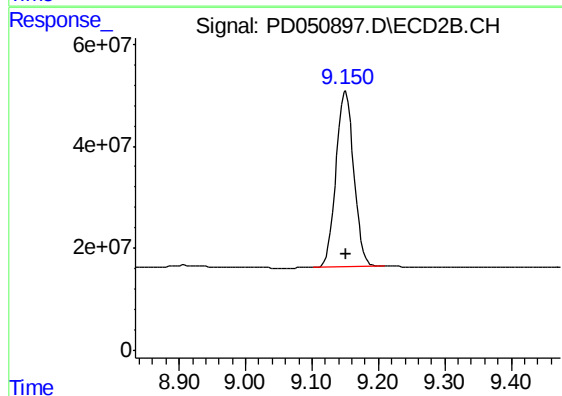

#27 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 646579703
Conc: 34.77 ng/ml