

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
 Data File : PD056797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 13:14
 Operator : SG\AJ
 Sample : PB125669BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK69

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 22:40:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.960	16810990	31230319	20.298	25.976 #
27)	SA Decachlor...	7.960	8.995	36133577	53960951	40.016	44.850
Target Compounds							
15)	B Endosulfa...	0.000	6.871	0	1500535	N.D.	1.024


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
Data File : PD056797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 13:14
Operator : SG\AJ
Sample : PB125669BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK69

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 22:40:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

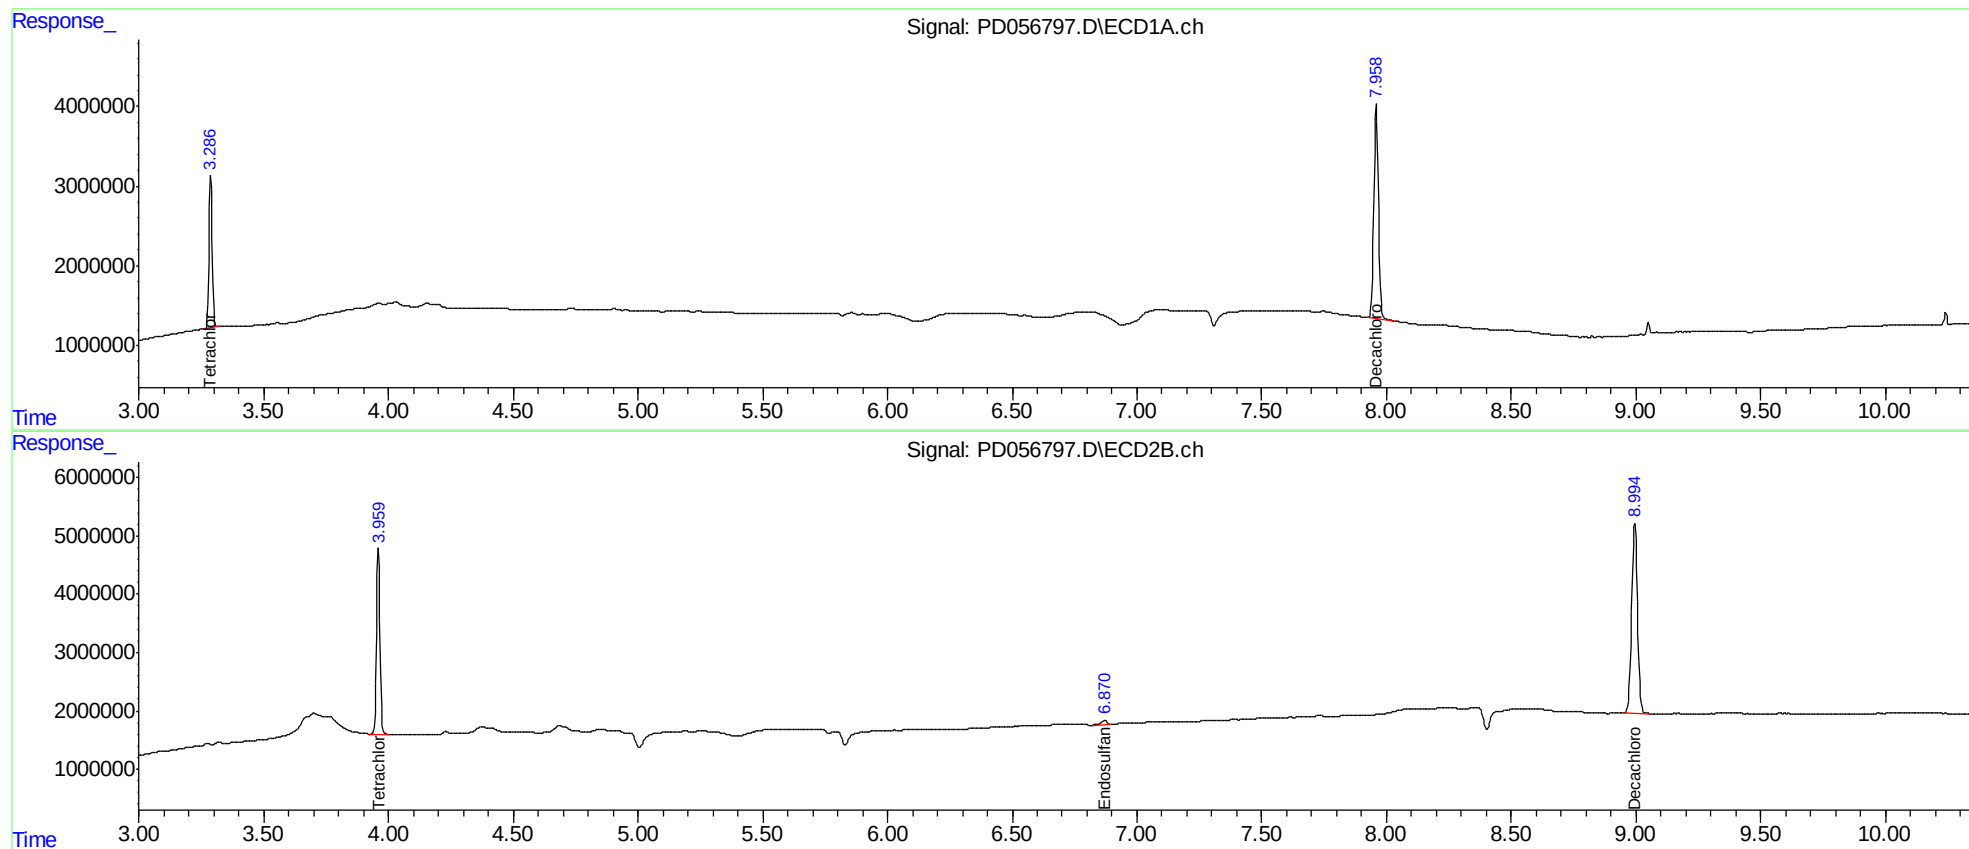


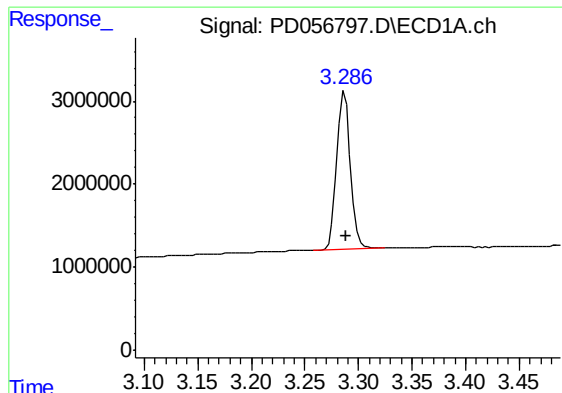

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 16810990
Conc: 20.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK69

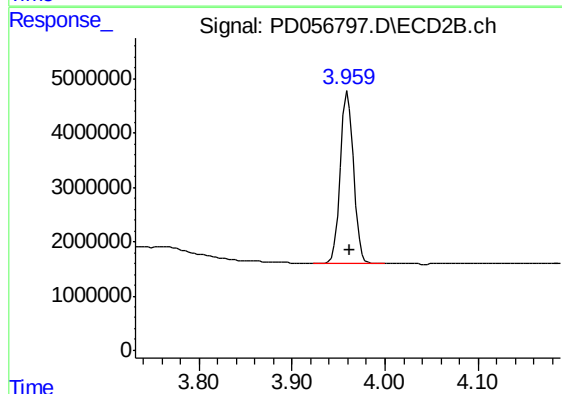


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 31230319
Conc: 25.98 ng/ml

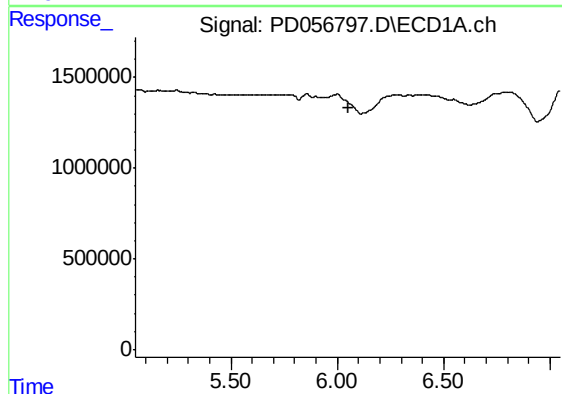


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

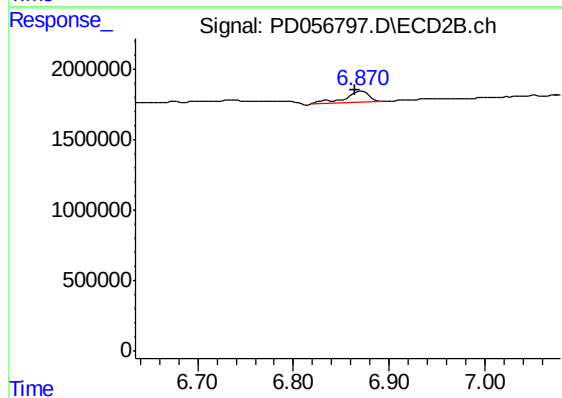

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.007 min
Response: 1500535
Conc: 1.02 ng/ml

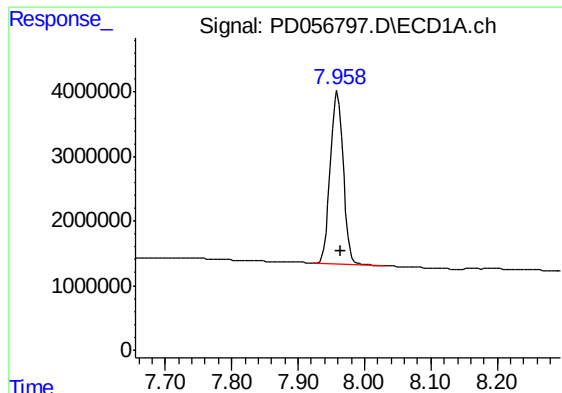

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 36133577
Conc: 40.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK69

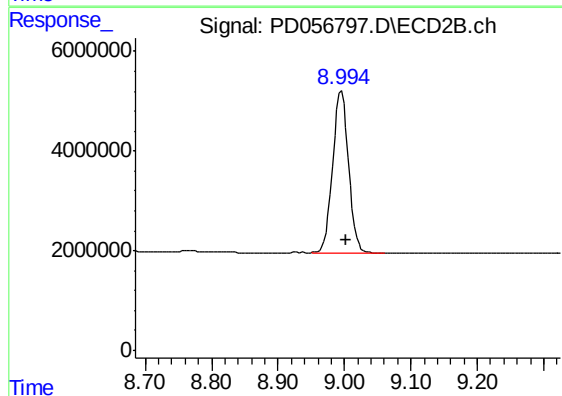

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.007 min
Response: 53960951
Conc: 44.85 ng/ml