

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
 Data File : PD056806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 15:20
 Operator : SG\AJ
 Sample : K6278-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C70

Manual Integrations
 APPROVED

Ankita
 12/30/2019 4:15:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:47:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	6985847	12379104	8.435	10.297
2)	SA Decachlor...	7.957	8.994	10694432	13774775	11.844	11.449
Target Compounds							
3)	MA gamma-BHC...	3.992	4.610	2137639	2123606	1.904m	1.316m#
10)	B trans-Chl...	5.180	6.042	542683	6259857	0.518m	3.786 #
16)	A 4,4'-DDD	5.911	6.774	852332	3362640	1.198m	2.858 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
Data File : PD056806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 15:20
Operator : SG\AJ
Sample : K6278-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:47:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

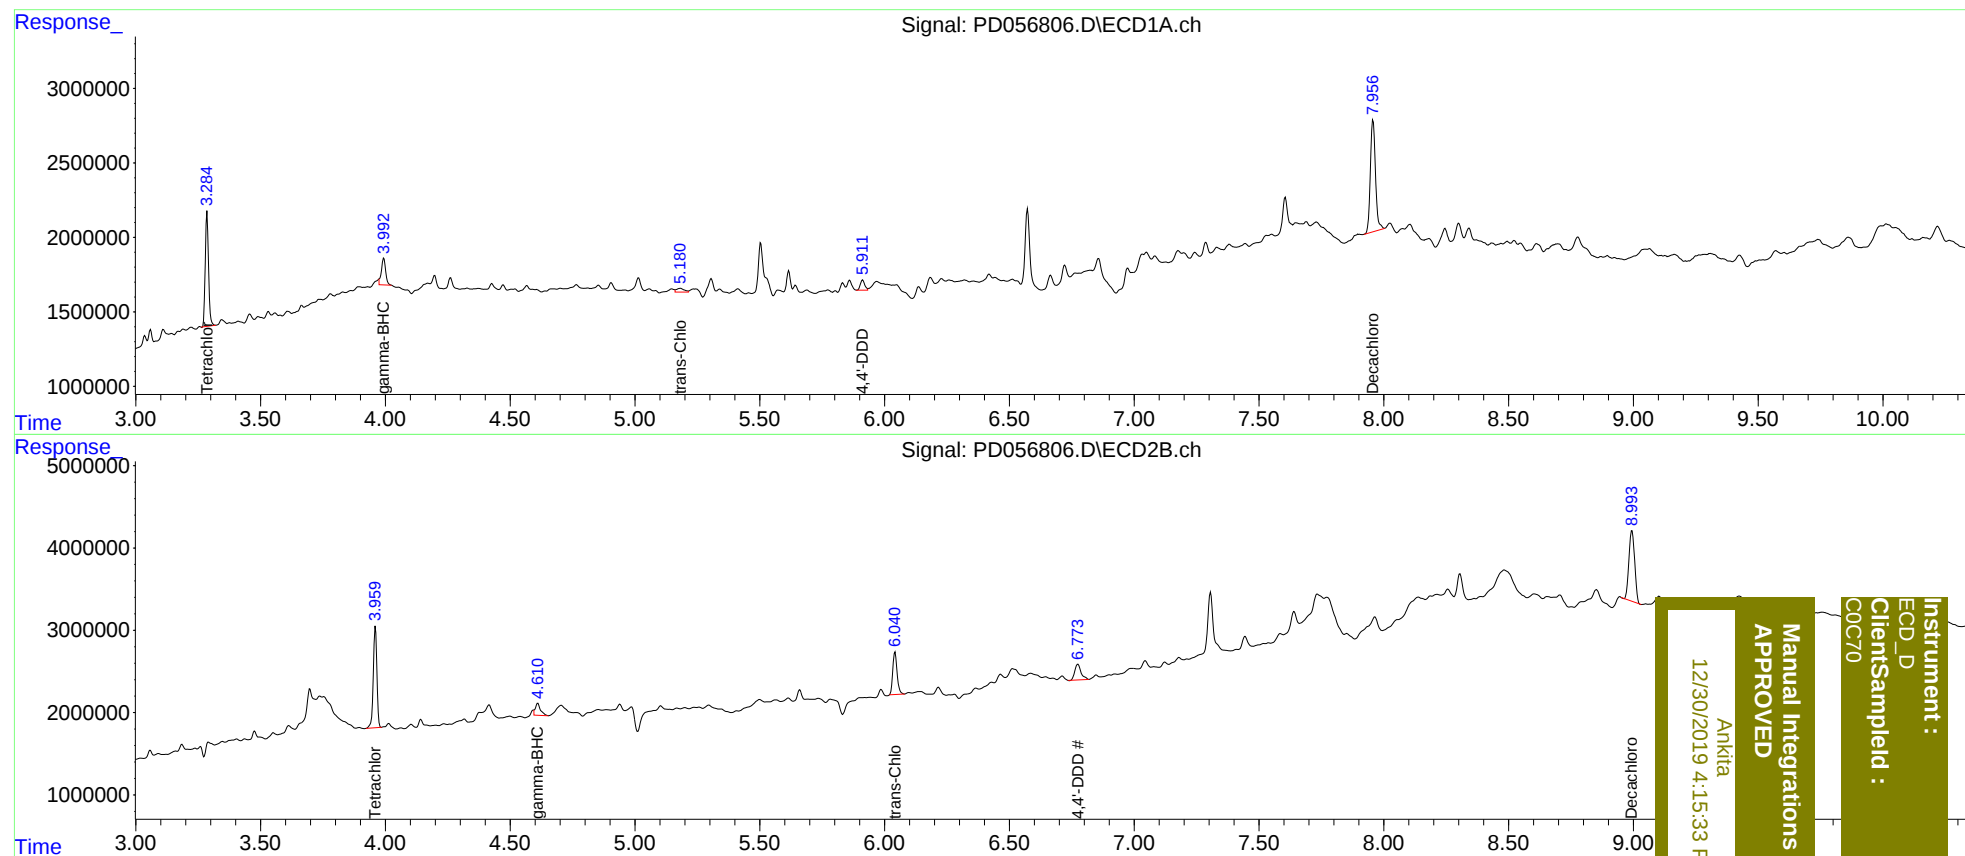

12/30/2019 4:15:33 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0C70