

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
 Data File : PD056805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2019 15:06
 Operator : SG\AJ
 Sample : K6278-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C67

Manual Integrations
 APPROVED

Ankita
 12/30/2019 4:15:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:38:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	7381797	11973924	8.913	9.960
27)	SA Decachlor...	7.957	8.994	9186655	12584880	10.174	10.460m
Target Compounds							
3)	MA gamma-BHC...	3.993	4.610	4174346	3995518	3.717m	2.476m#
13)	MA Dieldrin	5.535	6.426	6509879	9360650	6.409	5.957
14)	MA Endrin	5.772	6.644	3116101	2288053	3.729m	1.808 #
15)	B Endosulfa...	6.035	6.844	3077285	6149974	3.231m	4.197m#
16)	A 4,4'-DDD	5.909	6.778	1813795	34940948	2.549m	29.692m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122719\
Data File : PD056805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2019 15:06
Operator : SG\AJ
Sample : K6278-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:38:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

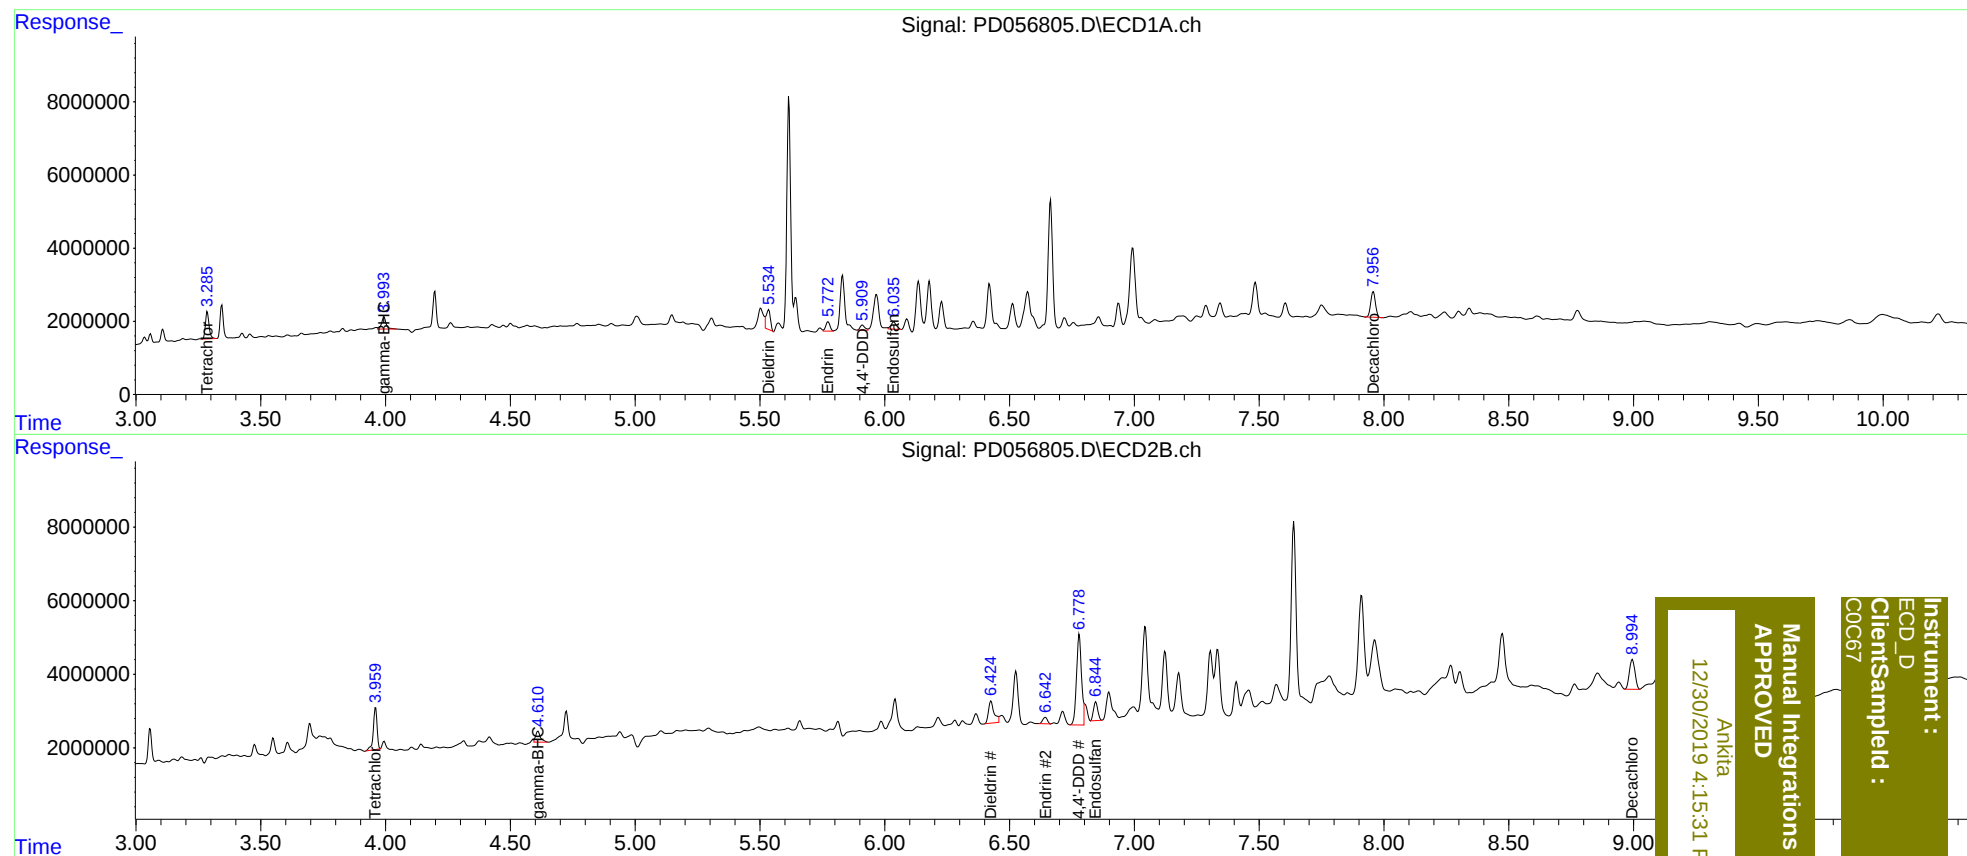

Manual Integrations
APPROVED

Ankita
12/30/2019 4:15:31 PM

Instrument :
ECD_D
Client Sample :
C0C67