

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
 Data File : PD067501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 09:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 04:06:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.032	0	3085620	N.D.	0.694 #
Target Compounds							
15)	B Endosulfa...	6.260f	0.000	3258364	0	1.659	N.D. #
18)	B Endrin al...	0.000	6.994	0	236709	N.D.	0.055 #
27)	Chlordane-5	6.260	0.000	3258364	0	40.637	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
Data File : PD067501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 09:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 04:06:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

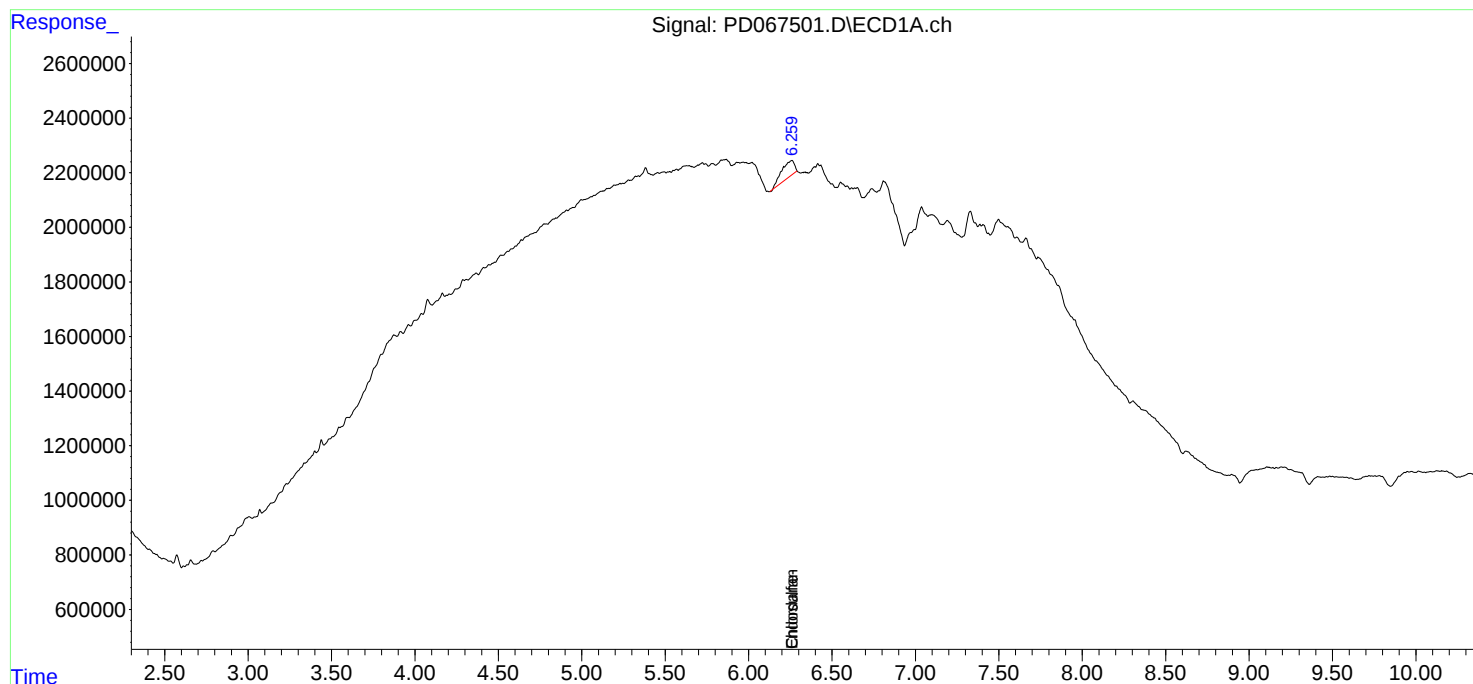


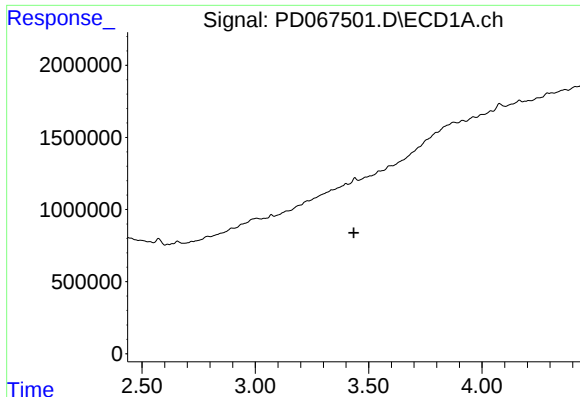

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

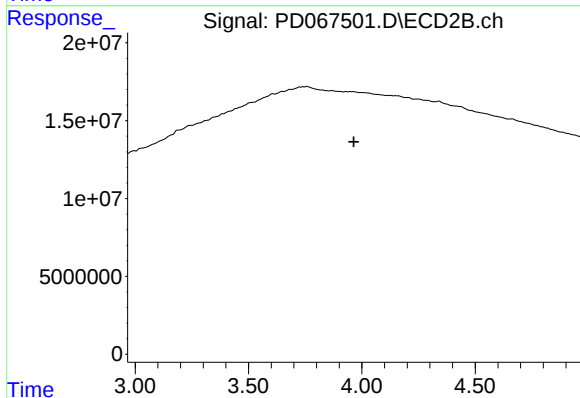


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.964 min
Response: 0
Conc: N.D.

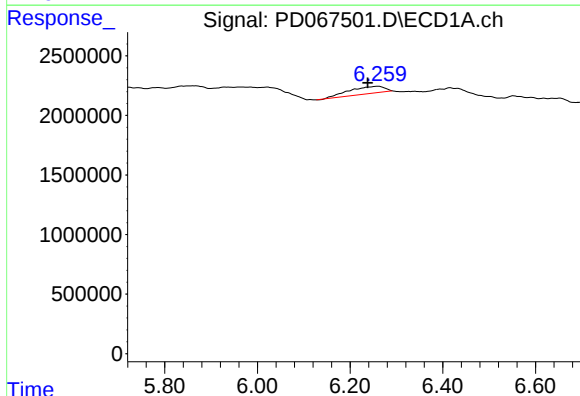


#15 Endosulfan II

R.T.: 6.260 min
Delta R.T.: 0.022 min
Response: 3258364
Conc: 1.66 ng/ml

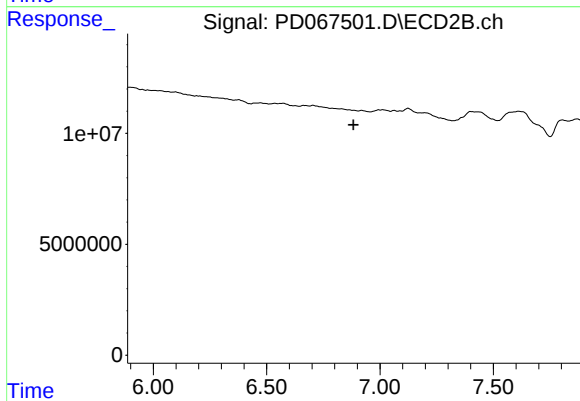

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.884 min
Response: 0
Conc: N.D.

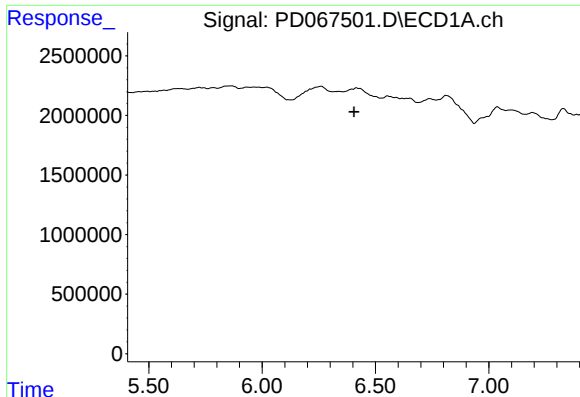

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

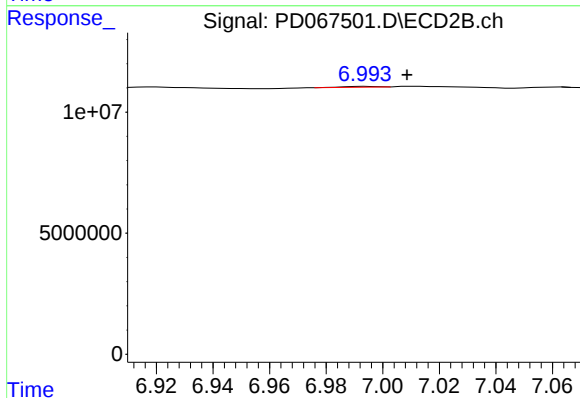


#18 Endrin aldehyde

R.T.: 6.994 min
Delta R.T.: -0.014 min
Response: 236709
Conc: 0.05 ng/ml

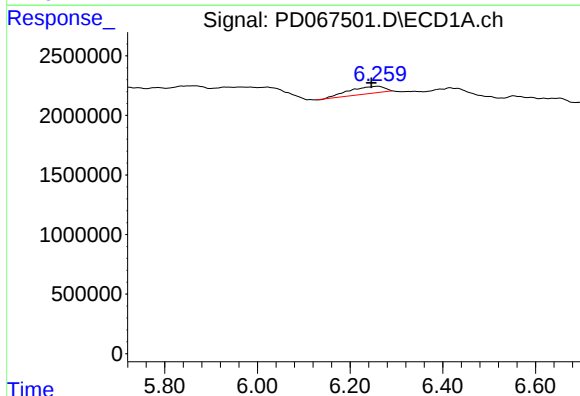


#27 Chlordane-5

R.T.: 6.260 min
Delta R.T.: 0.014 min
Response: 3258364
Conc: 40.64 ng/ml

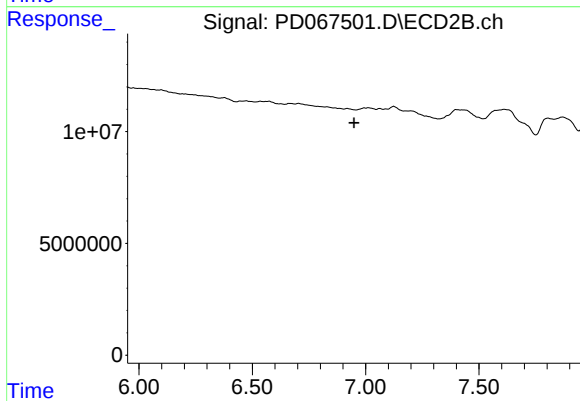

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.949 min
Response: 0
Conc: N.D.

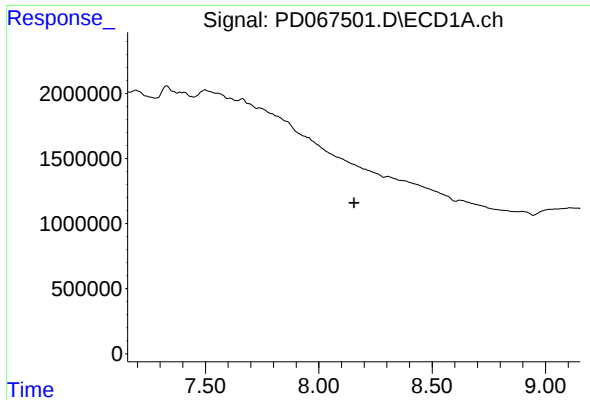

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

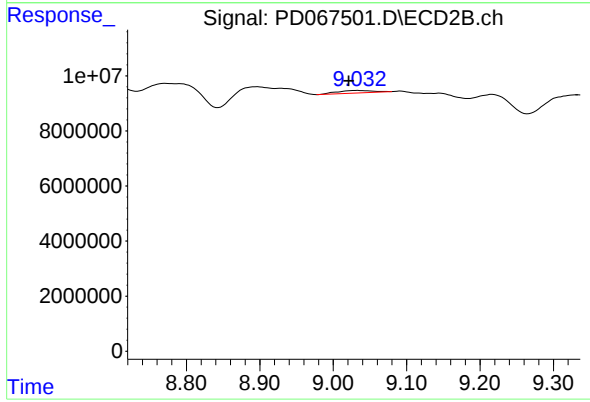

#28 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.011 min
Response: 3085620
Conc: 0.69 ng/ml