

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
 Data File : PD067507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 11:49
 Operator : AR\AJ
 Sample : M5210-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 124027

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
 Supervised By :mohammad ahmed 12/29/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:06:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 04:06:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.963	20744994	89662769	11.339	10.162m
28)	SA Decachlor...	8.156	9.018	10436681	54116424	11.321	12.174

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
Data File : PD067507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 11:49
Operator : AR\AJ
Sample : M5210-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
124027


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
Supervised By :mohammad ahmed 12/29/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:06:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 04:06:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

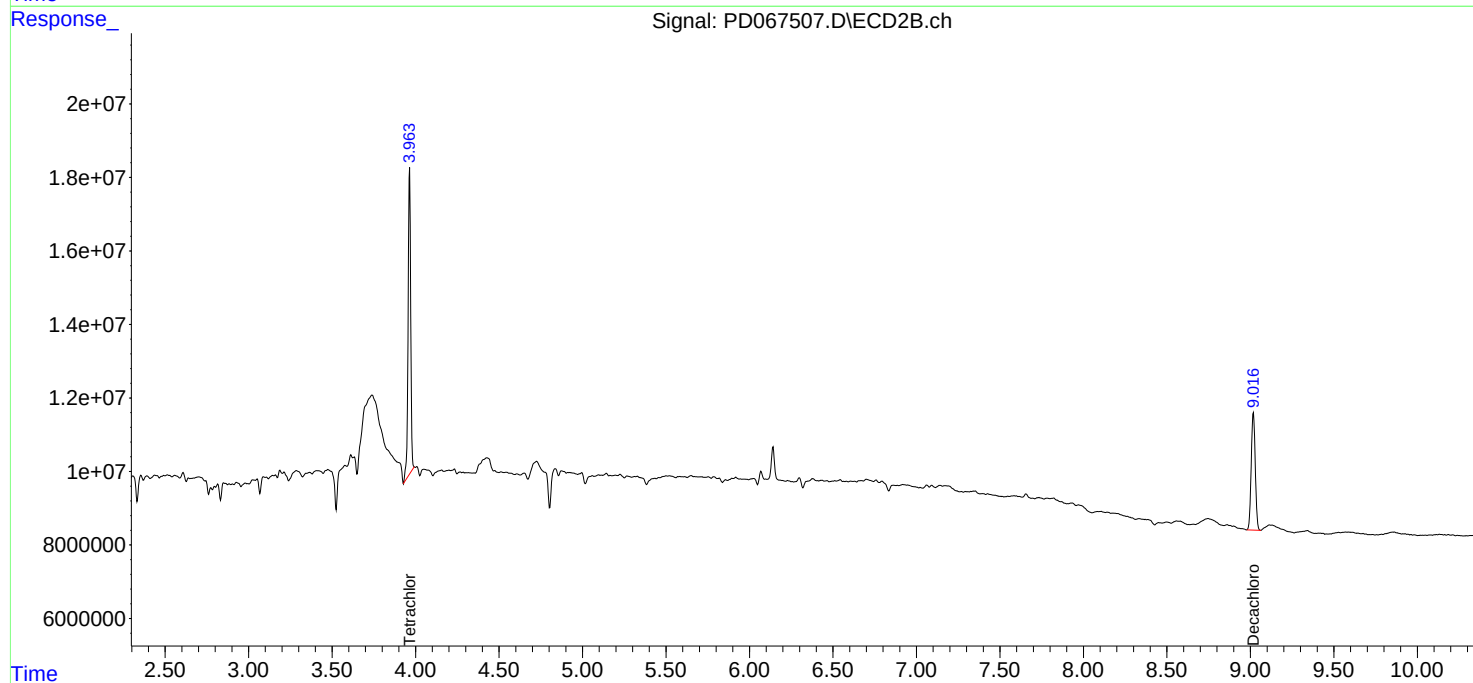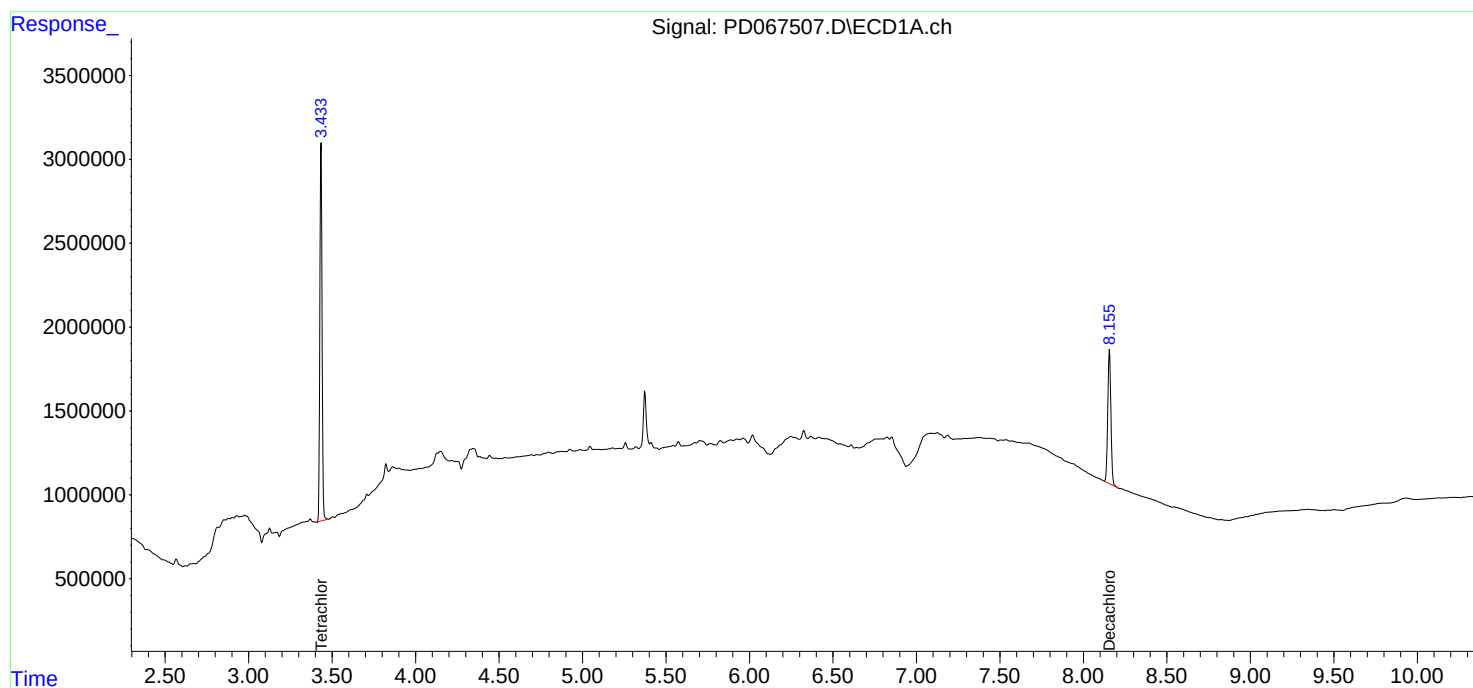

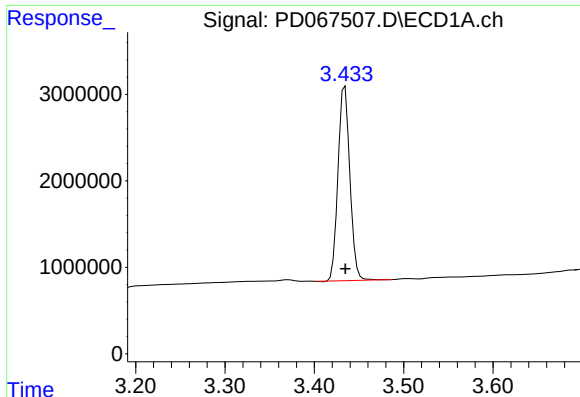

#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 20744994
Conc: 11.34 ng/ml


Instrument :

ECD_D

ClientSampleId :
124027


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
Supervised By :mohammad ahmed 12/29/2021

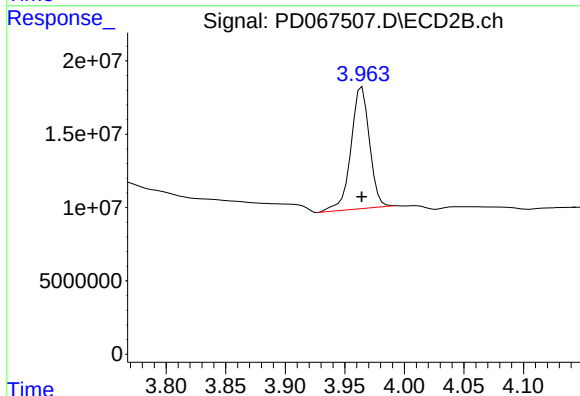


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.001 min
Response: 89662769
Conc: 10.16 ng/ml m

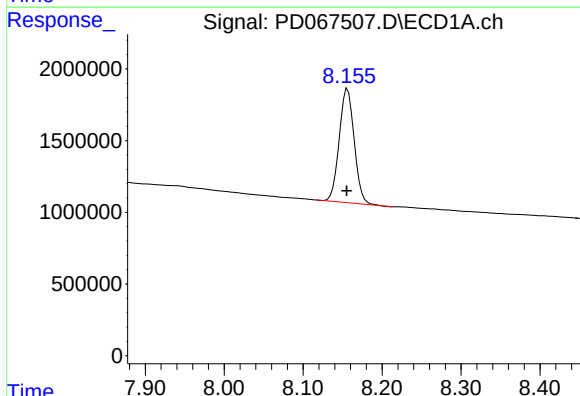

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.001 min
Response: 10436681
Conc: 11.32 ng/ml

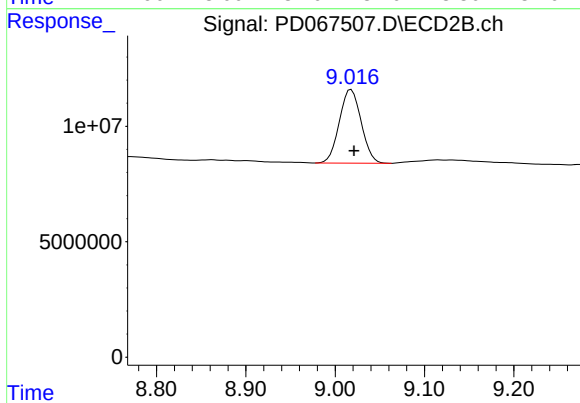

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: -0.003 min
Response: 54116424
Conc: 12.17 ng/ml