

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
 Data File : PD067508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 12:03
 Operator : AR\AJ
 Sample : M5210-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 R206

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
 Supervised By :mohammad ahmed 12/29/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:07:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 04:06:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.434	3.964	20411387	83100624	11.157	9.418
2) SA Decachlor...	8.156	9.016	8294075	41948993	8.997	9.437m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122721\
Data File : PD067508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 12:03
Operator : AR\AJ
Sample : M5210-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
R206


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
Supervised By :mohammad ahmed 12/29/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:07:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 04:06:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

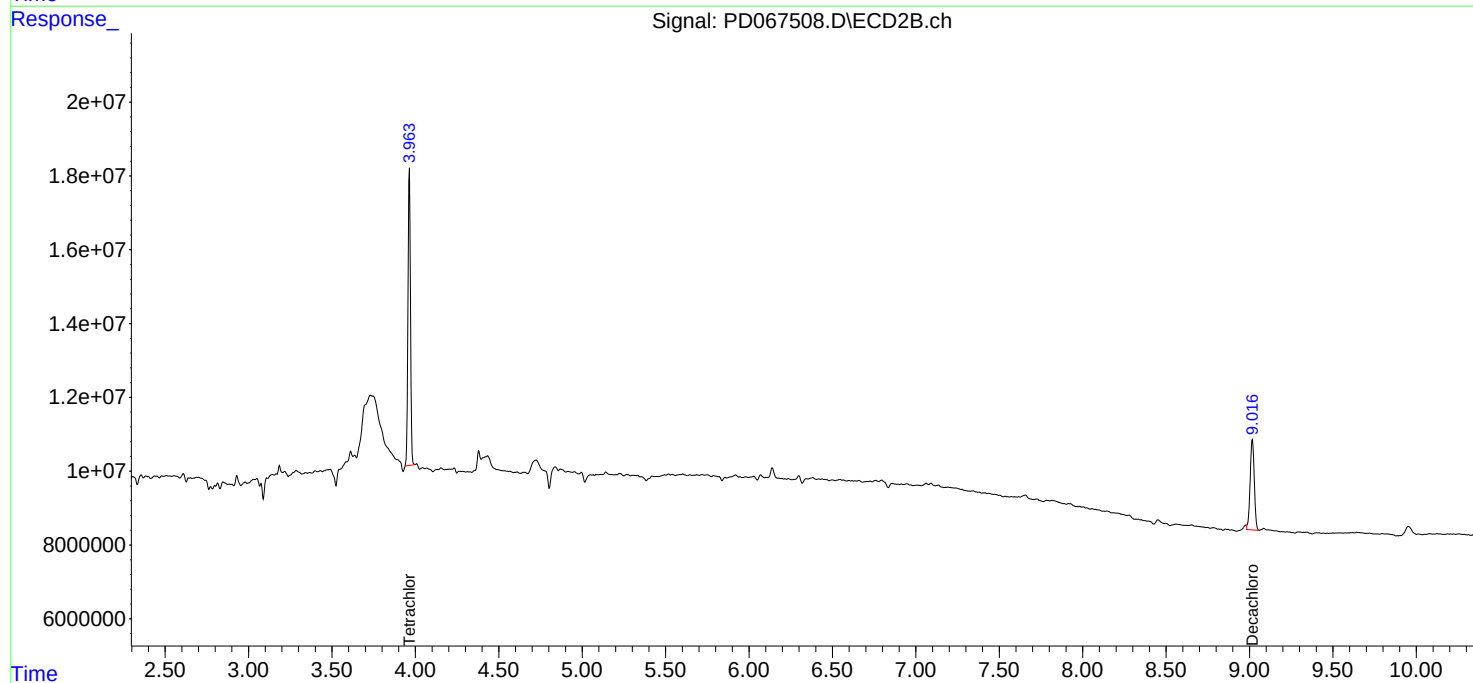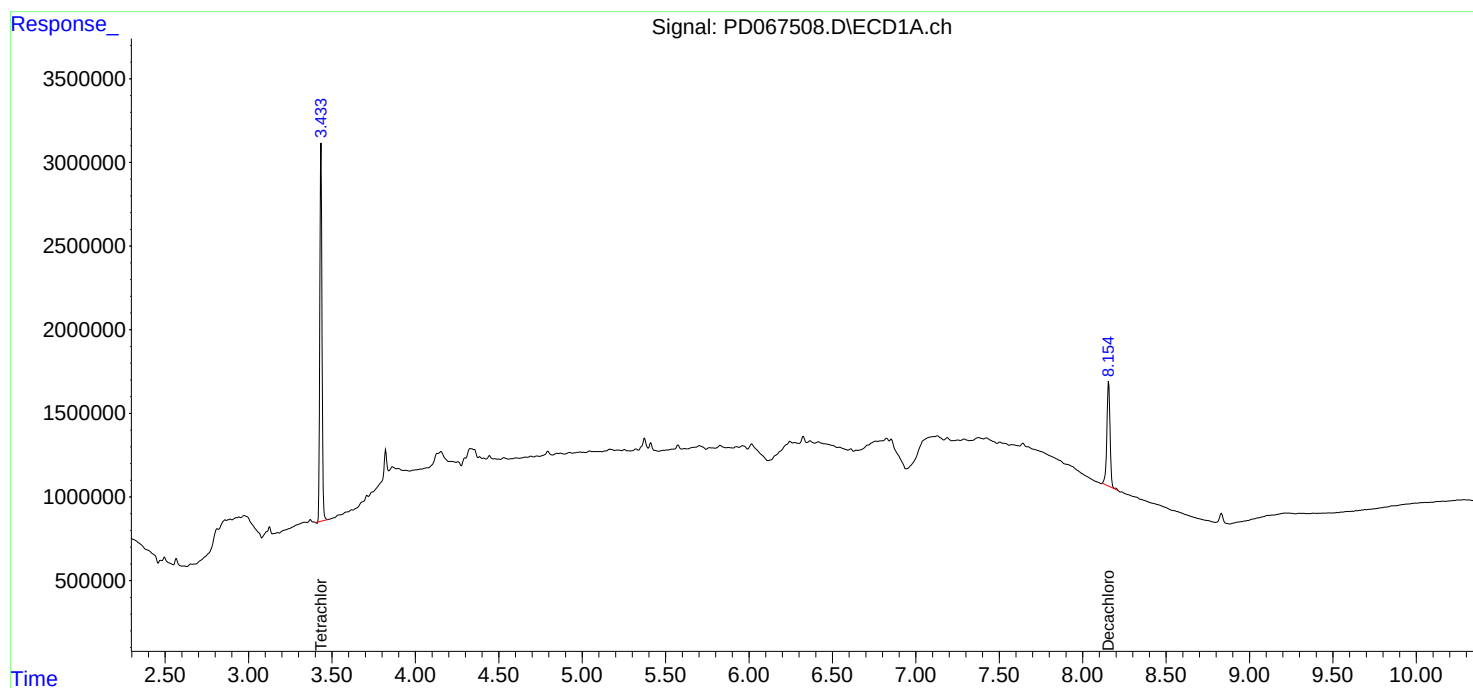

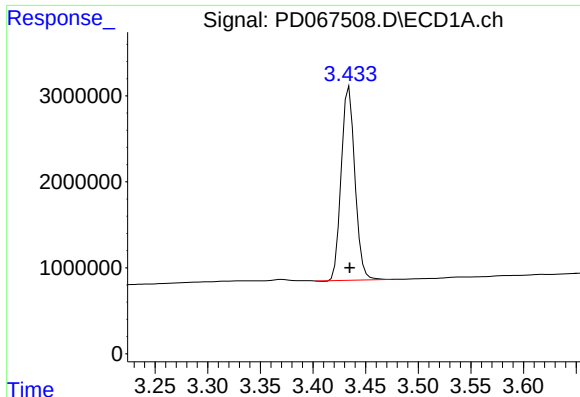


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 20411387
Conc: 11.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
R206


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/28/2021
Supervised By :mohammad ahmed 12/29/2021

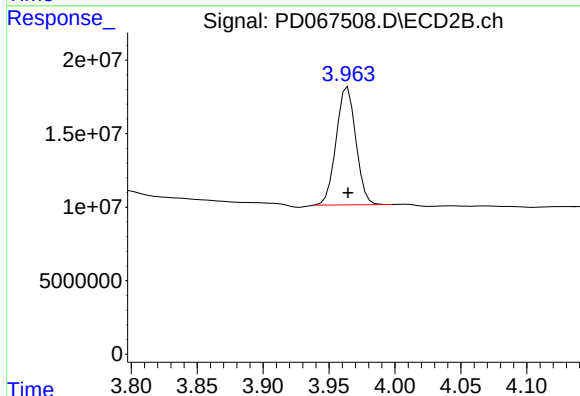


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 83100624
Conc: 9.42 ng/ml

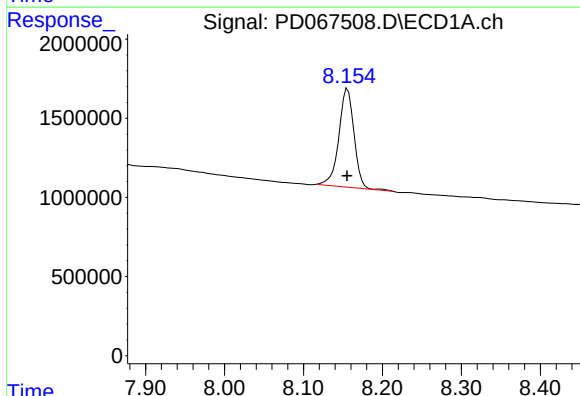

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.000 min
Response: 8294075
Conc: 9.00 ng/ml

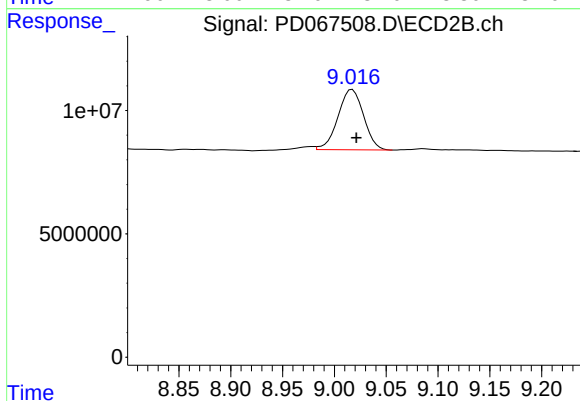

#28 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.005 min
Response: 41948993
Conc: 9.44 ng/ml m