

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122722\
 Data File : PD073490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 12:55
 Operator : AR\AJ
 Sample : TOXAPH501
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 13:25:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122722CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 27 13:24:47 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.693	3.454	191.9E6	4928.5E6	79.433	76.876
27)	SA Decachlor...	7.818	8.900	397.0E6	2509.6E6	159.772	156.144
Target Compounds							
22)	Toxaphene-1	5.237	5.760	122.8E6	911.2E6	7607.588	7409.242
23)	Toxaphene-2	5.596	6.137	142.1E6	1786.6E6	8545.959	7720.451
24)	Toxaphene-3	5.881	6.959	196.8E6	4732.5E6	8427.302	8244.261
25)	Toxaphene-4	6.640	7.049	877.9E6	3991.1E6	8737.723	8329.063
26)	Toxaphene-5	6.950	7.476	502.7E6	2539.5E6	8868.746	8315.654

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122722\
Data File : PD073490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 12:55
Operator : AR\AJ
Sample : TOXAPH501
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 13:25:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122722CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 27 13:24:47 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

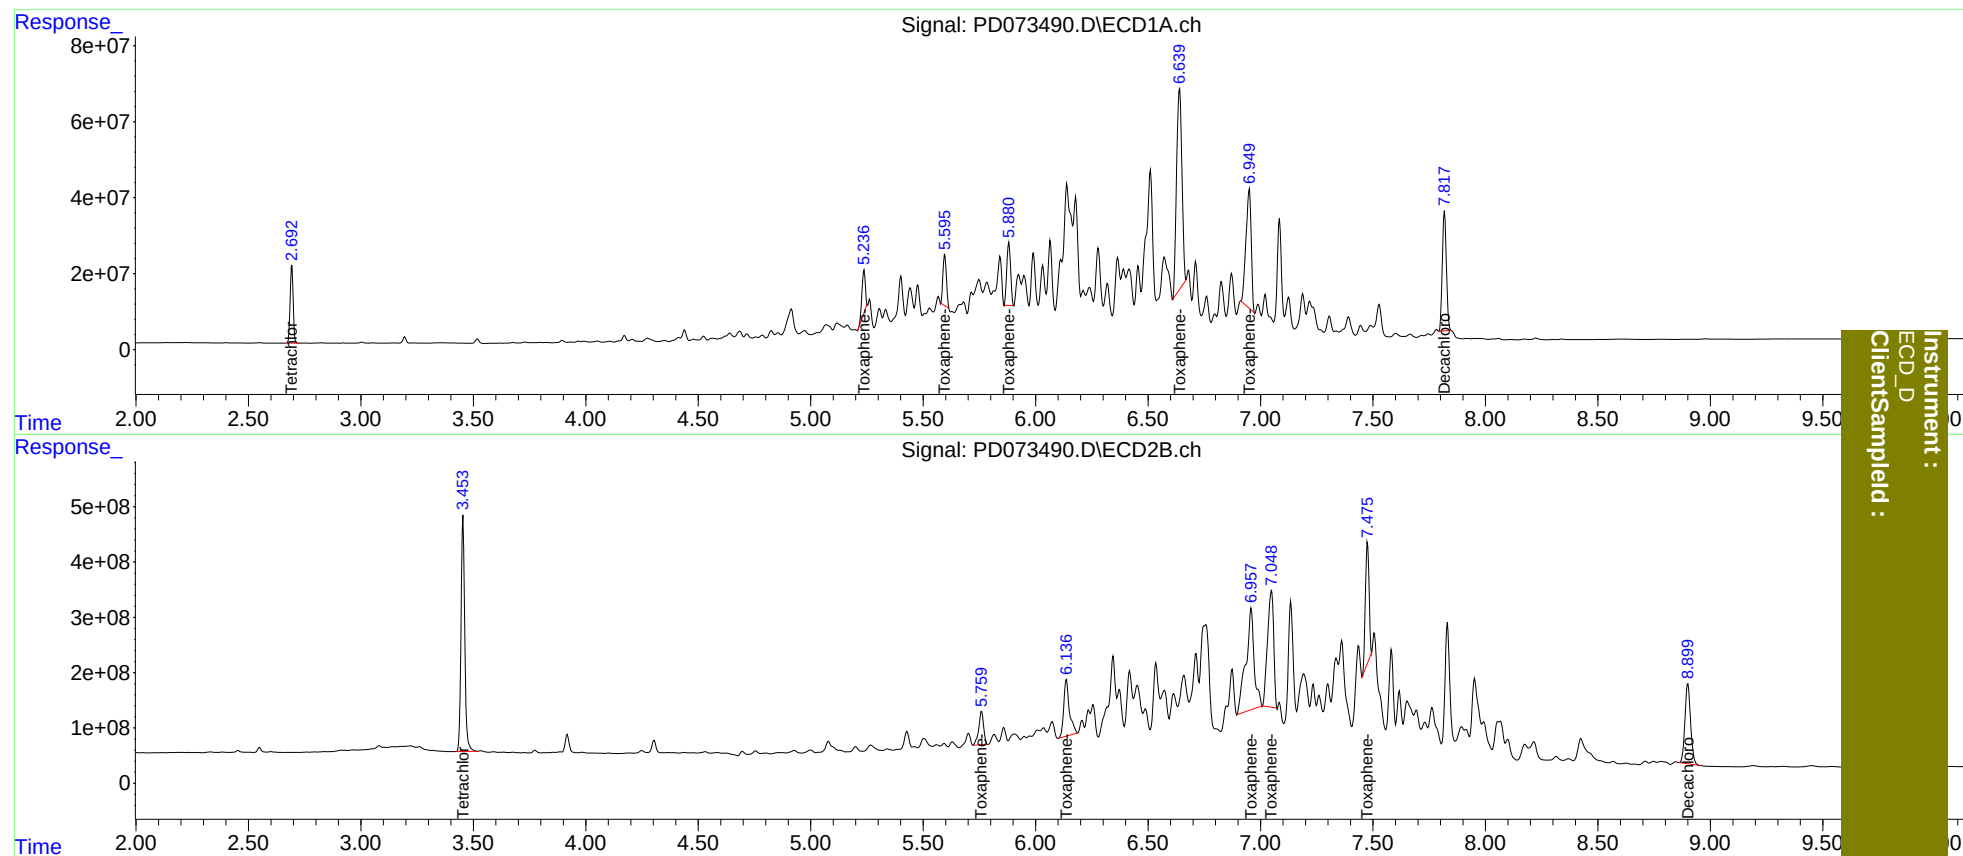

Instrument :
ECD_D
ClientSampled :
0