

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122722\
 Data File : PD073497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 14:29
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 02:52:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 28 02:49:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.693	3.455	101.5E6	2677.0E6	40.213	39.984
27)	SA Decachlor...	7.818	8.901	230.4E6	1415.1E6	80.453	81.131
Target Compounds							
2)	A alpha-BHC	3.195	3.918	168.7E6	3289.1E6	40.452	39.786
3)	MA gamma-BHC...	3.526	4.251	141.1E6	2535.7E6	40.424	40.008
4)	MA Heptachlor	3.857	4.817	150.1E6	1828.7E6	40.542	40.354
9)	A Endosulfan I	5.009	5.972	129.5E6	1343.4E6	40.483	40.317
13)	MA Dieldrin	5.275	6.248	294.6E6	2900.7E6	81.385	80.588
14)	MA Endrin	5.551	6.480	256.9E6	2358.2E6	81.177	80.578
16)	A 4,4'-DDD	5.698	6.615	229.4E6	2122.6E6	81.177	80.801
17)	MA 4,4'-DDT	5.946	6.922	231.8E6	2091.7E6	81.126	80.952
20)	A Methoxychlor	6.529	7.402	592.0E6	4385.5E6	405.184	408.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122722\
Data File : PD073497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 14:29
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 02:52:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122722CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 28 02:49:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

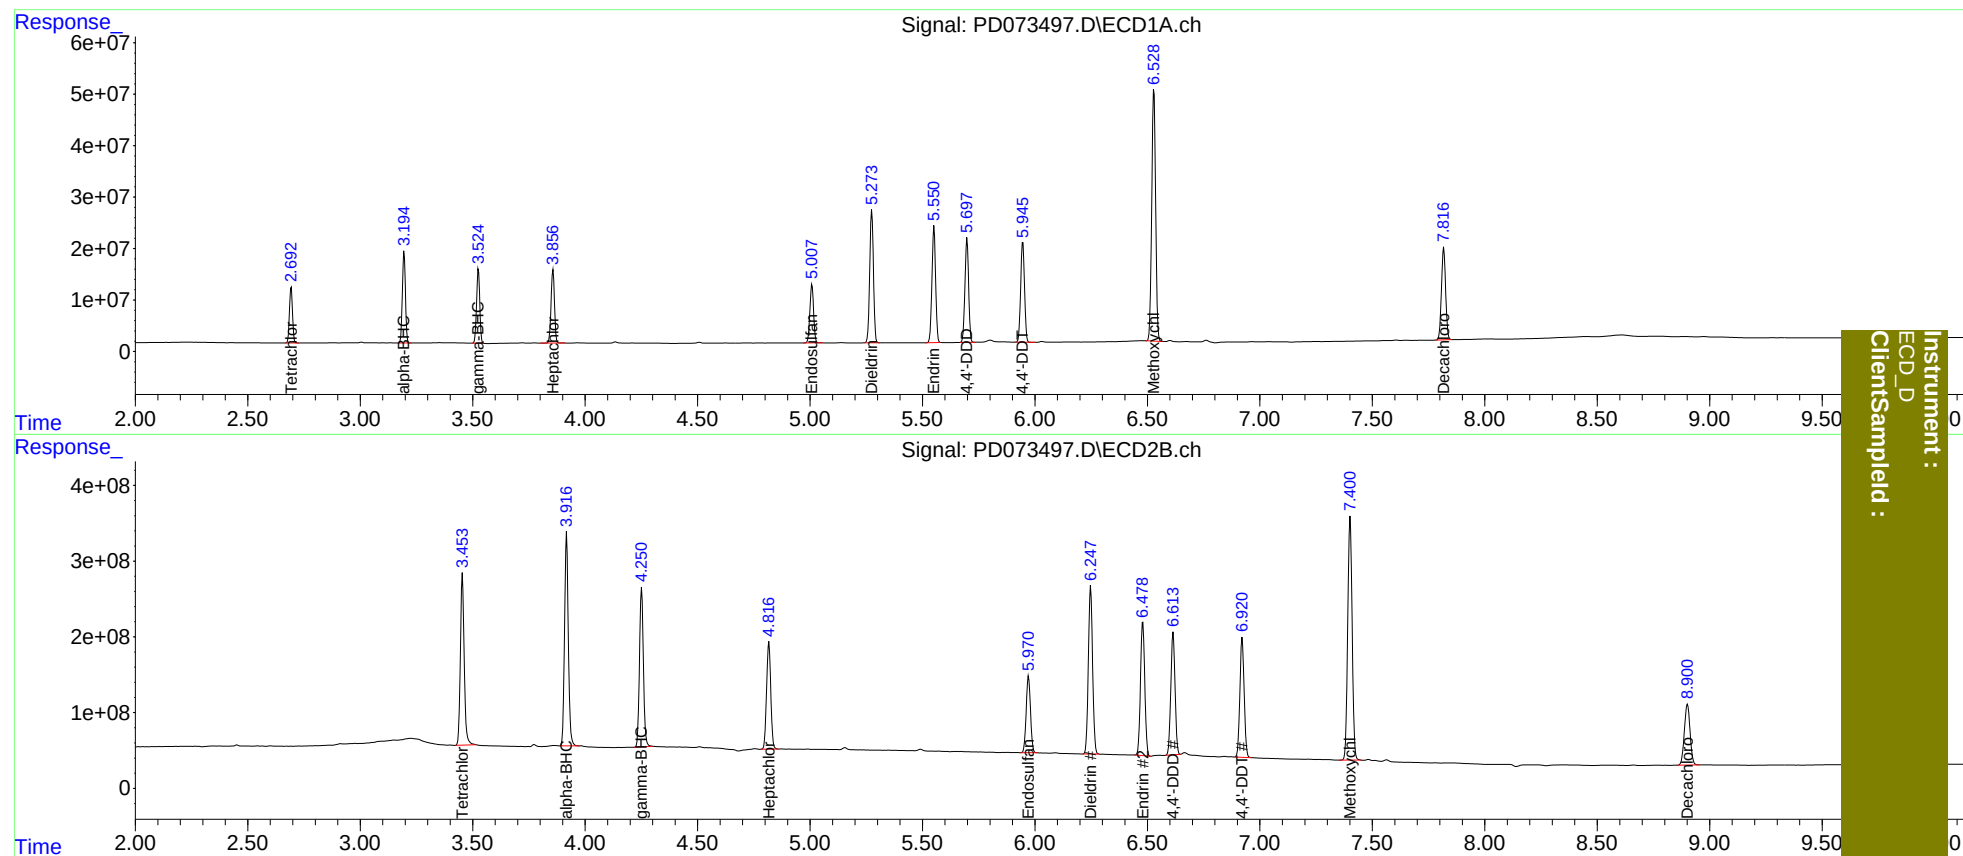

Instrument :
ECD_D
ClientSampled :
0