

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122723\
 Data File : PD080516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 20:20
 Operator : AR\AJ
 Sample : PIBLK141
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 01:45:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.798	27442053	48380434	21.493	21.758
27)	SA Decachlor...	9.111	7.938	42870083	57619017	26.664	24.005
Target Compounds							
2)	A alpha-BHC	0.000	3.287	0	110468	N.D.	<MDL
4)	MA Heptachlor	0.000	3.934f	0	142045	N.D.	<MDL
5)	MB Aldrin	0.000	4.273	0	215569	N.D.	<MDL
6)	B beta-BHC	0.000	3.934	0	142045	N.D.	<MDL
8)	B Heptachlo...	0.000	4.780	0	147890	N.D.	<MDL
14)	MA Endrin	0.000	5.679	0	268749	N.D.	0.102
15)	B Endosulfa...	0.000	5.917f	0	269941	N.D.	<MDL
18)	B Endrin al...	0.000	6.155	0	237338	N.D.	0.103


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122723\
Data File : PD080516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 20:20
Operator : AR\AJ
Sample : PIBLK141
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 01:45:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

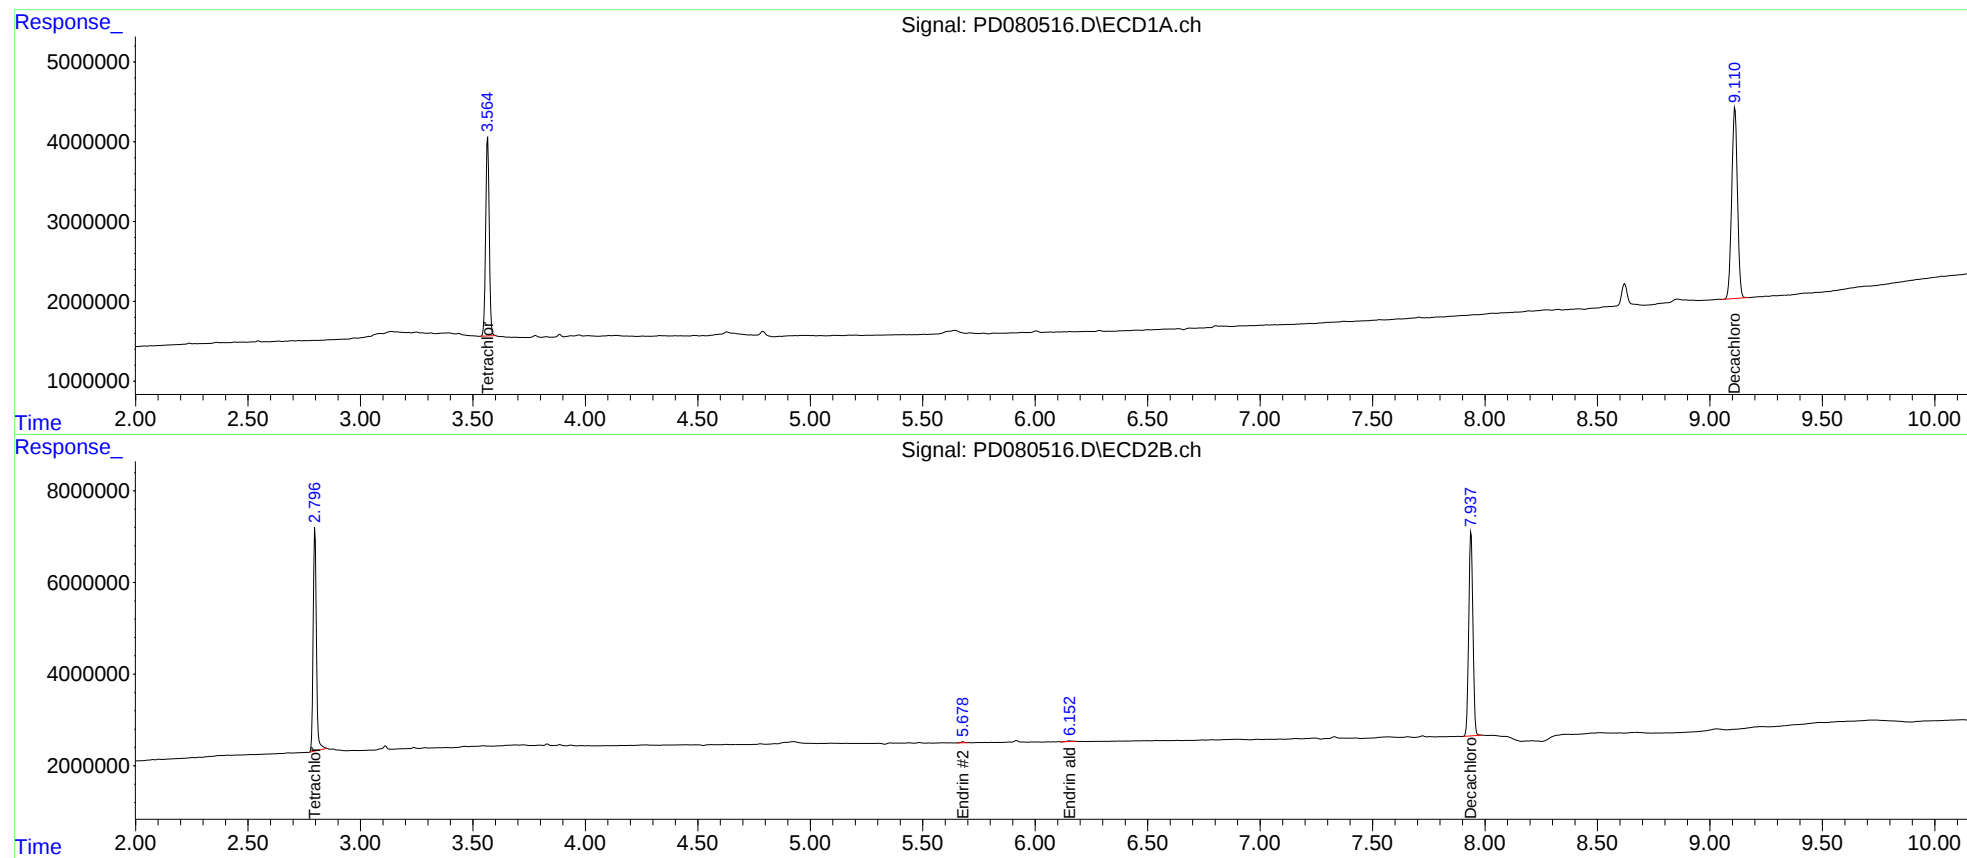

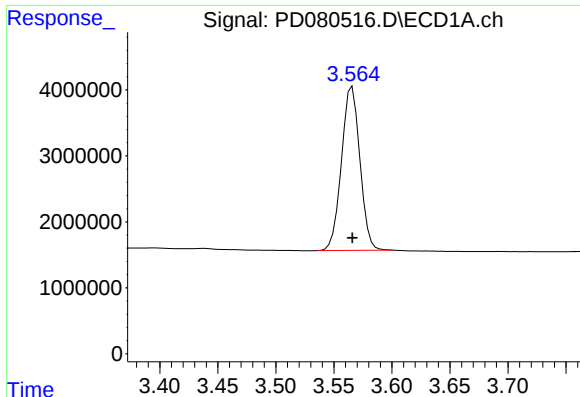


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 27442053
Conc: 21.49 ng/ml

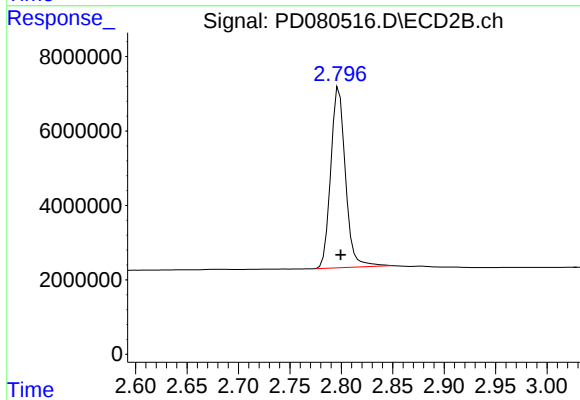


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: -0.002 min
Response: 48380434
Conc: 21.76 ng/ml

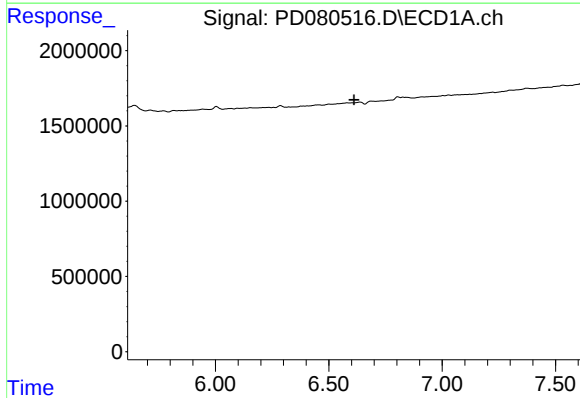


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

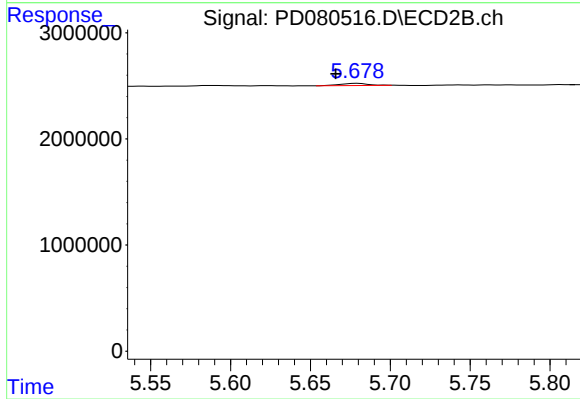


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.013 min
Response: 268749
Conc: 0.10 ng/ml

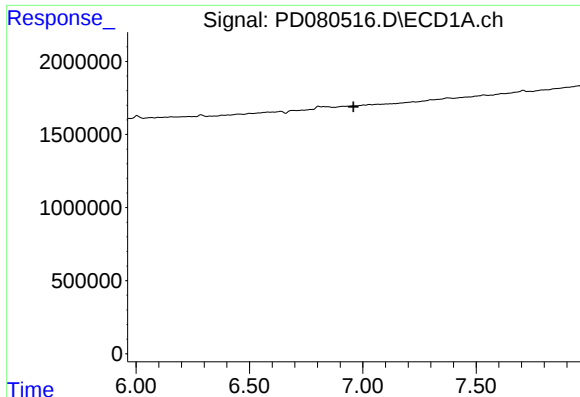


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

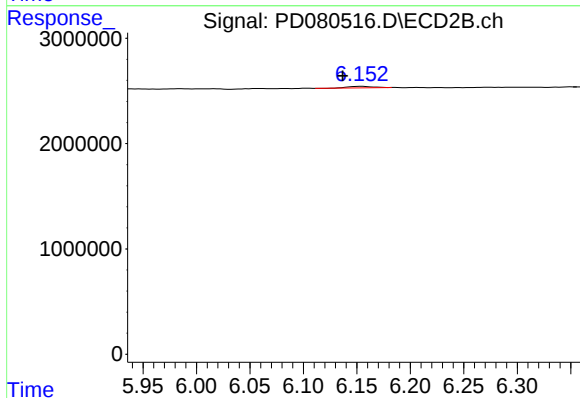


#18 Endrin aldehyde

R.T.: 6.155 min
Delta R.T.: 0.018 min
Response: 237338
Conc: 0.10 ng/ml

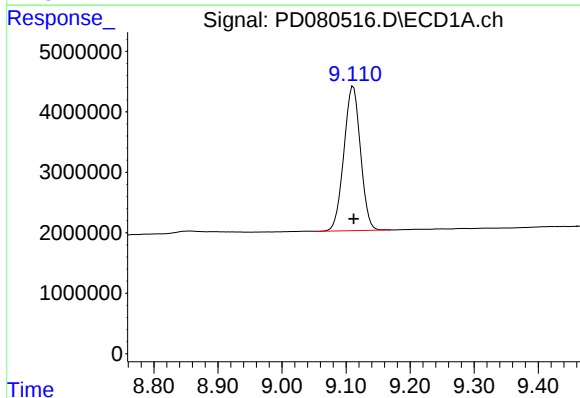

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 42870083
Conc: 26.66 ng/ml

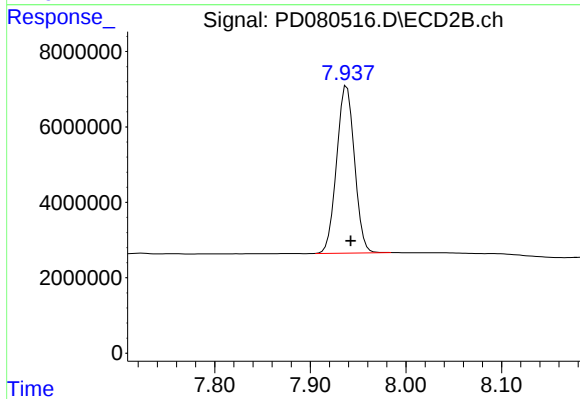

#27 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.004 min
Response: 57619017
Conc: 24.01 ng/ml