

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:29
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:30:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:29:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.964	108.3E6	324.0E6	50.000	50.000
28)	SA Decachlor...	8.157	9.019	42997468	231.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.295	4.953	40640126	136.0E6	500.000	500.000
24)	Chlordane-2	4.792	5.422	45099588	137.3E6	500.000	500.000
25)	Chlordane-3	5.354	6.068	135.6E6	479.1E6	500.000	500.000
26)	Chlordane-4	5.412	6.141	111.6E6	564.3E6	500.000	500.000
27)	Chlordane-5	6.245	6.950	42584496	115.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:29
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:30:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:29:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

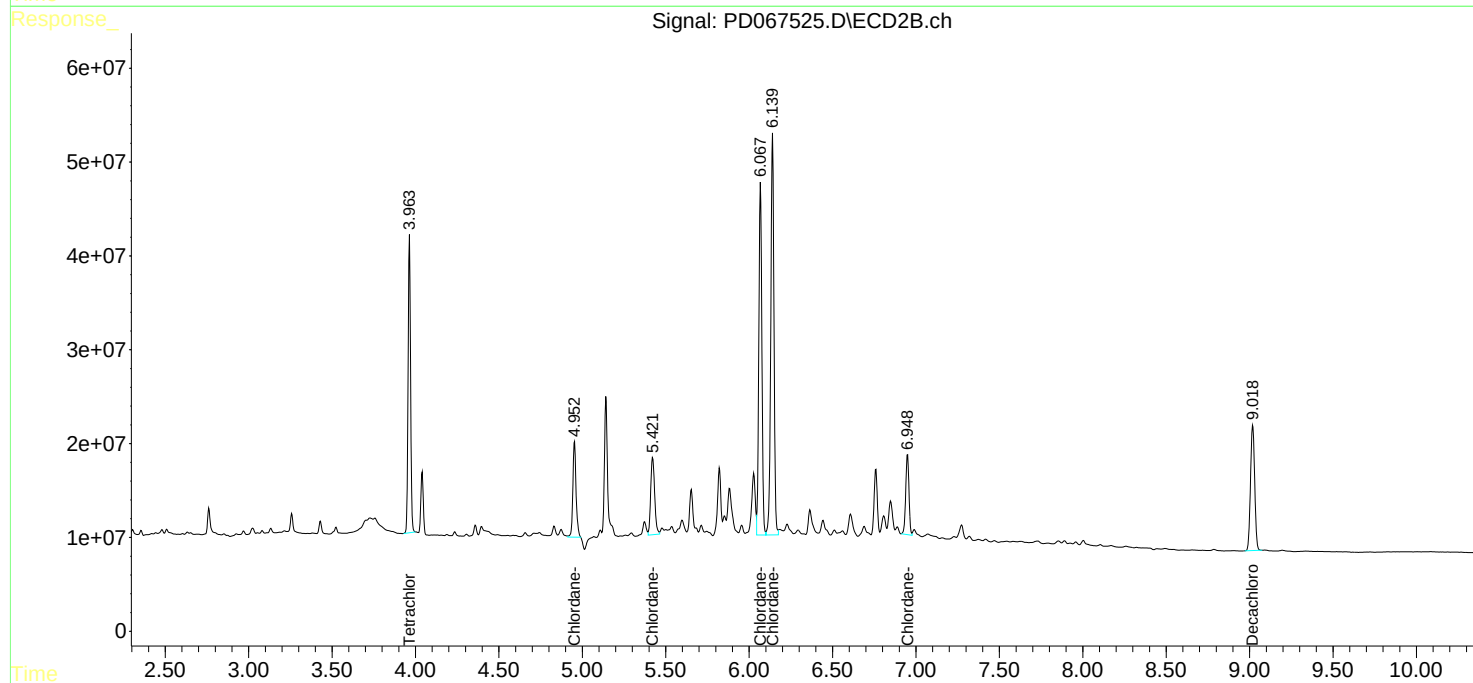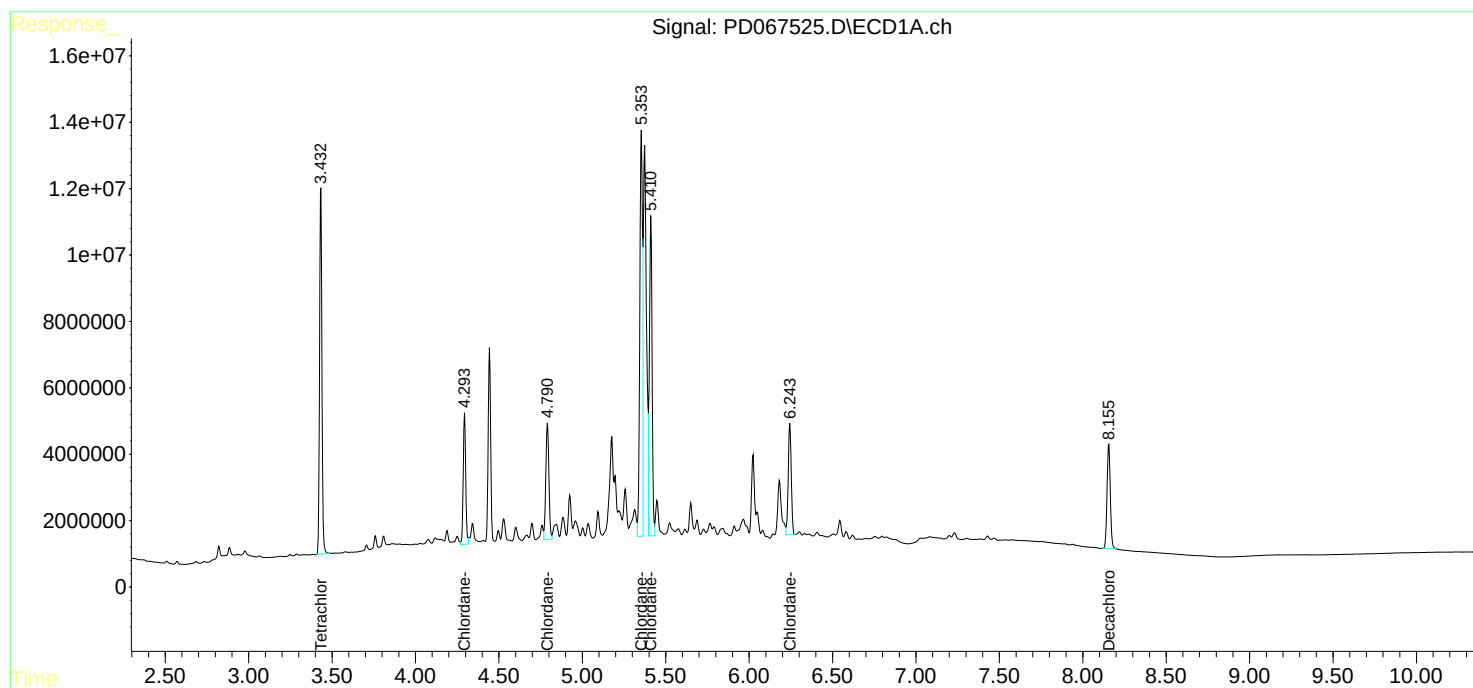


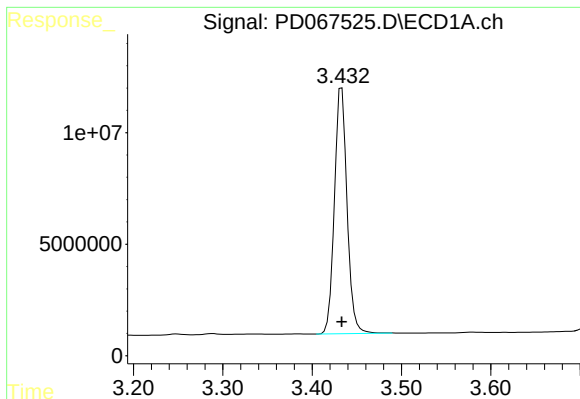

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 108316376
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

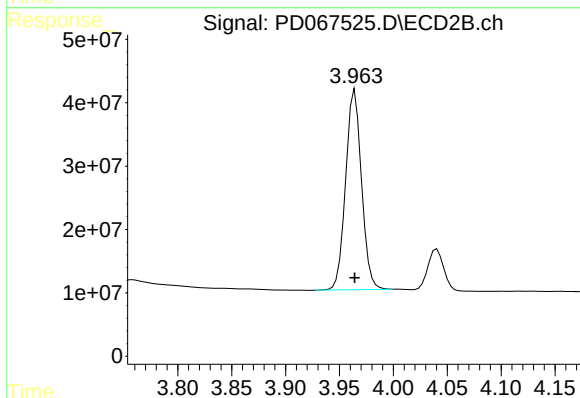


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 323988568
Conc: 50.00 ng/ml

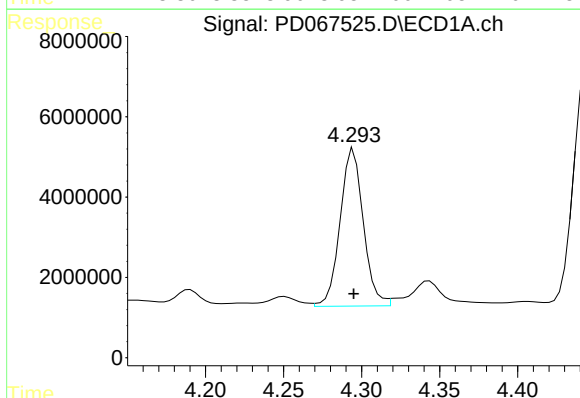


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.000 min
Response: 40640126
Conc: 500.00 ng/ml

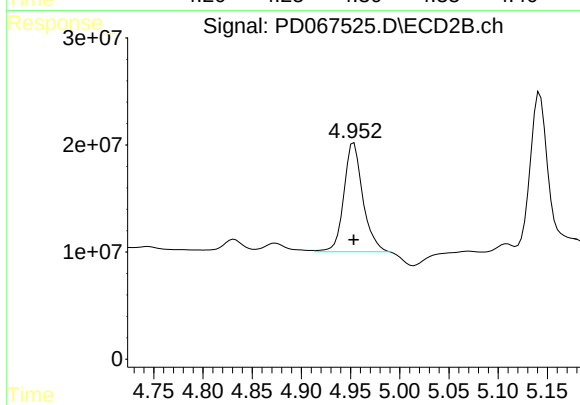

#23 Chlordane-1


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 136023032
Conc: 500.00 ng/ml

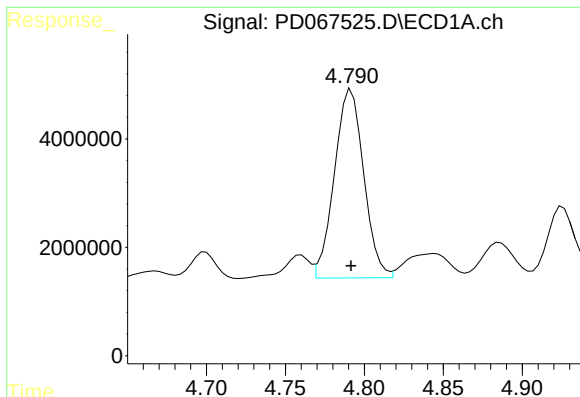

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 45099588
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

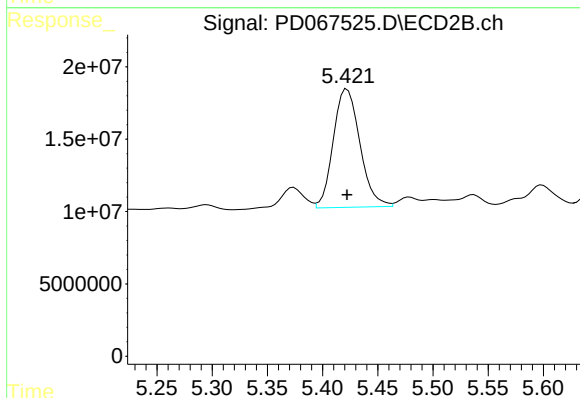


#24 Chlordane-2

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 137339157
Conc: 500.00 ng/ml

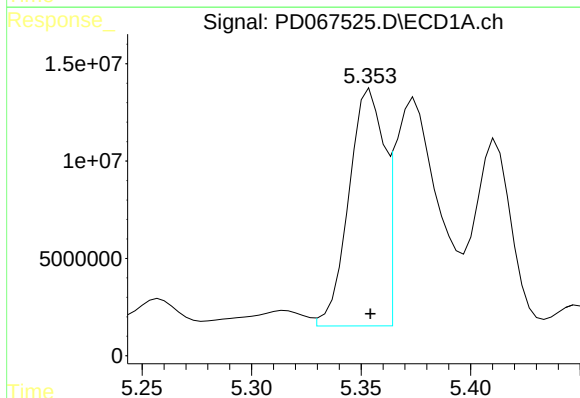


#25 Chlordane-3

R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 135610619
Conc: 500.00 ng/ml

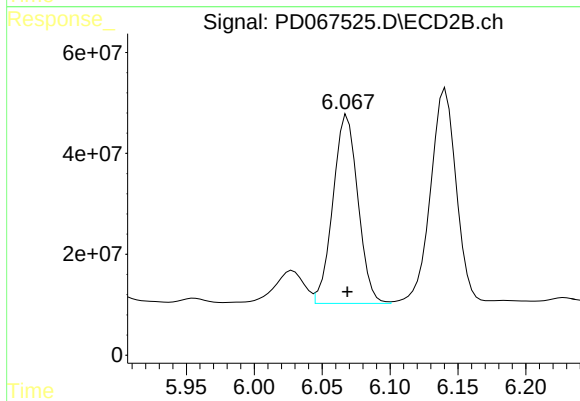

#25 Chlordane-3


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 479145638
Conc: 500.00 ng/ml

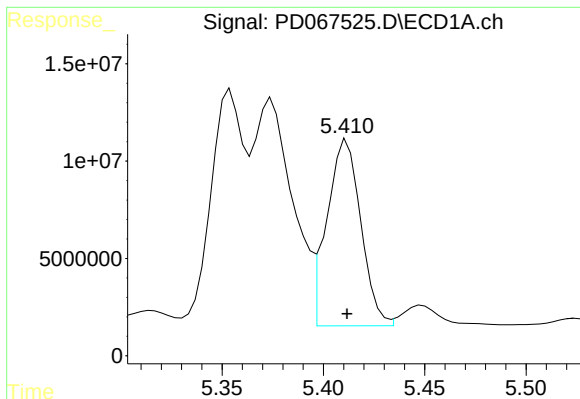

#26 Chlordane-4


R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 111611287
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

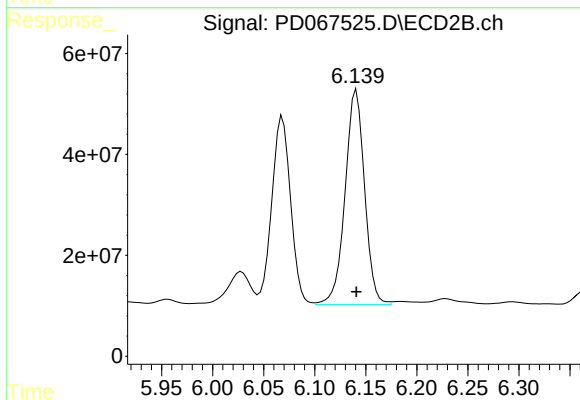


#26 Chlordane-4

R.T.: 6.141 min
Delta R.T.: 0.000 min
Response: 564250350
Conc: 500.00 ng/ml

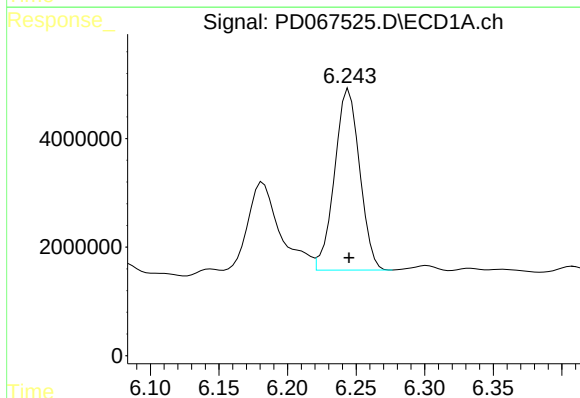


#27 Chlordane-5

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 42584496
Conc: 500.00 ng/ml

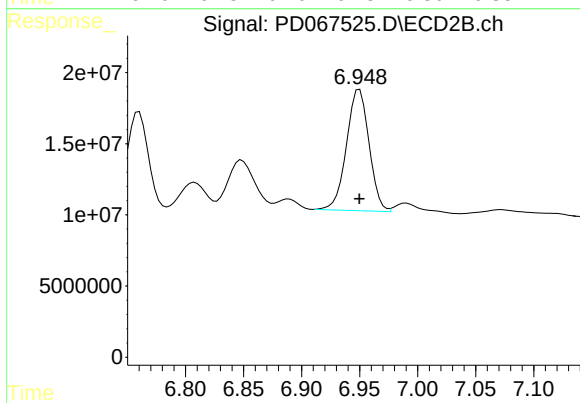

#27 Chlordane-5


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 115150524
Conc: 500.00 ng/ml

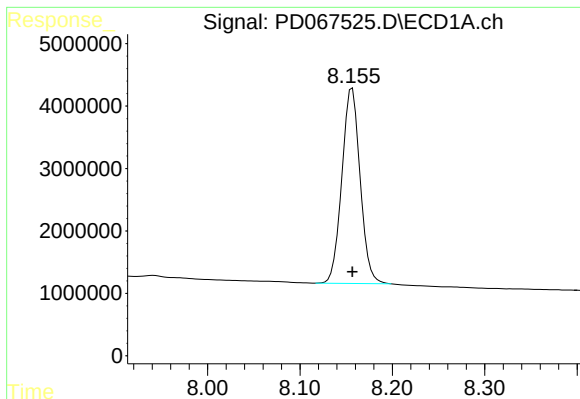

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 42997468
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

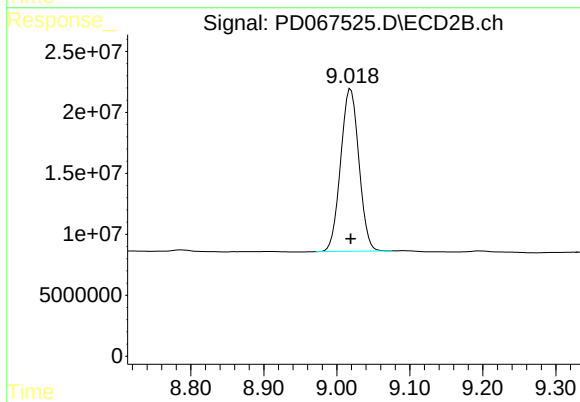

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 231503170
Conc: 50.00 ng/ml