

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:56
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:40:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:29:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.964	10214659	36821629	4.774	5.595
28)	SA Decachlor...	8.157	9.019	5793639	29373744	6.381	6.083
Target Compounds							
23)	Chlordane-1	4.294	4.954	5906169	19047220	74.250	71.161
24)	Chlordane-2	4.791	5.422	5753770	16149548	63.540	59.142
25)	Chlordane-3	5.354	6.069	13665140	58669942	51.490	61.020
26)	Chlordane-4	5.411	6.140	12067636	71490652	55.346	62.826
27)	Chlordane-5	6.245	6.949	5637379	10098941	65.359	45.361 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:56
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:40:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:29:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

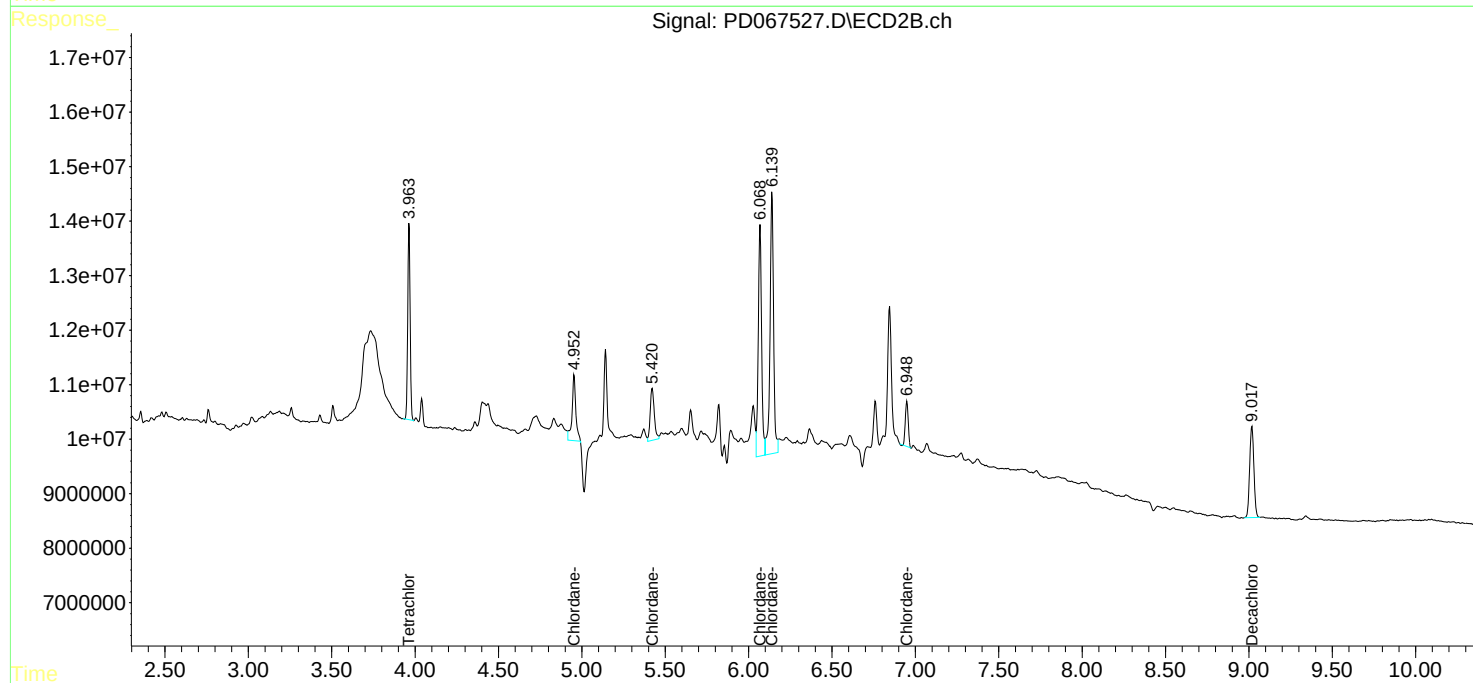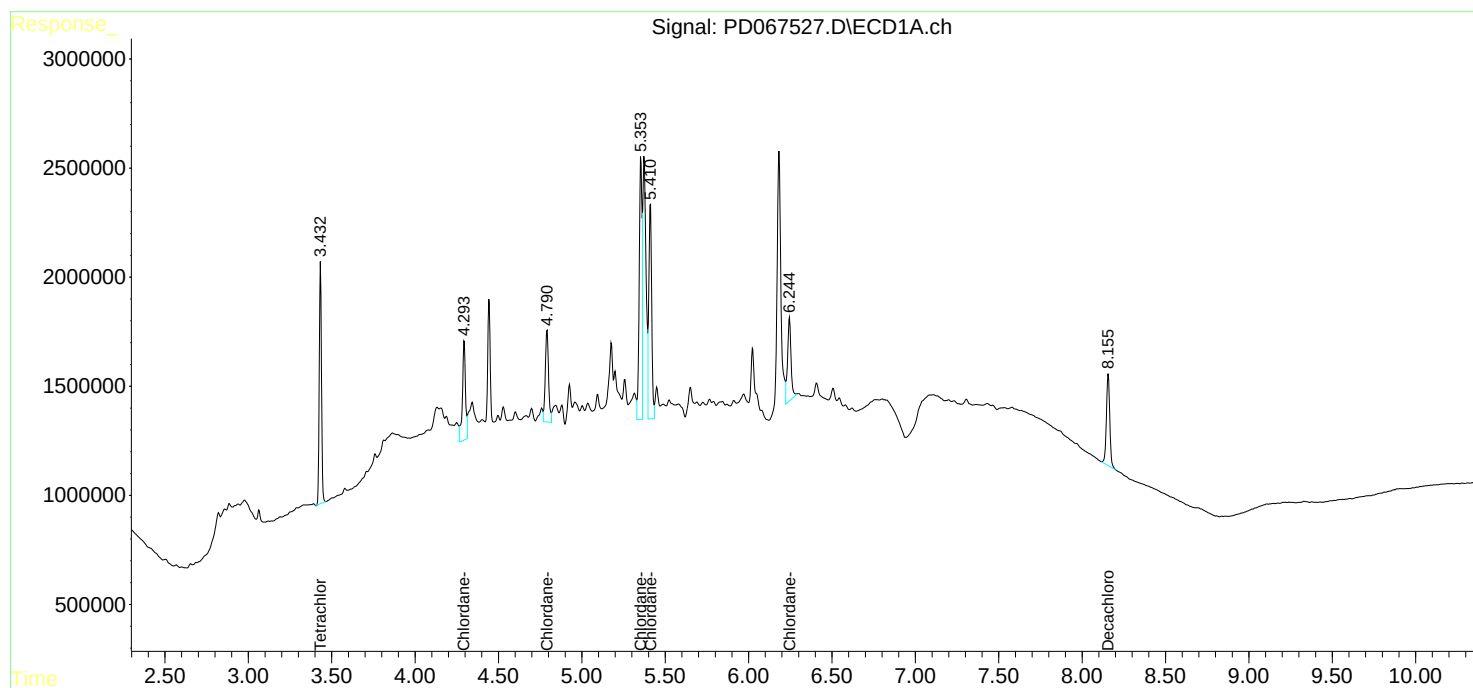


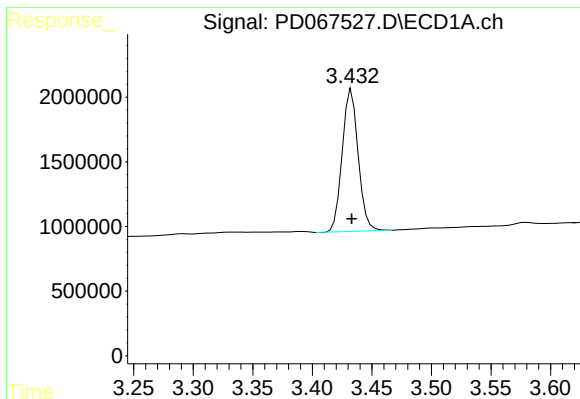

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 10214659
Conc: 4.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

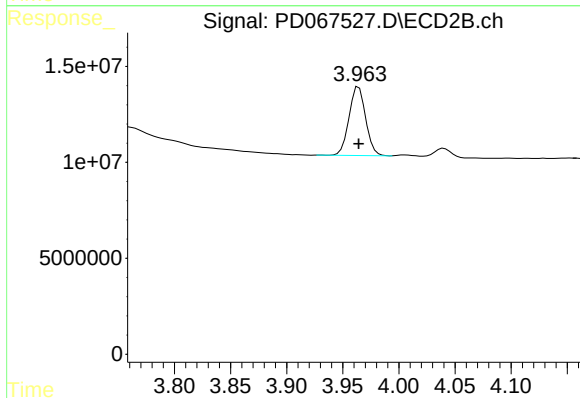


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 36821629
Conc: 5.60 ng/ml

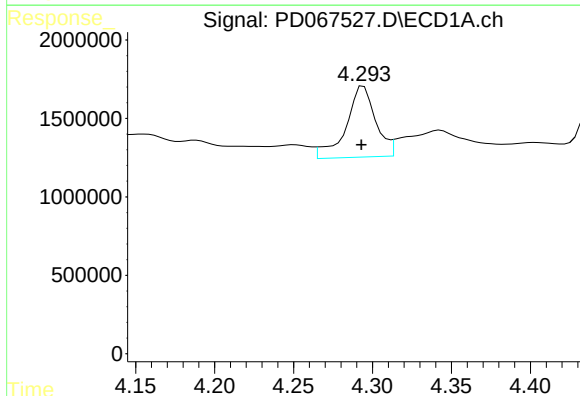


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: 0.001 min
Response: 5906169
Conc: 74.25 ng/ml

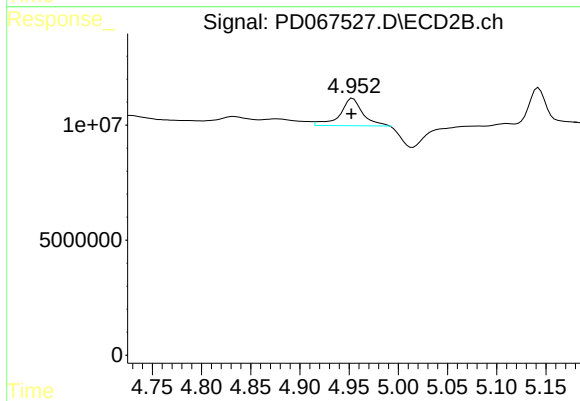

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.001 min
Response: 19047220
Conc: 71.16 ng/ml

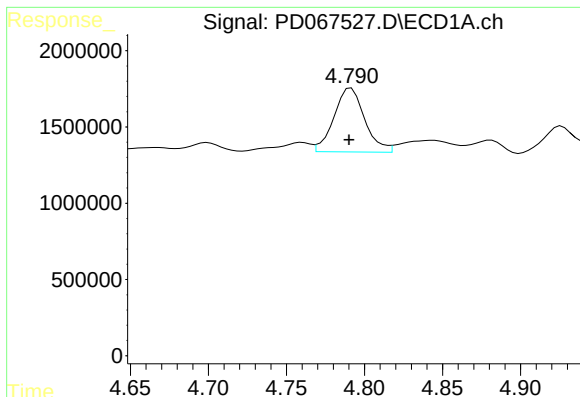

#24 Chlordane-2


R.T.: 4.791 min
Delta R.T.: 0.001 min
Response: 5753770
Conc: 63.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

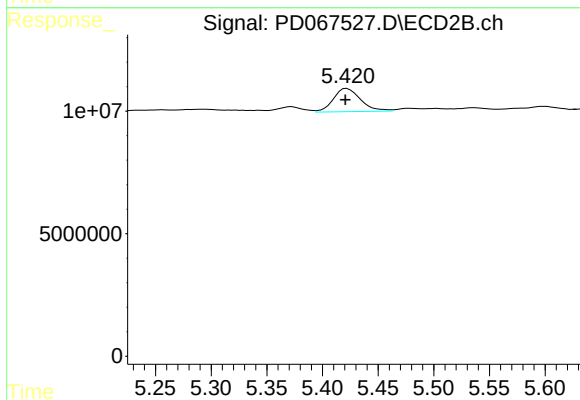


#24 Chlordane-2

R.T.: 5.422 min
Delta R.T.: 0.001 min
Response: 16149548
Conc: 59.14 ng/ml

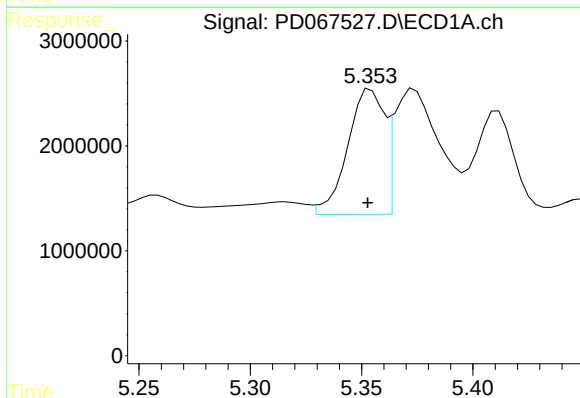


#25 Chlordane-3

R.T.: 5.354 min
Delta R.T.: 0.002 min
Response: 13665140
Conc: 51.49 ng/ml

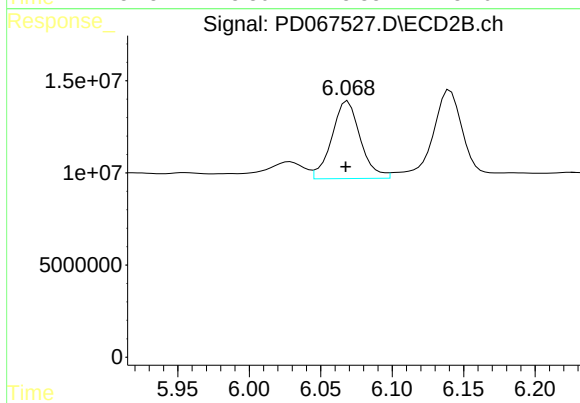

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: 0.001 min
Response: 58669942
Conc: 61.02 ng/ml

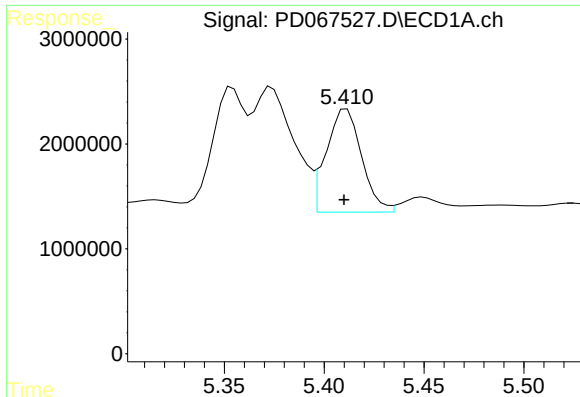

#26 Chlordane-4


R.T.: 5.411 min
Delta R.T.: 0.001 min
Response: 12067636
Conc: 55.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

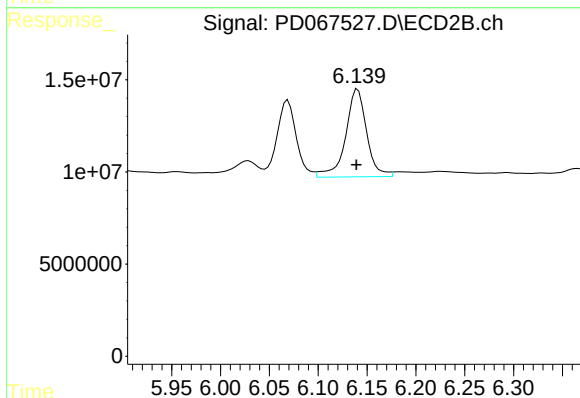


#26 Chlordane-4

R.T.: 6.140 min
Delta R.T.: 0.001 min
Response: 71490652
Conc: 62.83 ng/ml

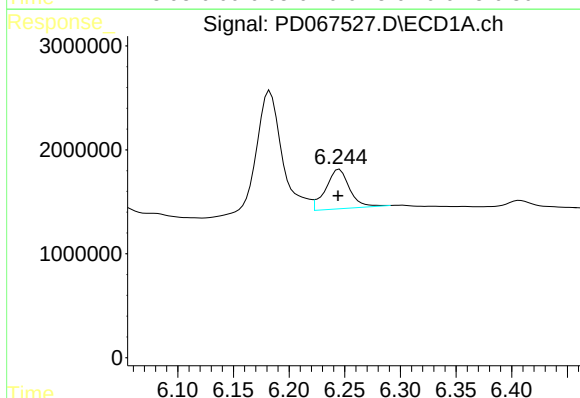


#27 Chlordane-5

R.T.: 6.245 min
Delta R.T.: 0.001 min
Response: 5637379
Conc: 65.36 ng/ml

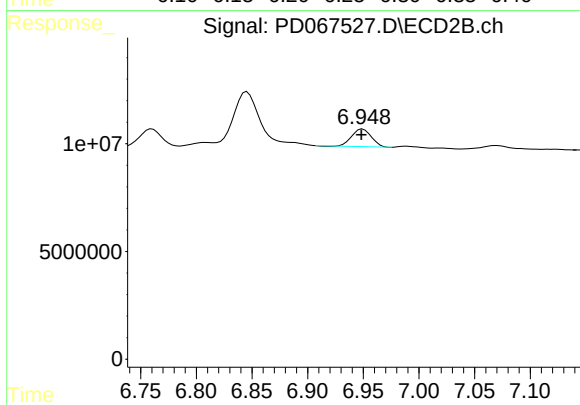

#27 Chlordane-5


R.T.: 6.949 min
Delta R.T.: 0.001 min
Response: 10098941
Conc: 45.36 ng/ml

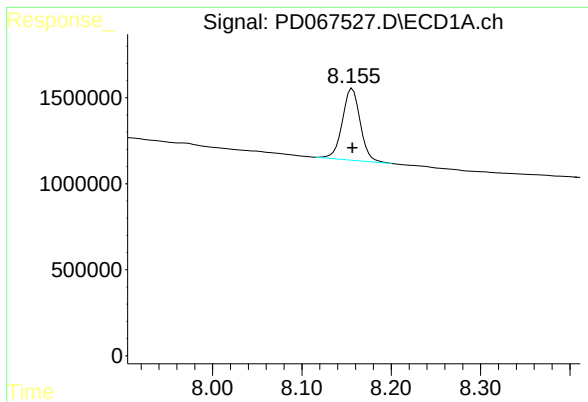

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 5793639
Conc: 6.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

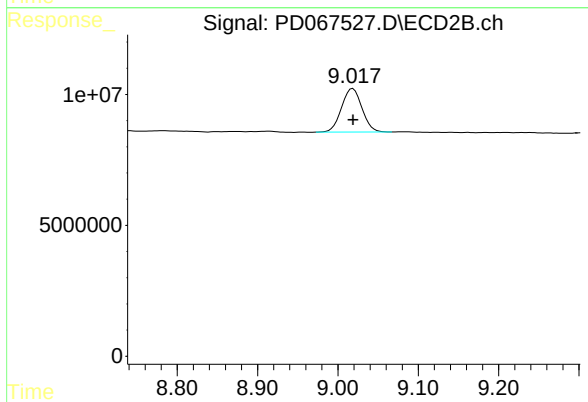

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 29373744
Conc: 6.08 ng/ml