

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 16:38
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 03:08:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	42424483	157.7E6	23.346	23.893
28)	SA Decachlor...	8.157	9.019	20412619	109.4E6	22.980	23.015
Target Compounds							
9)	A Endosulfan I	5.466	6.192	25670655	72644745	11.538	11.999
10)	B gamma-Chl...	5.354	6.069	28599299	74390139	11.568	11.467
12)	B 4,4'-DDE	5.575	6.301	49345334	142.8E6	22.289	23.191
13)	MA Dieldrin	5.708	6.450	52718761	152.6E6	21.836	22.979
19)	B Endosulfa...	6.618	7.232	32690782	112.9E6	20.249	20.654
20)	A Methoxychlor	6.877	7.555	80720539	277.0E6	95.091	95.473
21)	B Endrin ke...	7.110	7.704	36836217	142.0E6	21.524	22.622



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 16:38
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 03:08:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

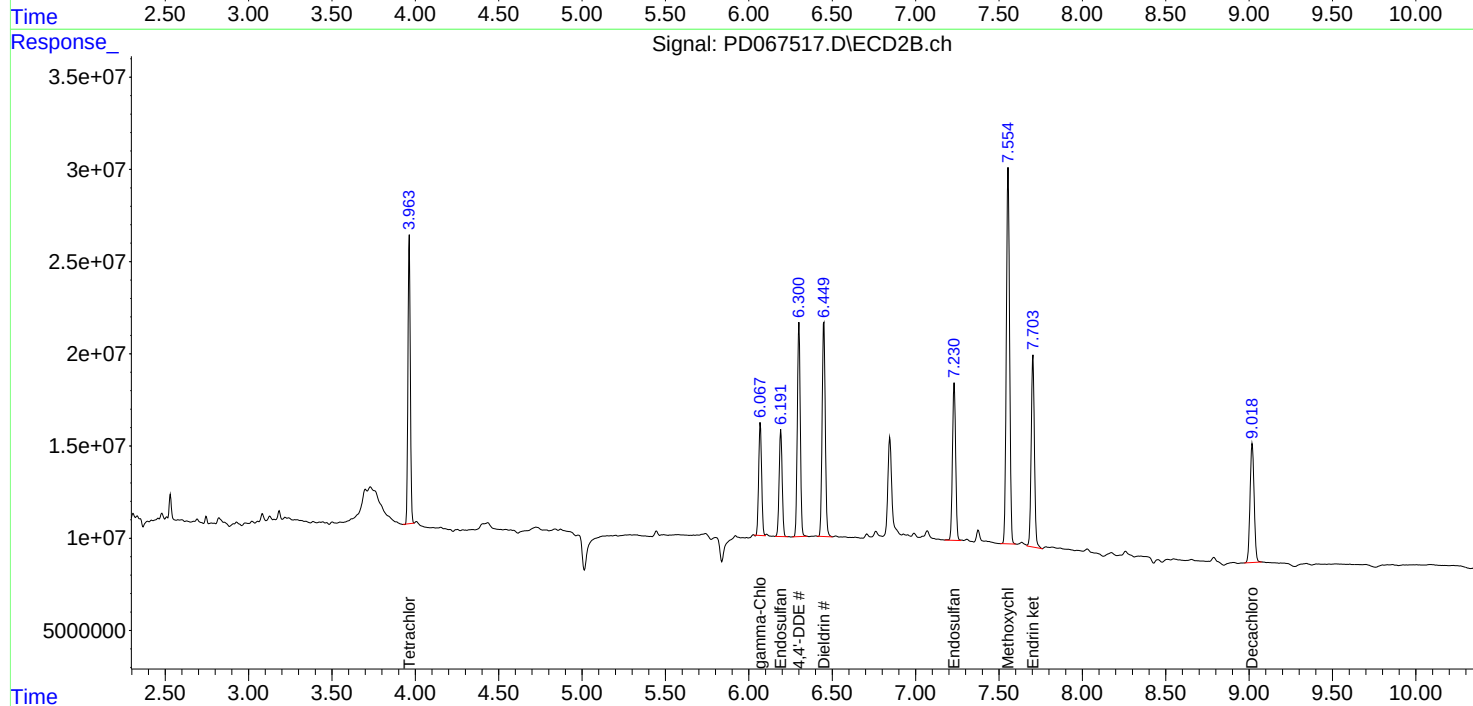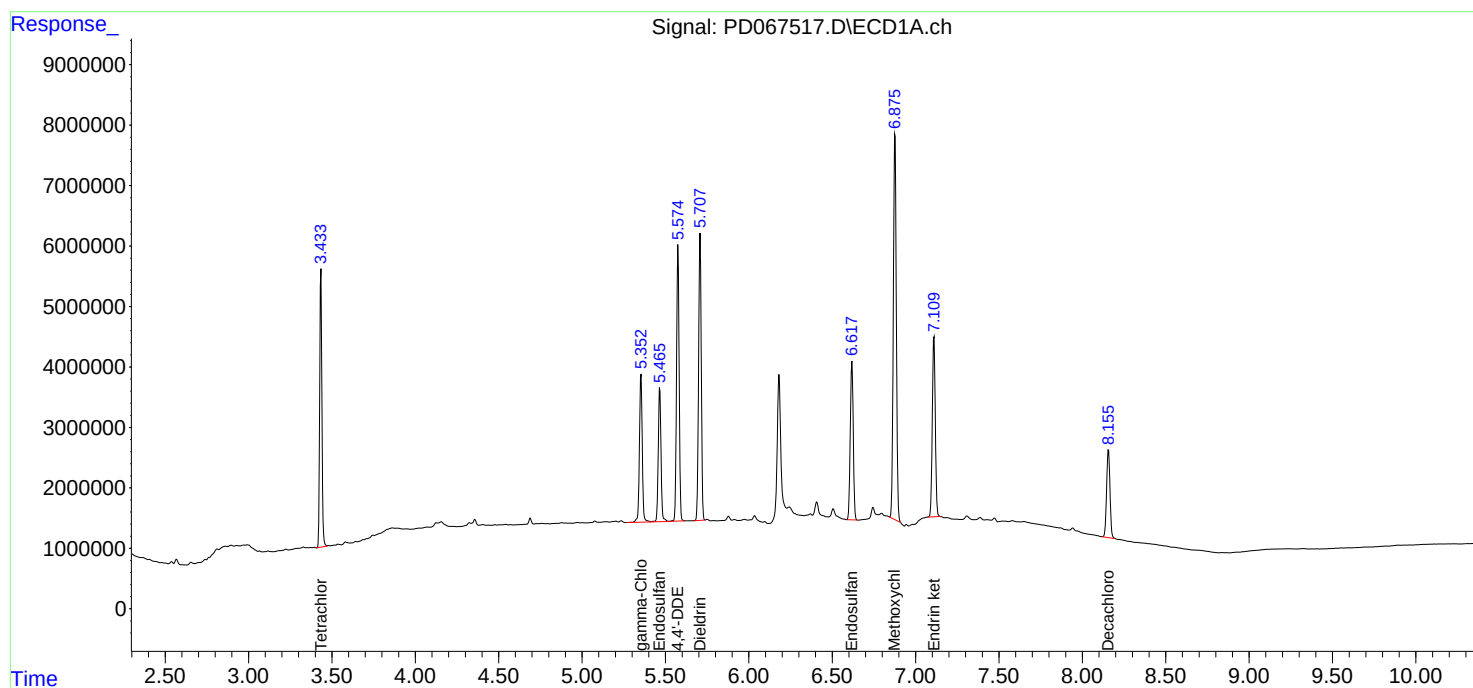


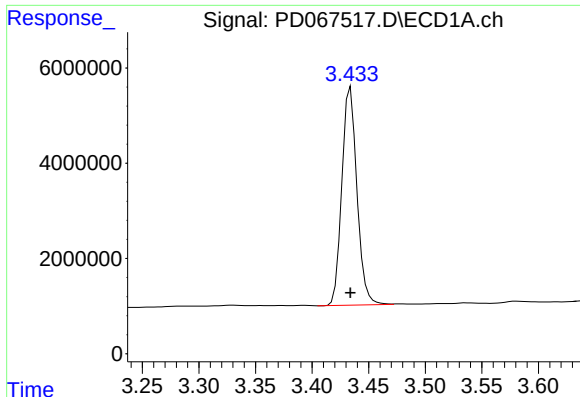

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 42424483
Conc: 23.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

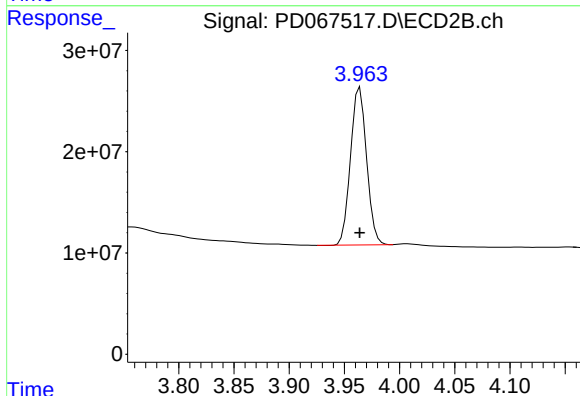


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 157650694
Conc: 23.89 ng/ml

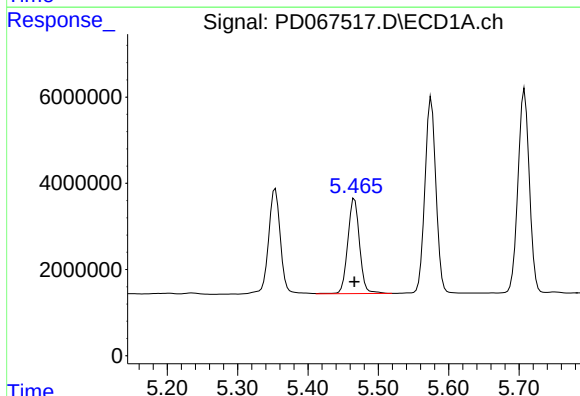


#9 Endosulfan I

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 25670655
Conc: 11.54 ng/ml

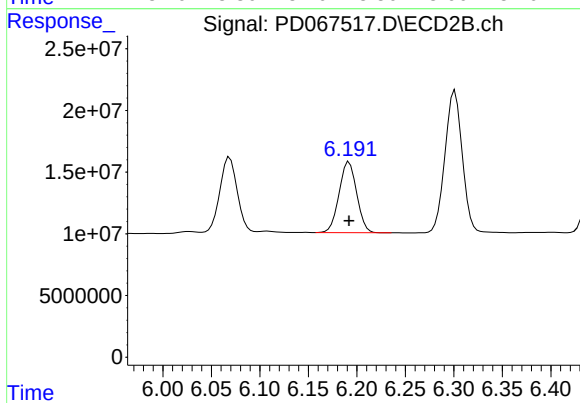

#9 Endosulfan I


R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 72644745
Conc: 12.00 ng/ml

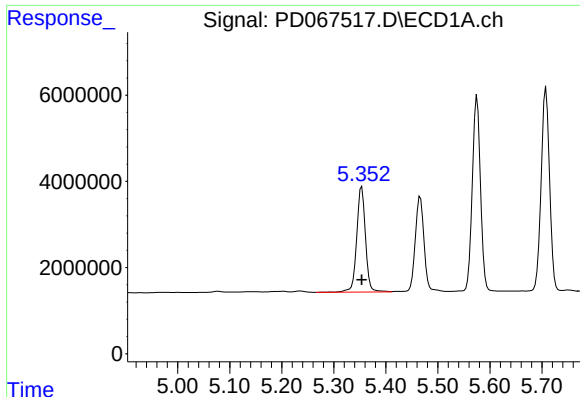

#10 gamma-Chlordane


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 28599299
Conc: 11.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

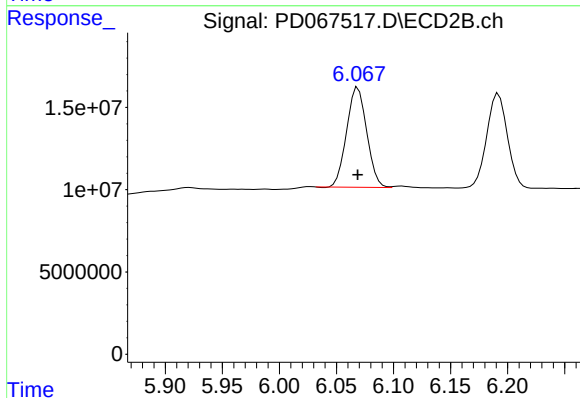


#10 gamma-Chlordane

R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 74390139
Conc: 11.47 ng/ml

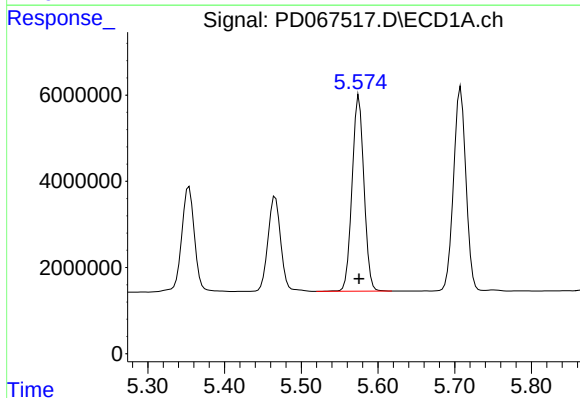


#12 4,4'-DDE

R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 49345334
Conc: 22.29 ng/ml

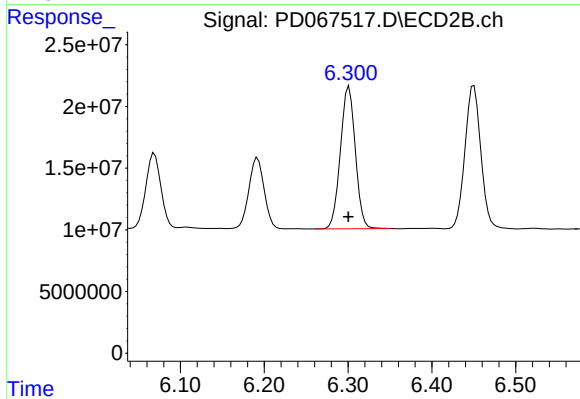

#12 4,4'-DDE


R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 142847879
Conc: 23.19 ng/ml

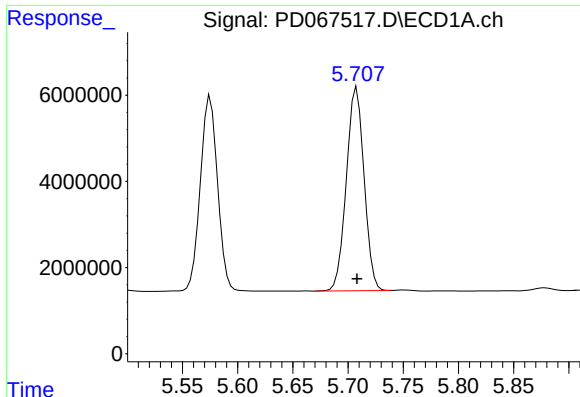

#13 Dieldrin


R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 52718761
Conc: 21.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

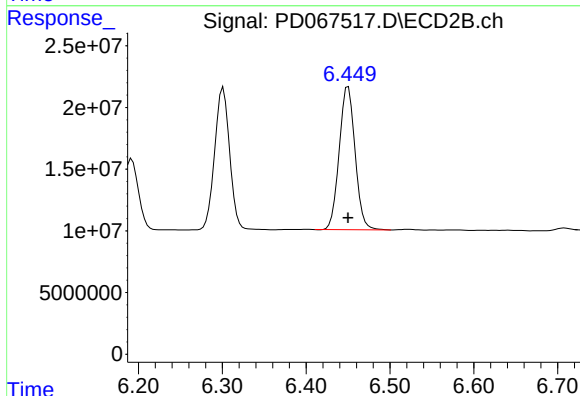


#13 Dieldrin

R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 152646070
Conc: 22.98 ng/ml

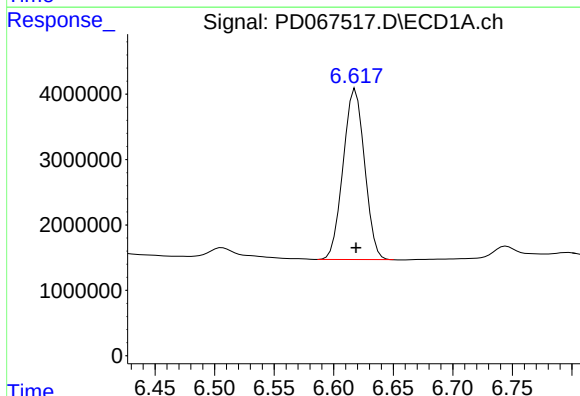


#19 Endosulfan Sulfate

R.T.: 6.618 min
Delta R.T.: 0.000 min
Response: 32690782
Conc: 20.25 ng/ml

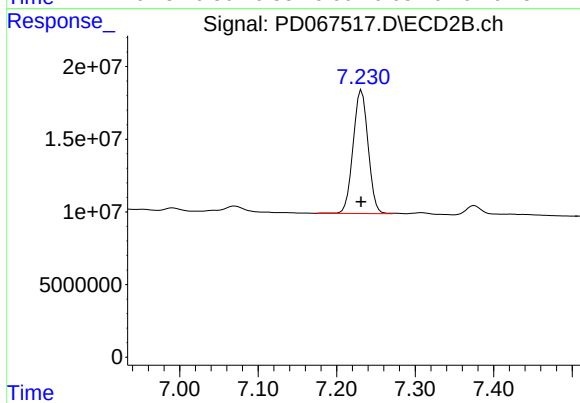

#19 Endosulfan Sulfate


R.T.: 7.232 min
Delta R.T.: 0.000 min
Response: 112885154
Conc: 20.65 ng/ml

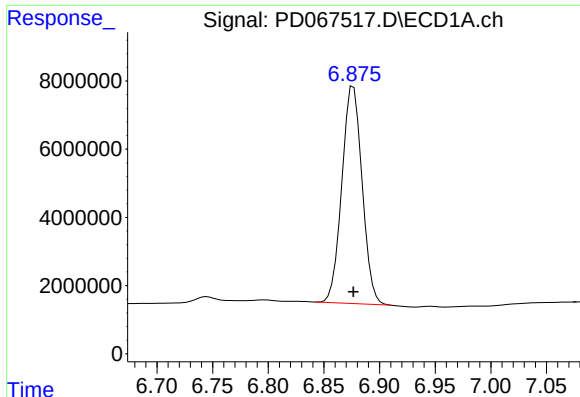

#20 Methoxychlor


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 80720539
Conc: 95.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

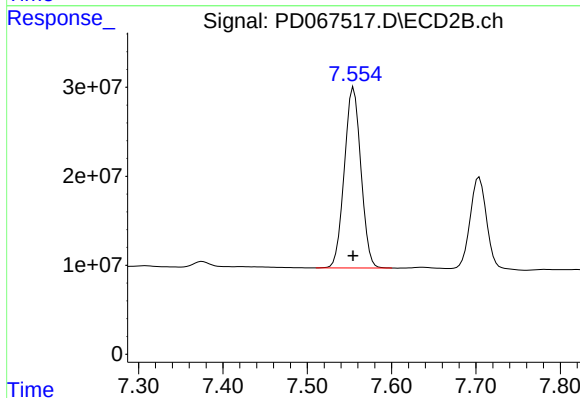


#20 Methoxychlor

R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 277008456
Conc: 95.47 ng/ml

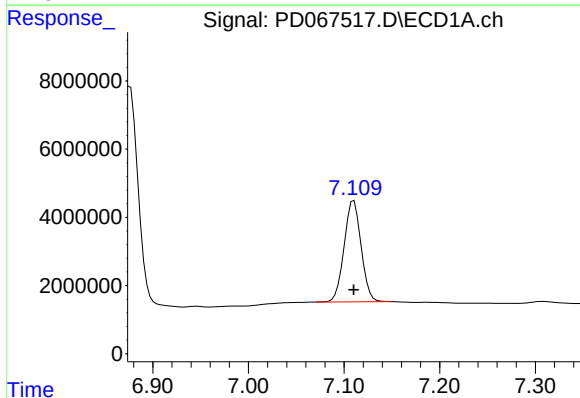


#21 Endrin ketone

R.T.: 7.110 min
Delta R.T.: 0.000 min
Response: 36836217
Conc: 21.52 ng/ml

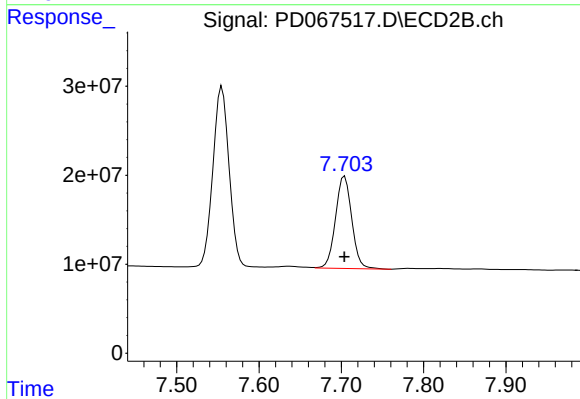

#21 Endrin ketone


R.T.: 7.704 min
Delta R.T.: 0.000 min
Response: 141956697
Conc: 22.62 ng/ml

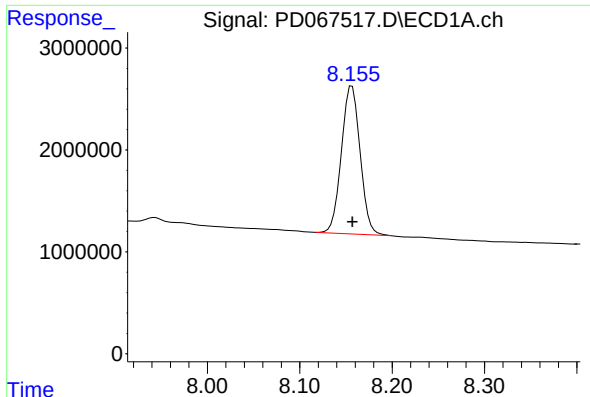

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 20412619
Conc: 22.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

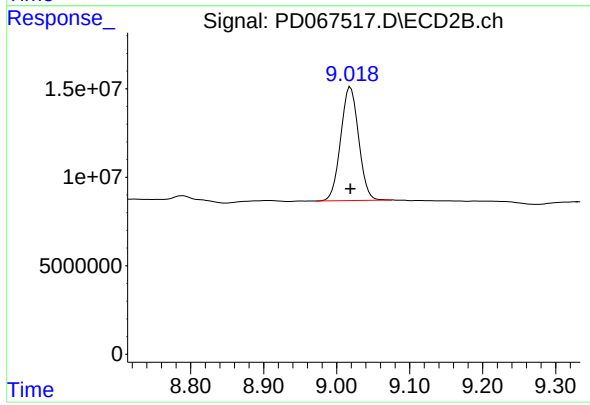

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 109379576
Conc: 23.01 ng/ml