

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:01
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:32:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:29:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.964	214.6E6	603.5E6	99.521	96.448
28)	SA Decachlor...	8.157	9.019	77808162	421.6E6	95.002	95.320
Target Compounds							
23)	Chlordane-1	4.295	4.954	77980276	252.0E6	979.279	961.807
24)	Chlordane-2	4.792	5.423	84037320	252.6E6	964.635	958.218
25)	Chlordane-3	5.355	6.069	268.0E6	908.4E6	994.029	973.249
26)	Chlordane-4	5.412	6.141	219.0E6	1061.3E6	990.499	969.308
27)	Chlordane-5	6.246	6.950	81678404	215.7E6	979.079	967.279



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:01
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:32:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:29:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

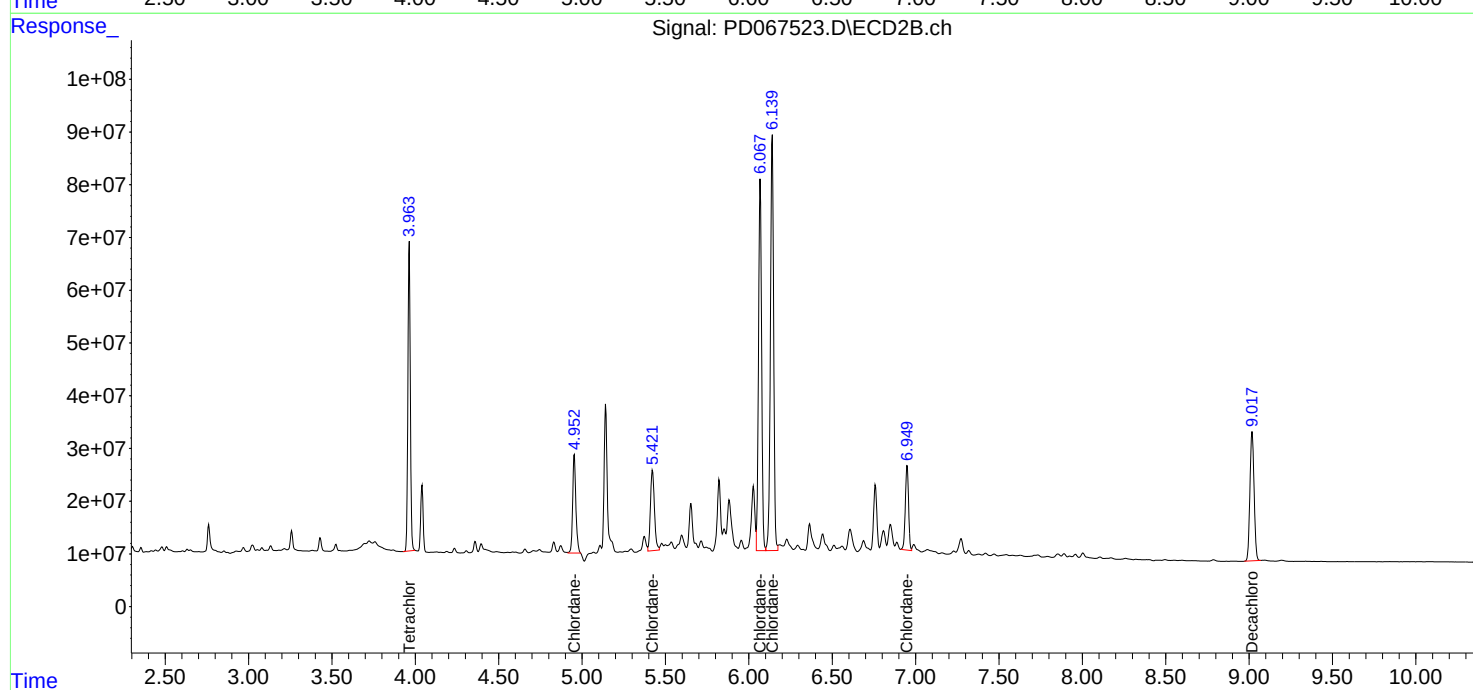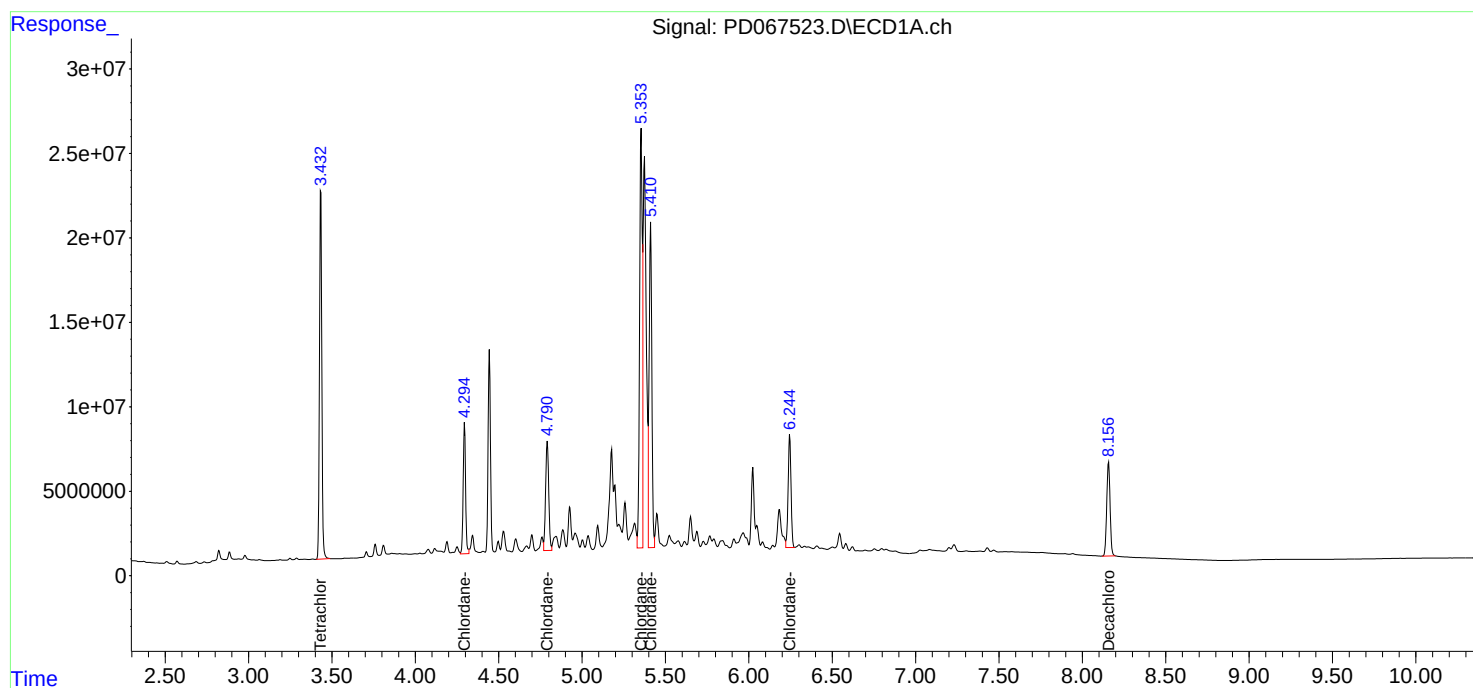


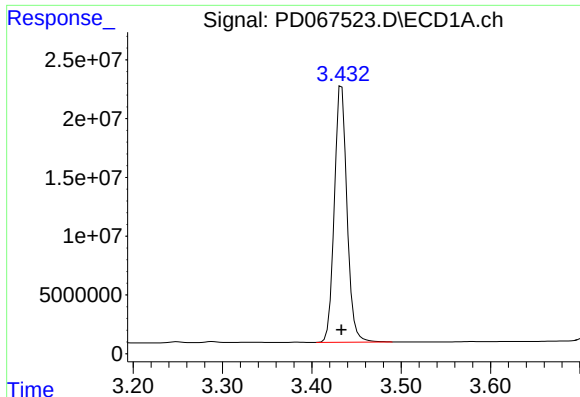

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 214565998
Conc: 99.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

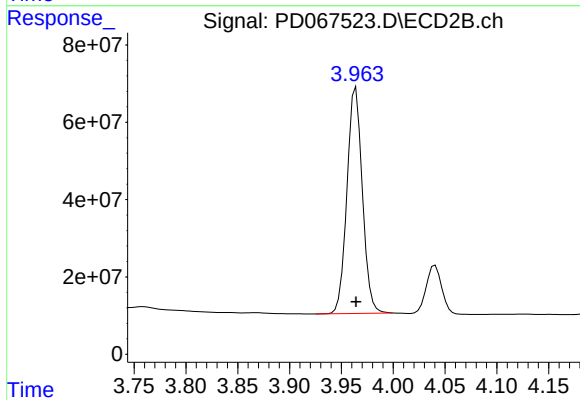


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 603519243
Conc: 96.45 ng/ml

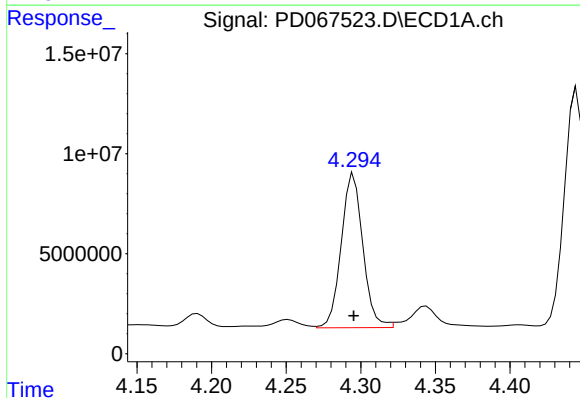


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.000 min
Response: 77980276
Conc: 979.28 ng/ml

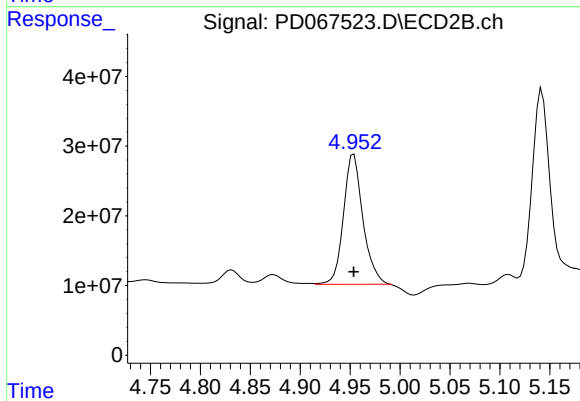

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 252029880
Conc: 961.81 ng/ml

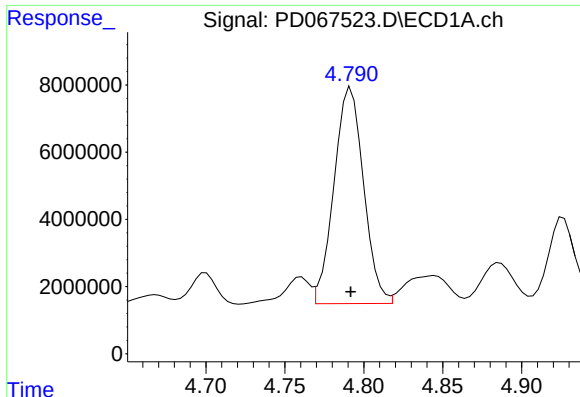

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 84037320
Conc: 964.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

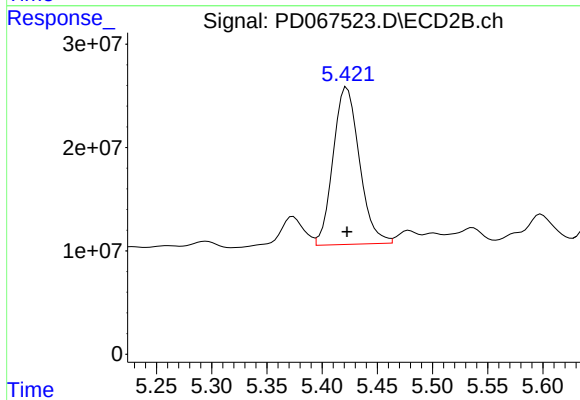


#24 Chlordane-2

R.T.: 5.423 min
Delta R.T.: 0.000 min
Response: 252645516
Conc: 958.22 ng/ml

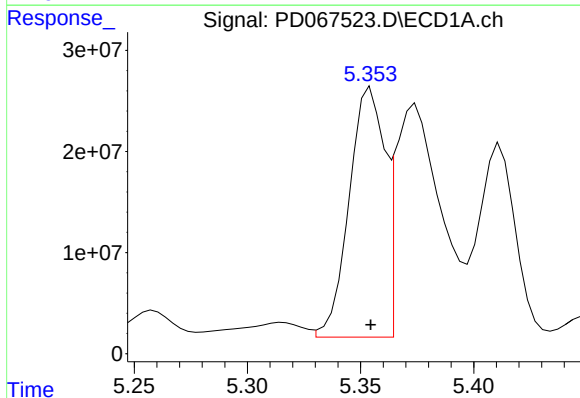


#25 Chlordane-3

R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 268001474
Conc: 994.03 ng/ml

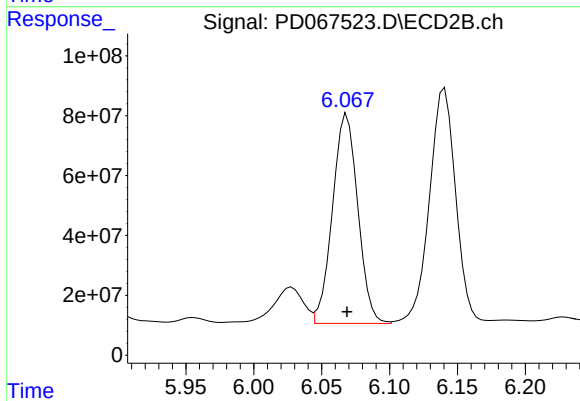

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 908357132
Conc: 973.25 ng/ml

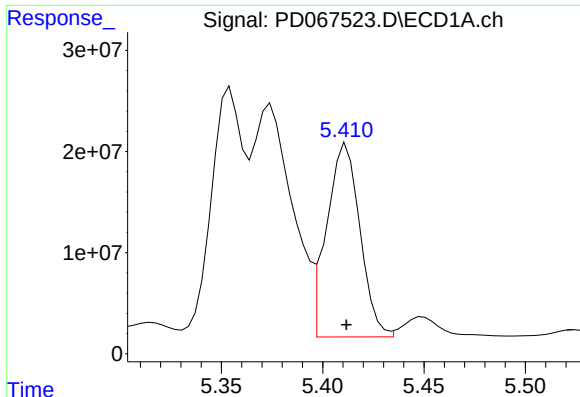

#26 Chlordane-4


R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 219021024
Conc: 990.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

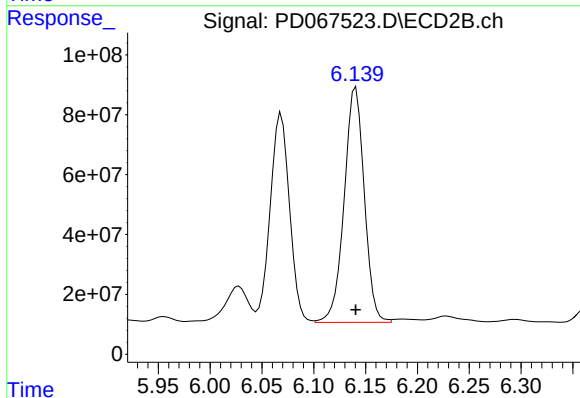


#26 Chlordane-4

R.T.: 6.141 min
Delta R.T.: 0.000 min
Response: 1061291783
Conc: 969.31 ng/ml

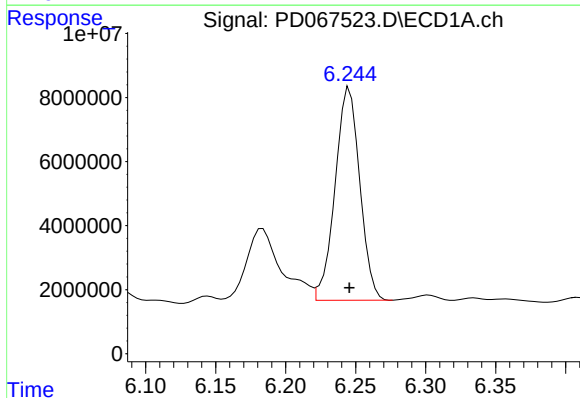


#27 Chlordane-5

R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 81678404
Conc: 979.08 ng/ml

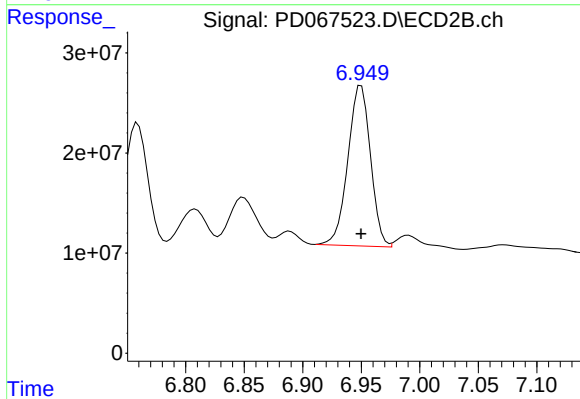

#27 Chlordane-5


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 215707028
Conc: 967.28 ng/ml

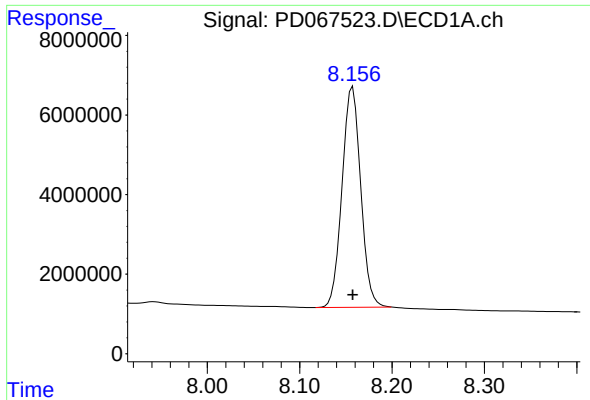

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 77808162
Conc: 95.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

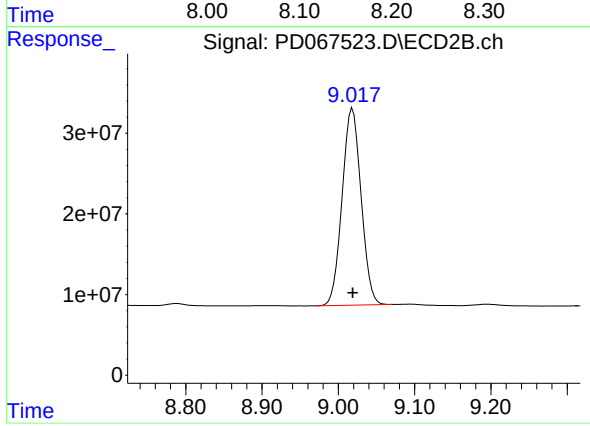

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 421604908
Conc: 95.32 ng/ml