

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:15
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:34:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:29:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.964	163.7E6	460.5E6	75.603	74.059
28)	SA Decachlor...	8.157	9.019	61021895	331.8E6	74.670	75.018
Target Compounds							
23)	Chlordane-1	4.295	4.953	59870090	193.7E6	751.233	742.707
24)	Chlordane-2	4.791	5.422	65088046	196.2E6	748.080	746.147
25)	Chlordane-3	5.354	6.068	205.4E6	697.4E6	757.819	748.159
26)	Chlordane-4	5.411	6.140	166.1E6	818.8E6	750.674	748.566
27)	Chlordane-5	6.245	6.949	60730769	165.3E6	735.175	744.045



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:15
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:34:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:29:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

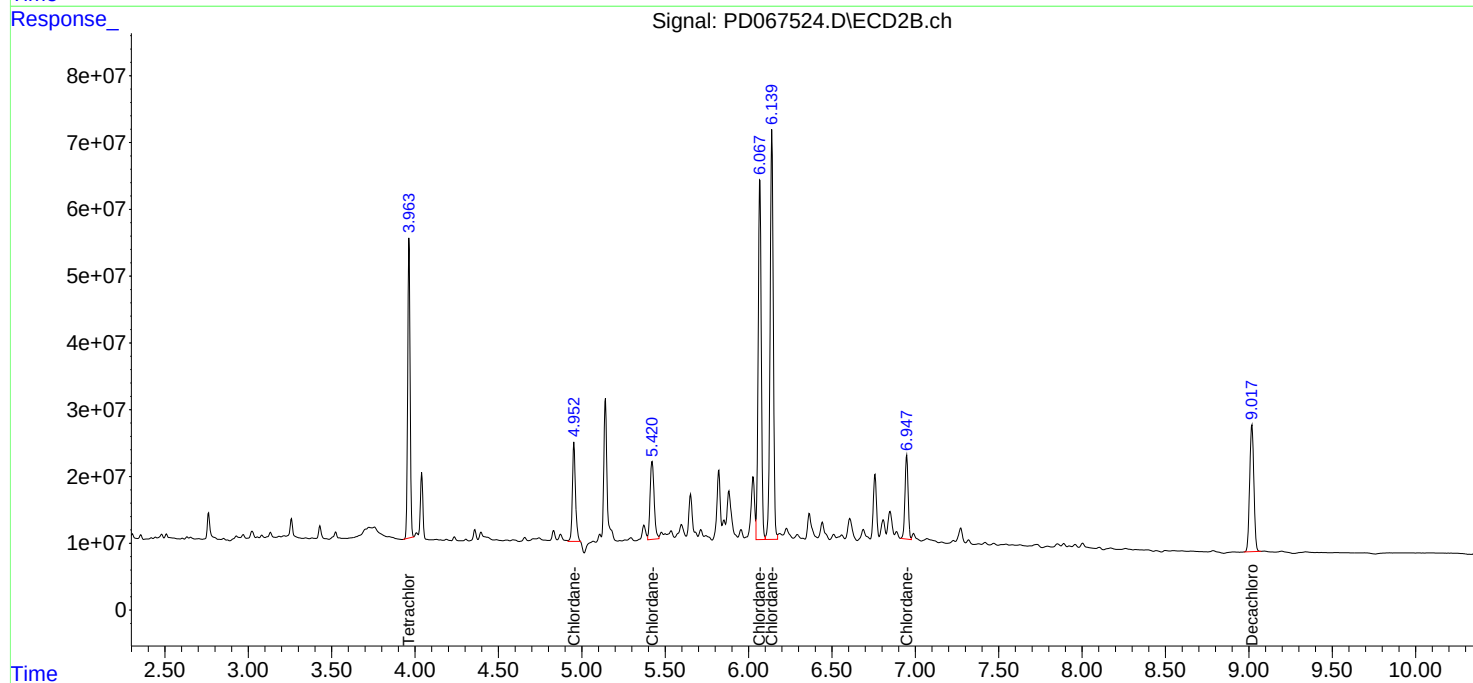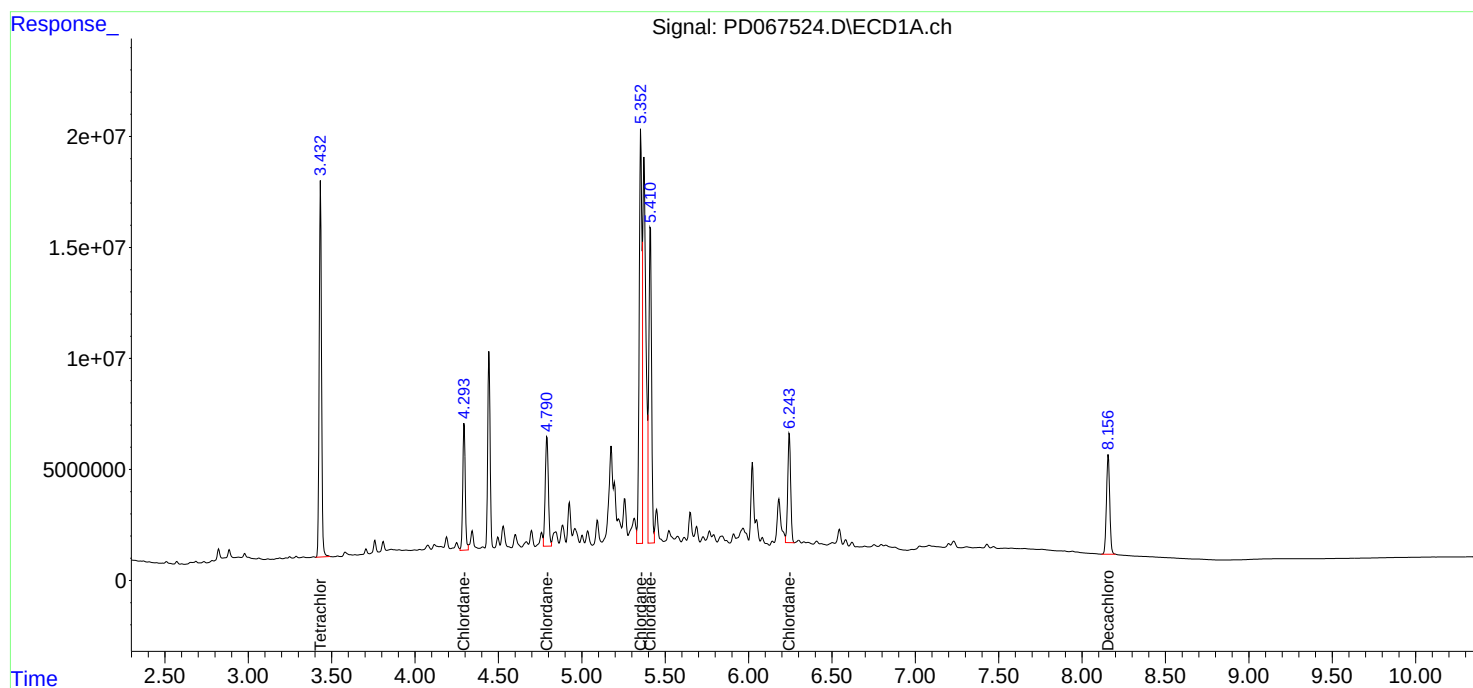


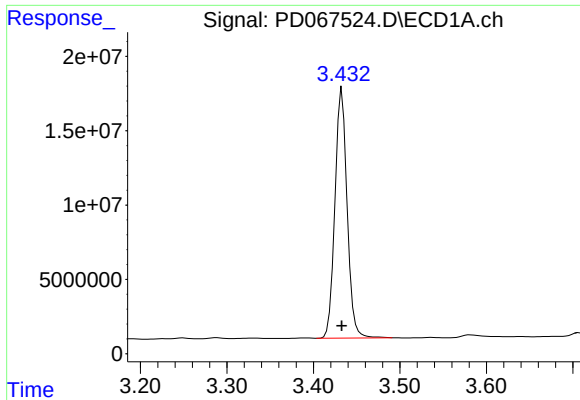

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 163657877
Conc: 75.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

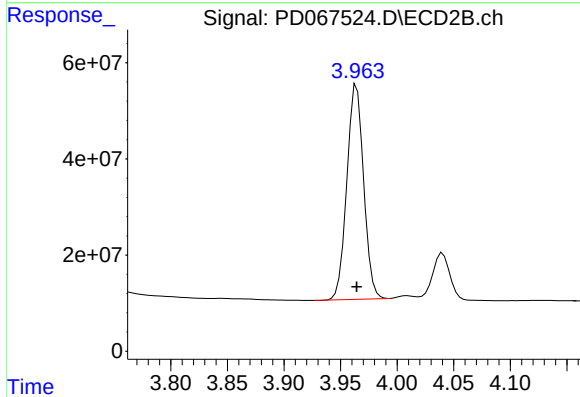


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 460532598
Conc: 74.06 ng/ml

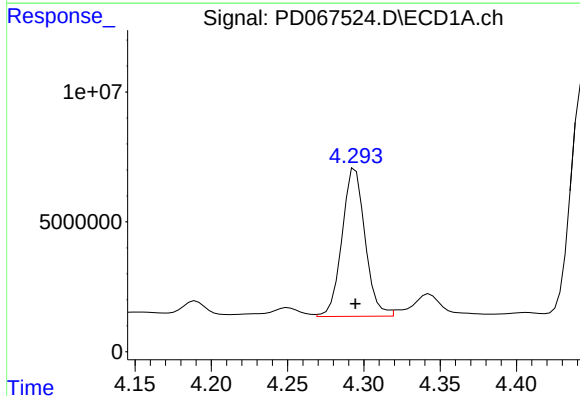


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.000 min
Response: 59870090
Conc: 751.23 ng/ml

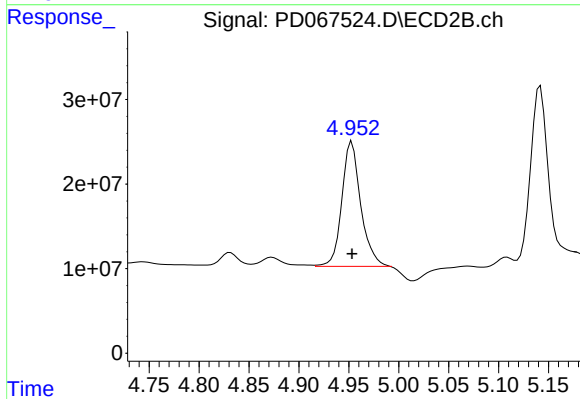

#23 Chlordane-1


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 193675770
Conc: 742.71 ng/ml

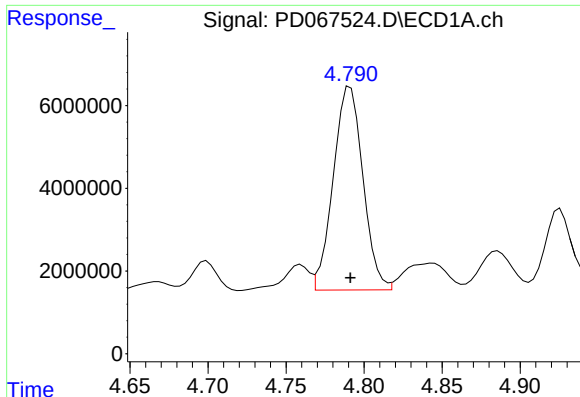

#24 Chlordane-2


R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 65088046
Conc: 748.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

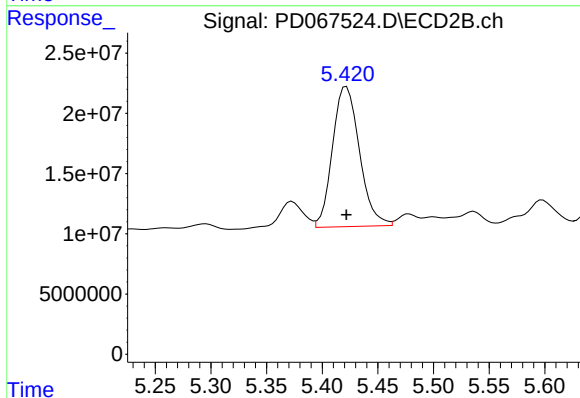


#24 Chlordane-2

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 196226637
Conc: 746.15 ng/ml

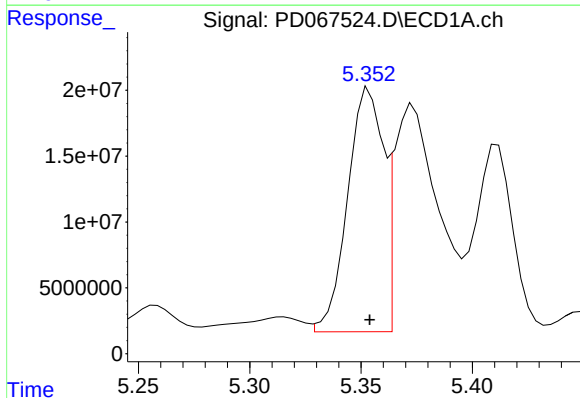


#25 Chlordane-3

R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 205387316
Conc: 757.82 ng/ml

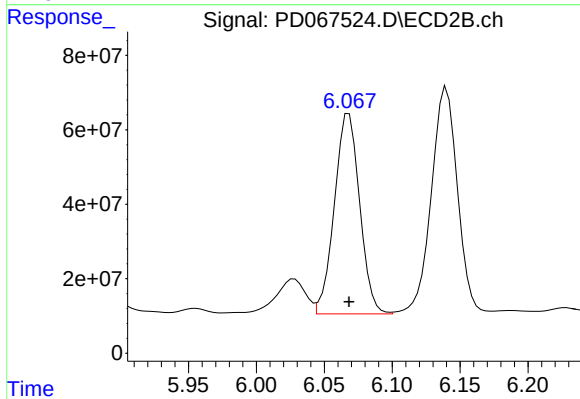

#25 Chlordane-3


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 697419570
Conc: 748.16 ng/ml

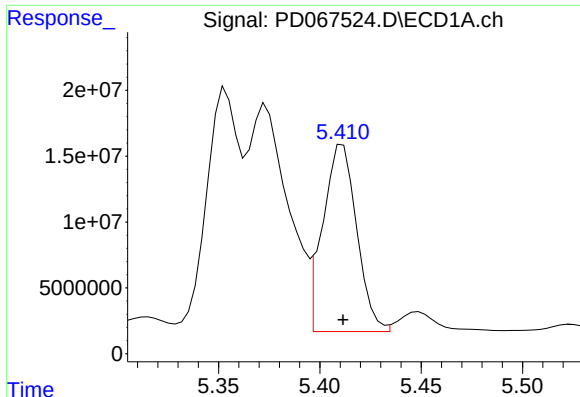

#26 Chlordane-4


R.T.: 5.411 min
Delta R.T.: 0.000 min
Response: 166064855
Conc: 750.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

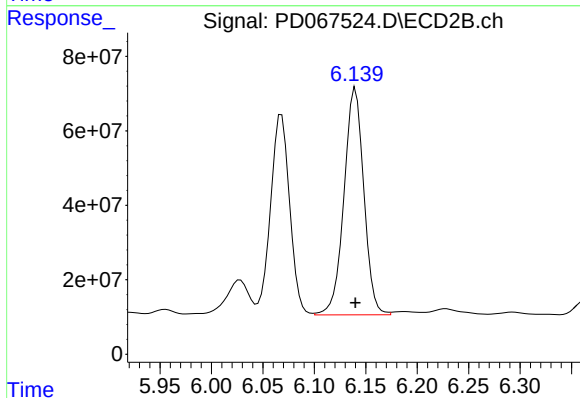


#26 Chlordane-4

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 818819277
Conc: 748.57 ng/ml

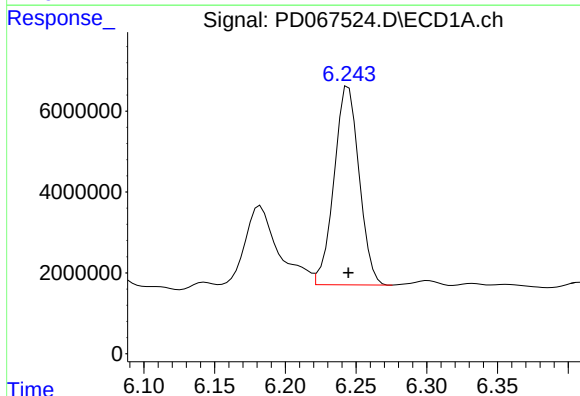


#27 Chlordane-5

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 60730769
Conc: 735.17 ng/ml

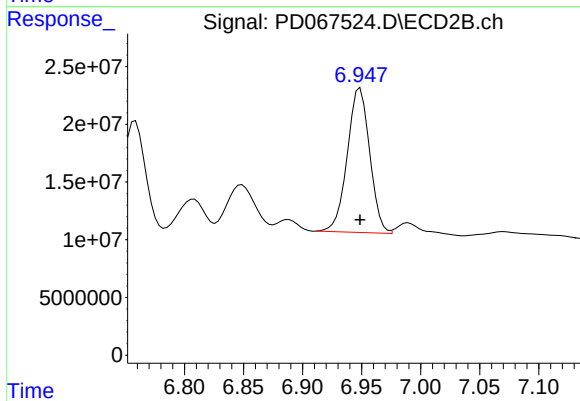

#27 Chlordane-5


R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 165268986
Conc: 744.05 ng/ml

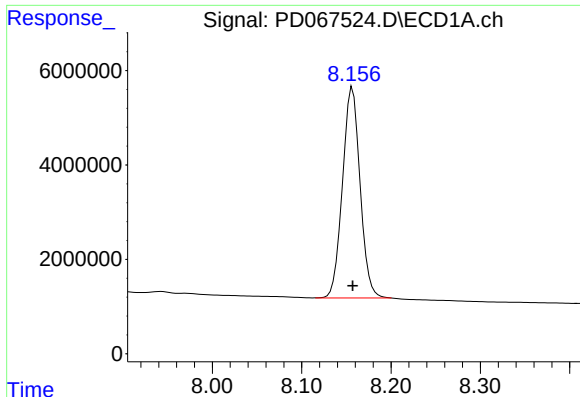

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 61021895
Conc: 74.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

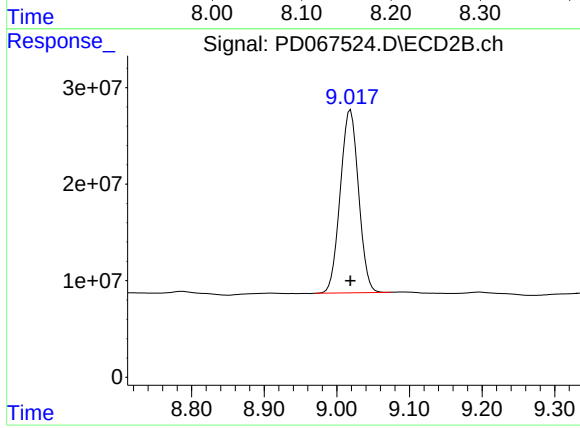

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 331847923
Conc: 75.02 ng/ml