

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 18:43
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:36:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:29:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	54023715	172.1E6	24.968	26.957
28)	SA Decachlor...	8.158	9.019	23227562	124.9E6	27.482	27.356
Target Compounds							
23)	Chlordane-1	4.295	4.954	20197214	73319090	252.563	272.666
24)	Chlordane-2	4.792	5.422	24263032	73469670	271.040	271.397
25)	Chlordane-3	5.355	6.069	66760331	248.9E6	247.234	262.511
26)	Chlordane-4	5.412	6.141	55611892	295.2E6	251.038	264.591
27)	Chlordane-5	6.246	6.950	22225343	58776359	264.019	260.802



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 18:43
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:36:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:29:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

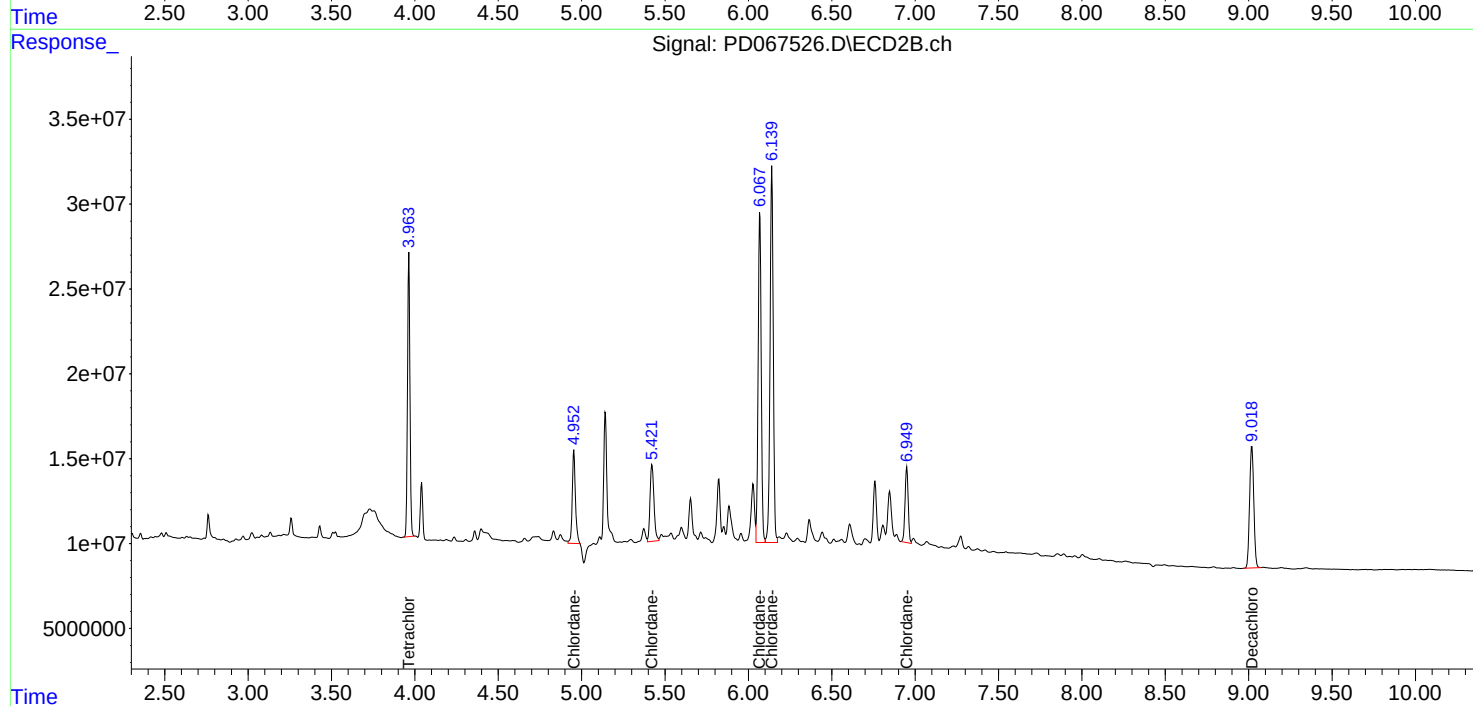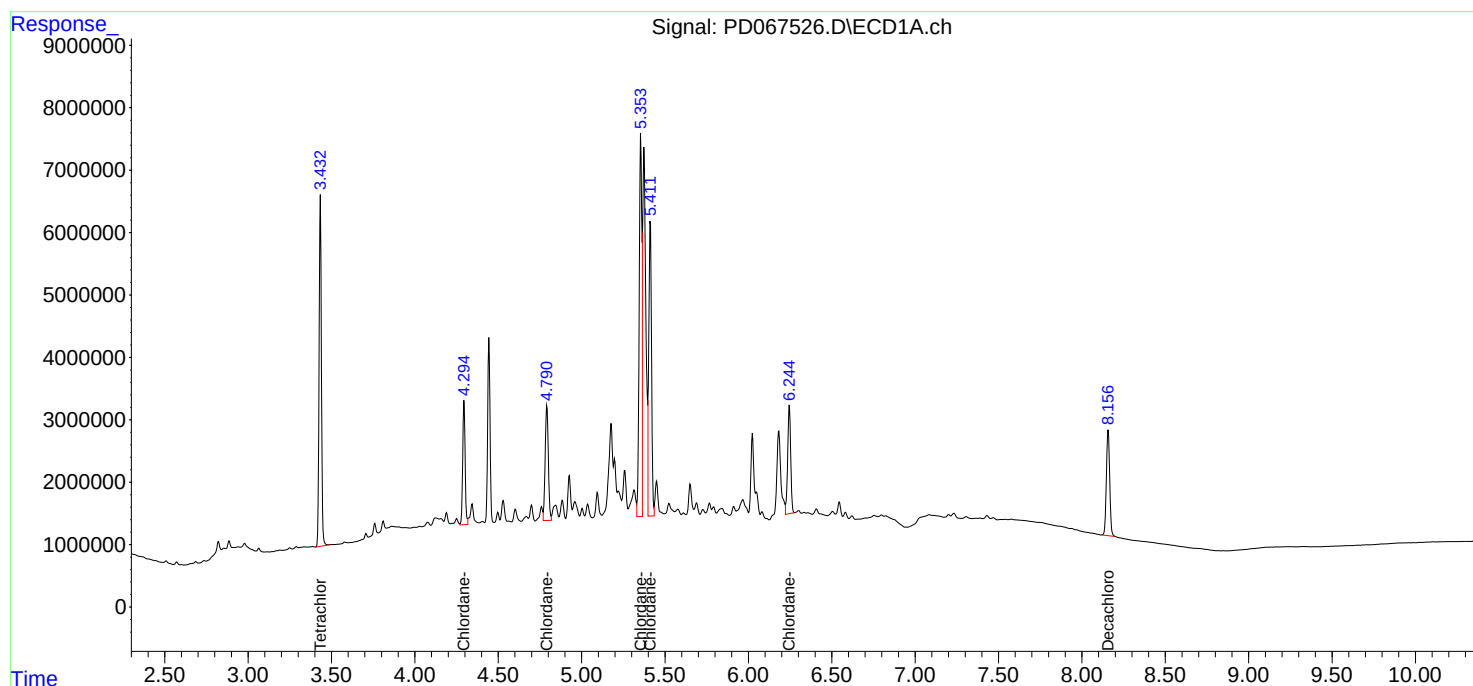


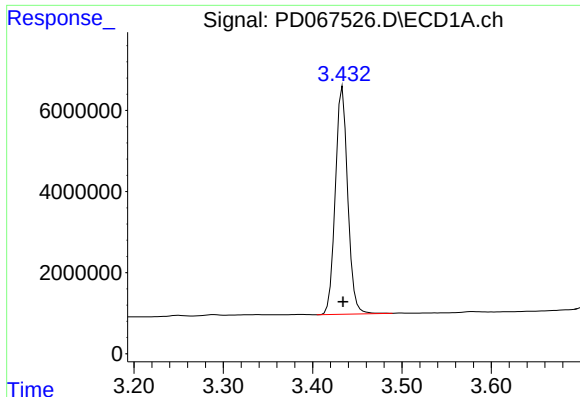

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 54023715
Conc: 24.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

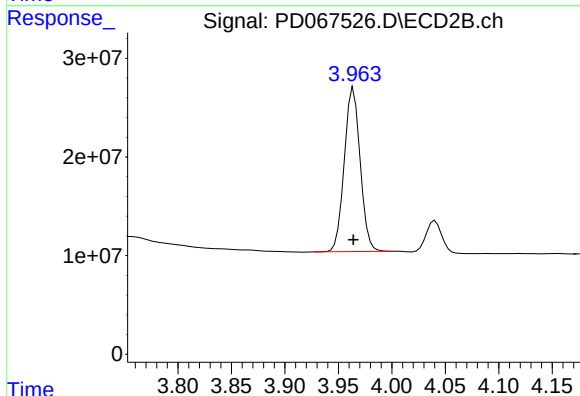


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 172124465
Conc: 26.96 ng/ml

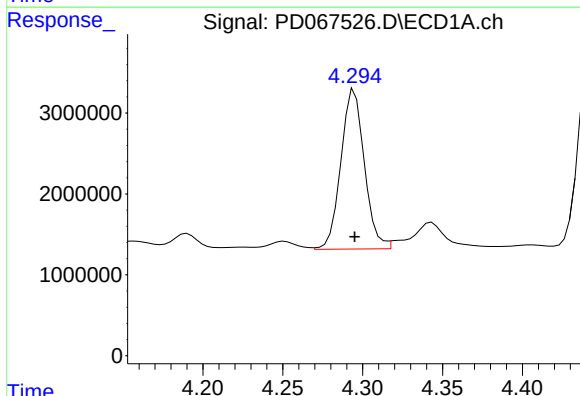


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.000 min
Response: 20197214
Conc: 252.56 ng/ml

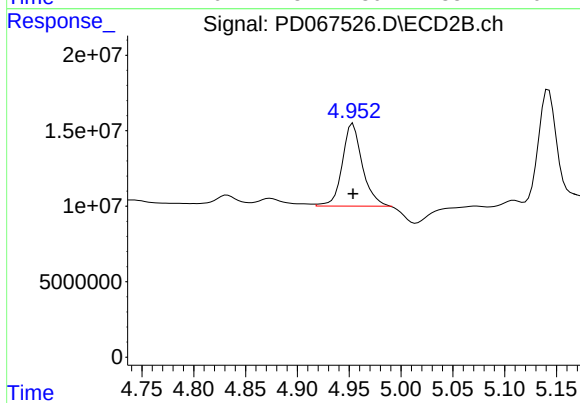

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 73319090
Conc: 272.67 ng/ml

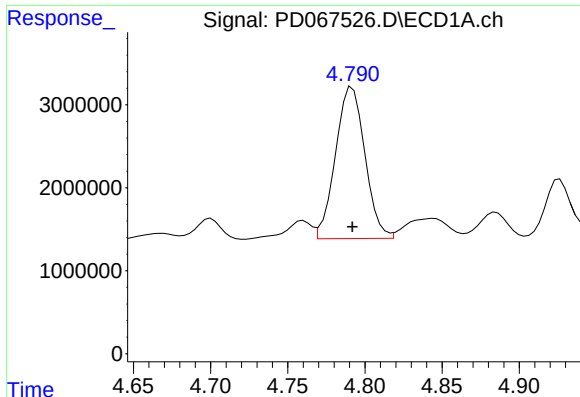

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 24263032
Conc: 271.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

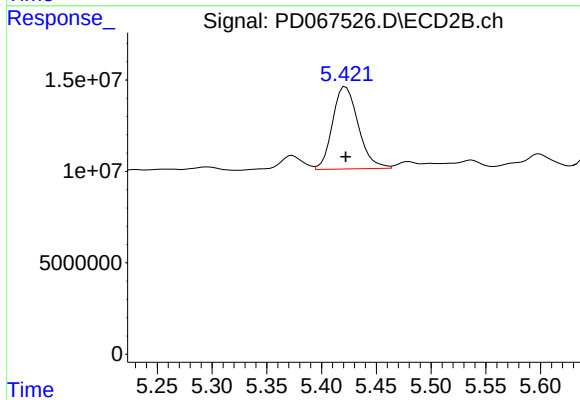


#24 Chlordane-2

R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 73469670
Conc: 271.40 ng/ml

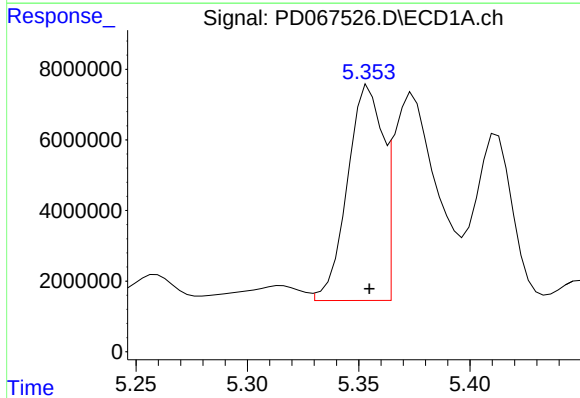


#25 Chlordane-3

R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 66760331
Conc: 247.23 ng/ml

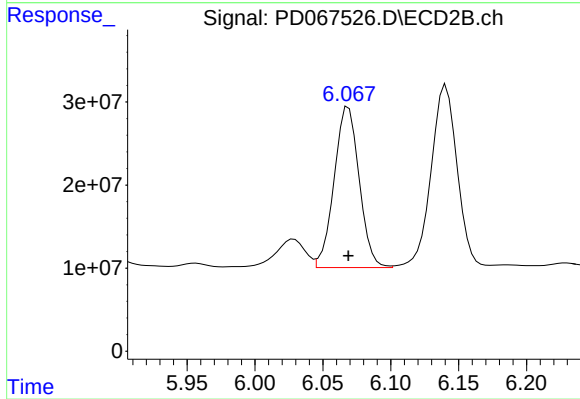

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 248858842
Conc: 262.51 ng/ml

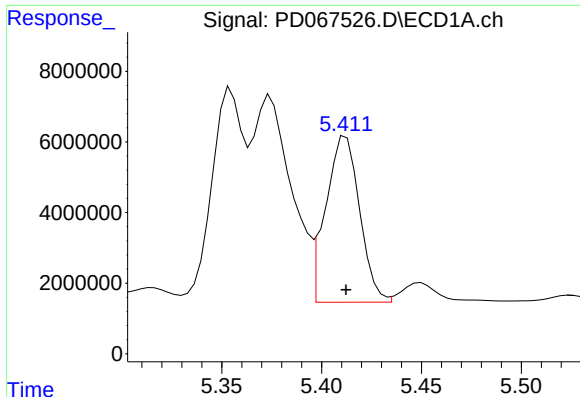

#26 Chlordane-4


R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 55611892
Conc: 251.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

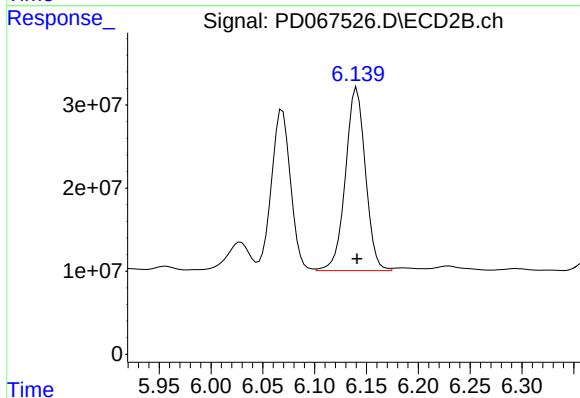


#26 Chlordane-4

R.T.: 6.141 min
Delta R.T.: 0.000 min
Response: 295165615
Conc: 264.59 ng/ml

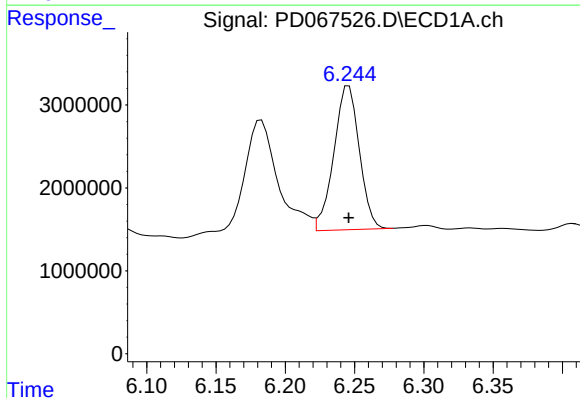


#27 Chlordane-5

R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 22225343
Conc: 264.02 ng/ml

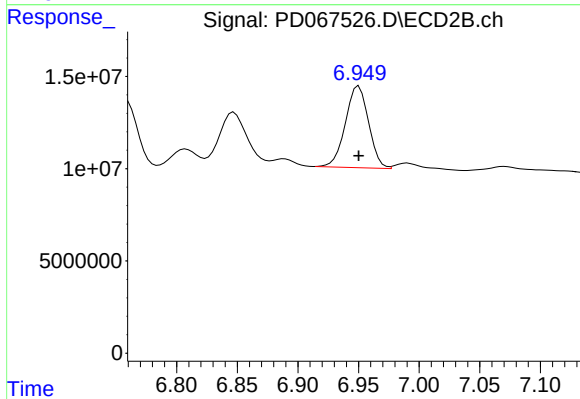

#27 Chlordane-5


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 58776359
Conc: 260.80 ng/ml

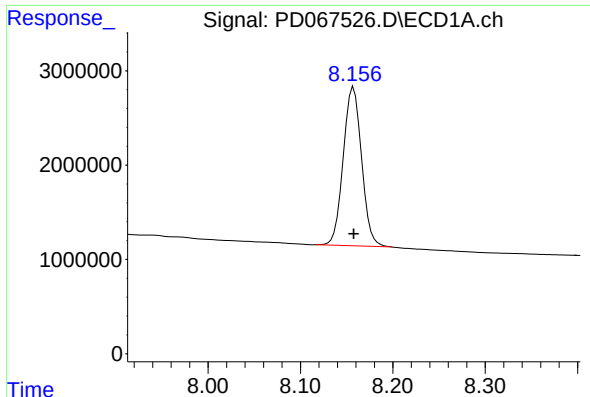

#28 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: 0.000 min
Response: 23227562
Conc: 27.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

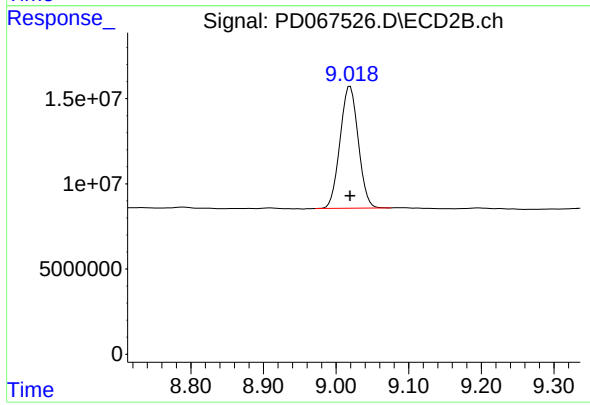

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 124937023
Conc: 27.36 ng/ml