

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
 Data File : PD067534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2021 20:33
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD122821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 01:49:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 01:42:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.964	104.6E6	310.6E6	48.908	47.194
28)	SA Decachlor...	8.157	9.019	41087398	222.6E6	45.256	46.105
Target Compounds							
23)	Chlordane-1	4.295	4.954	38994987	130.3E6	493.809	488.097
24)	Chlordane-2	4.792	5.422	43276743	132.9E6	478.969	484.422
25)	Chlordane-3	5.355	6.069	128.8E6	458.2E6	482.893	475.662
26)	Chlordane-4	5.412	6.141	107.0E6	538.0E6	486.185	471.240
27)	Chlordane-5	6.246	6.950	41179456	109.6E6	475.671	496.779



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122821\
Data File : PD067534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2021 20:33
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD122821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 01:49:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 01:42:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

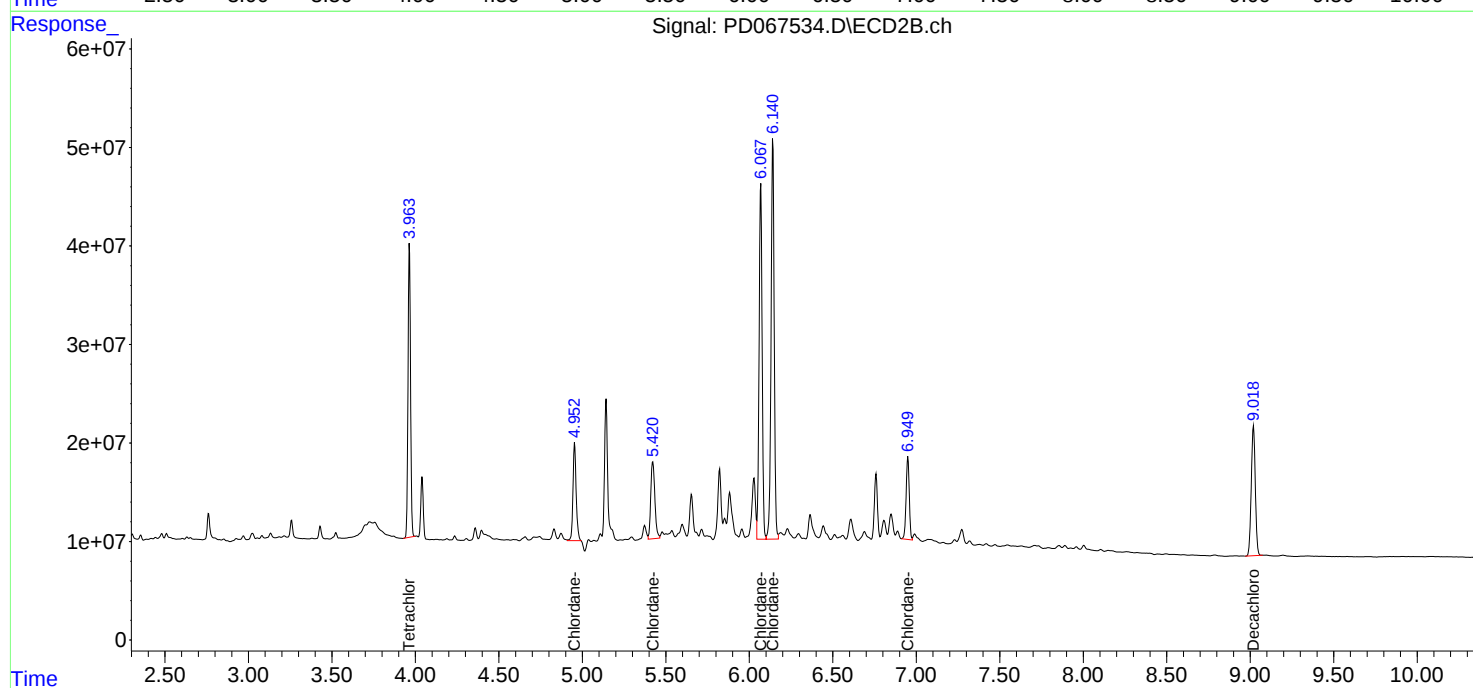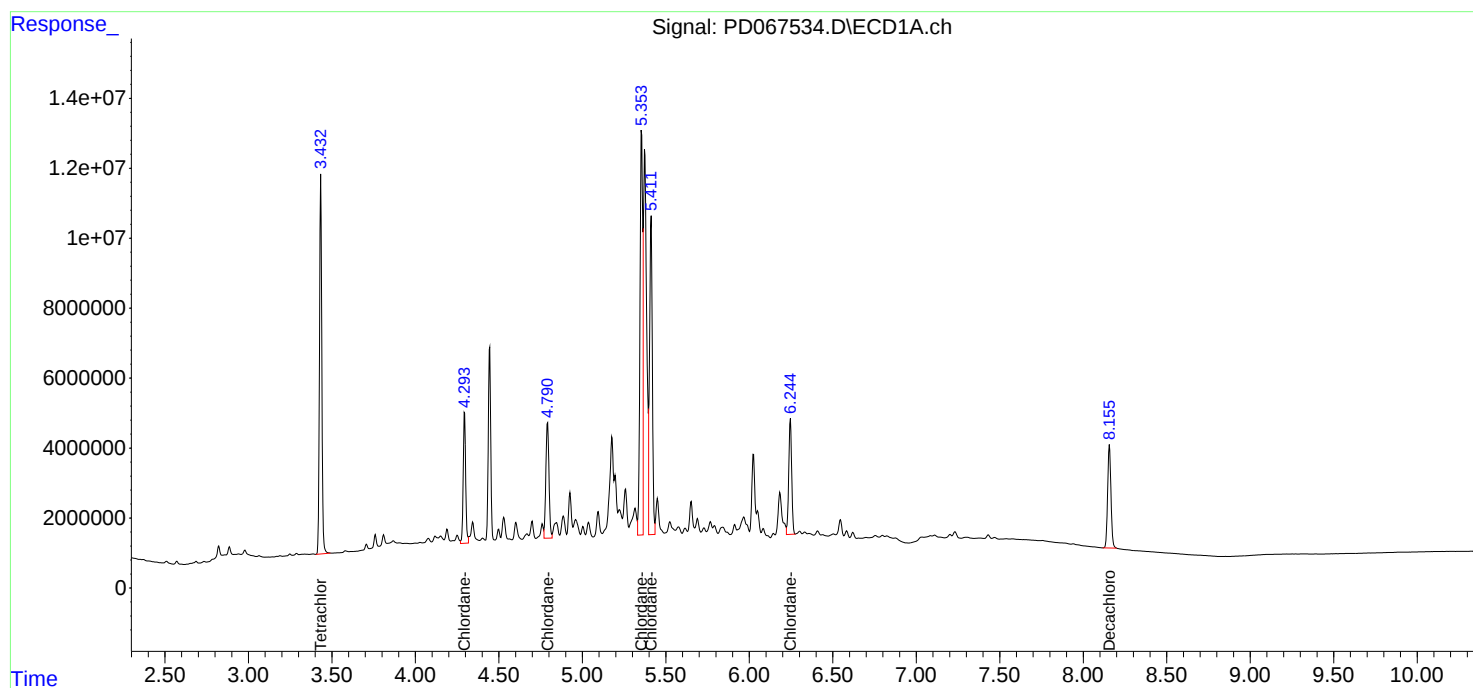


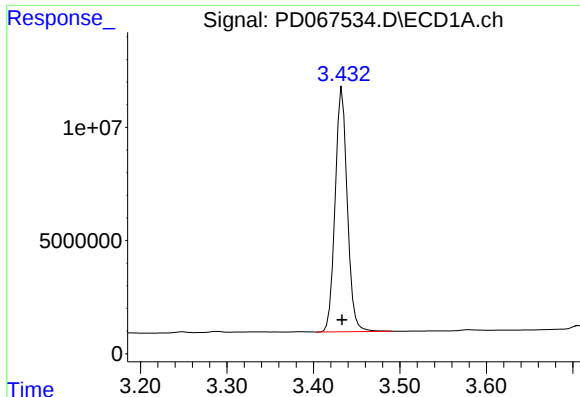

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 104642890
Conc: 48.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD122821

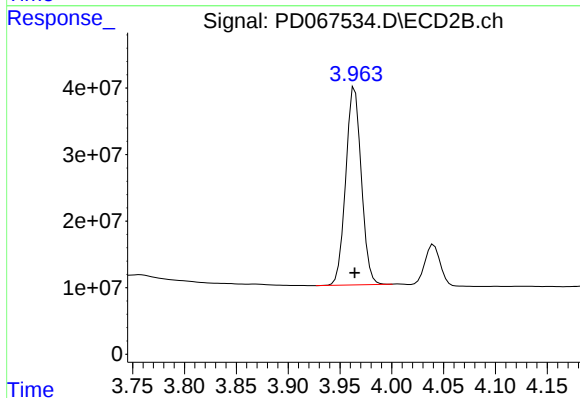


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 310577812
Conc: 47.19 ng/ml

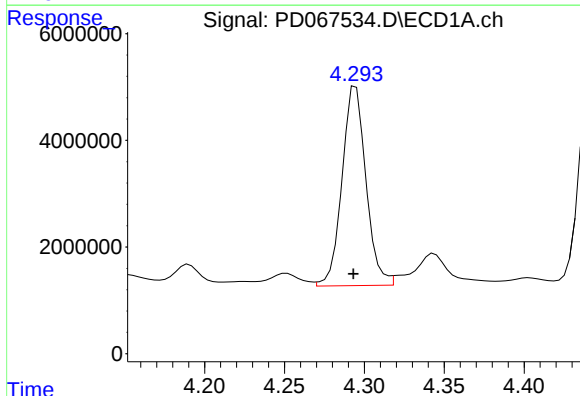


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.002 min
Response: 38994987
Conc: 493.81 ng/ml

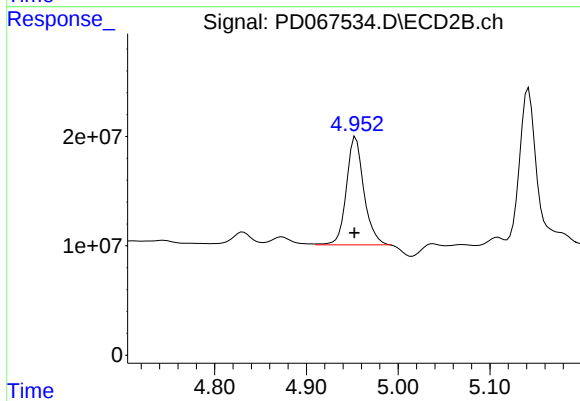

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.002 min
Response: 130339652
Conc: 488.10 ng/ml

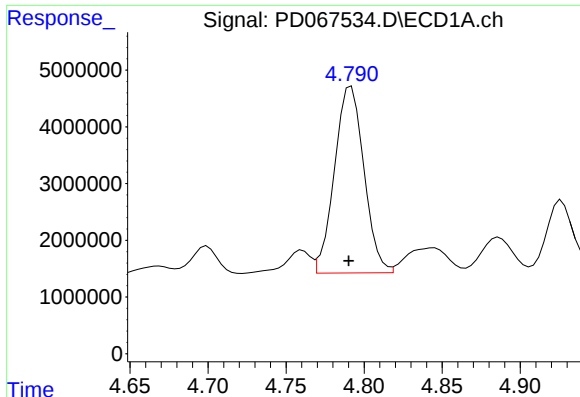

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.002 min
Response: 43276743
Conc: 478.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD122821

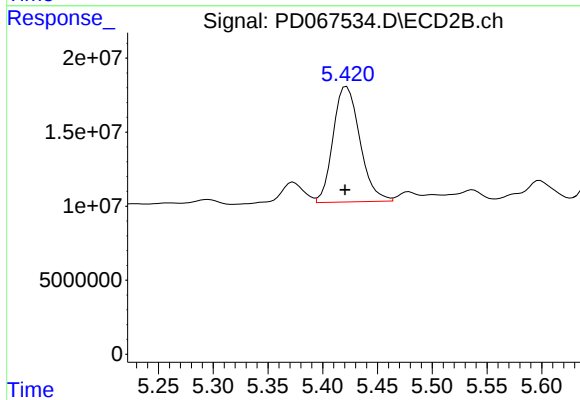


#24 Chlordane-2

R.T.: 5.422 min
Delta R.T.: 0.001 min
Response: 132919173
Conc: 484.42 ng/ml

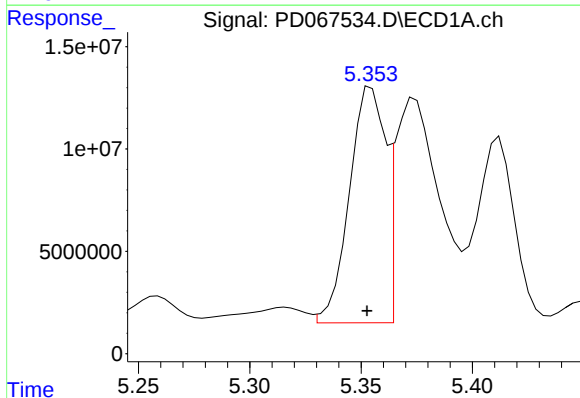


#25 Chlordane-3

R.T.: 5.355 min
Delta R.T.: 0.002 min
Response: 128754821
Conc: 482.89 ng/ml

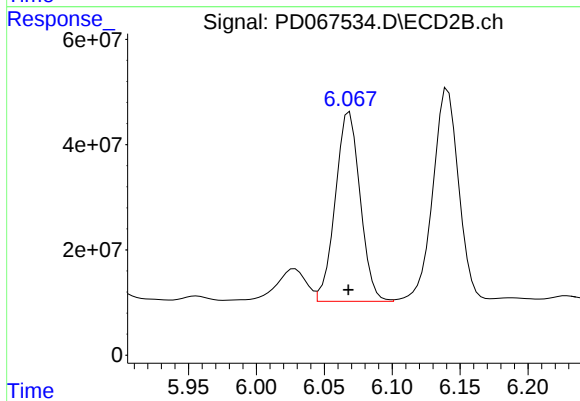

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: 0.001 min
Response: 458160511
Conc: 475.66 ng/ml

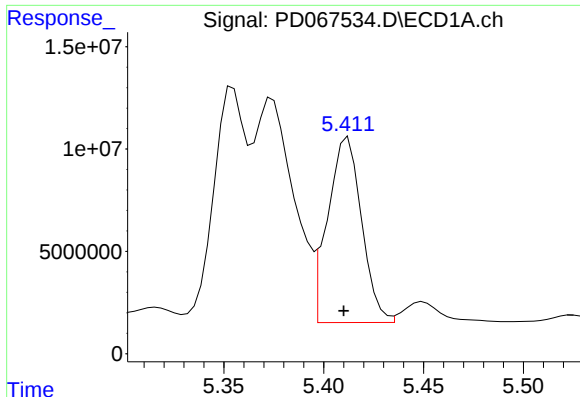

#26 Chlordane-4


R.T.: 5.412 min
Delta R.T.: 0.002 min
Response: 106984640
Conc: 486.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD122821

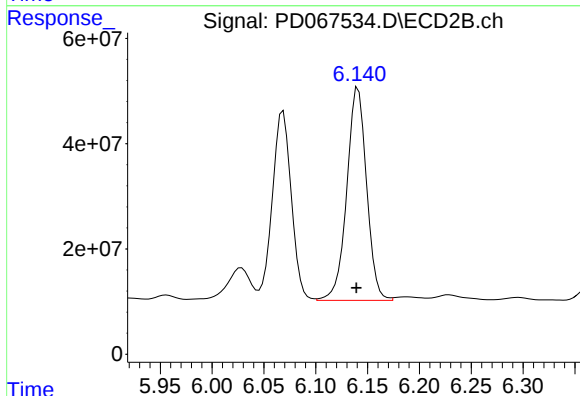


#26 Chlordane-4

R.T.: 6.141 min
Delta R.T.: 0.002 min
Response: 538012471
Conc: 471.24 ng/ml

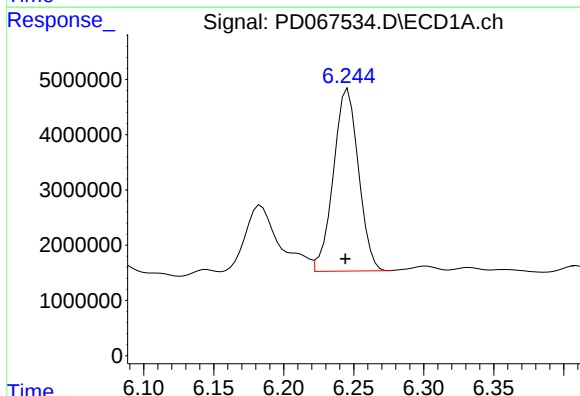


#27 Chlordane-5

R.T.: 6.246 min
Delta R.T.: 0.002 min
Response: 41179456
Conc: 475.67 ng/ml

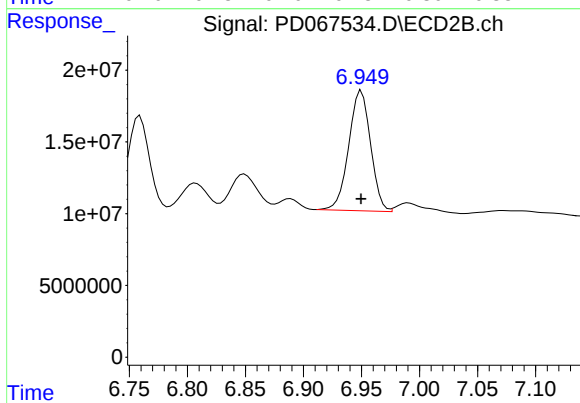

#27 Chlordane-5


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 109634197
Conc: 496.78 ng/ml

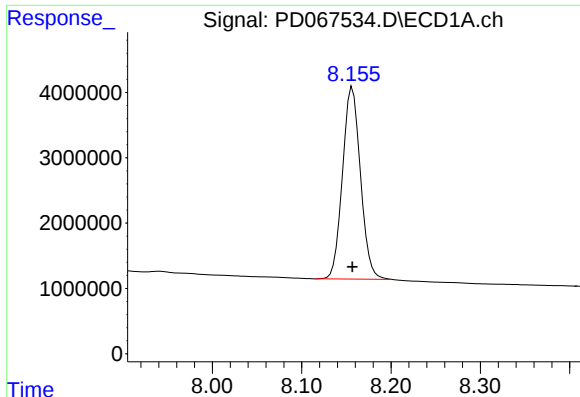

#28 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 41087398
Conc: 45.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD122821

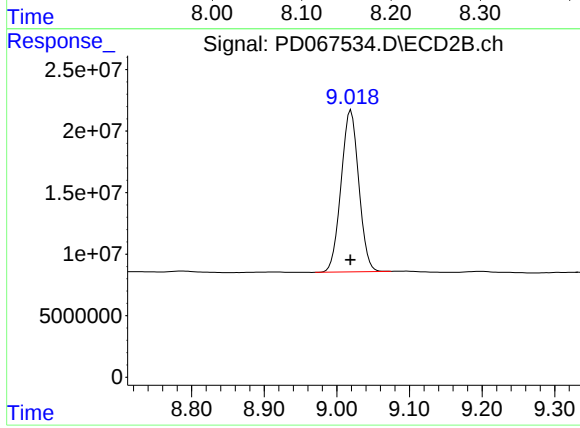

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 222620310
Conc: 46.10 ng/ml