

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 23:21
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:00:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 03:59:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	12160847	489.1E6	4.840	5.373
27)	SA Decachlor...	9.096	7.959	22455803	337.6E6	9.842	10.289
Target Compounds							
2)	A alpha-BHC	4.012	3.300	16137532	742.1E6	4.304	5.088
3)	MA gamma-BHC...	4.345	3.630	15934887	694.7E6	4.404	5.118
4)	MA Heptachlor	4.937	3.977	16708592	691.1E6	4.559	5.134
9)	A Endosulfan I	6.093	5.132	13580966	545.5E6	4.621	5.312
13)	MA Dieldrin	6.369	5.397	27662398	1117.5E6	8.656	10.262
14)	MA Endrin	6.598	5.673	21728537	786.4E6	8.644	10.097
16)	A 4,4'-DDD	6.730	5.821	20914850	833.6E6	8.619	10.308
17)	MA 4,4'-DDT	7.045	6.073	20601282	690.6E6	8.734	10.036
20)	A Methoxychlor	7.519	6.650	60170027	1493.0E6	45.197	52.334


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 23:21
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:00:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 03:59:30 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

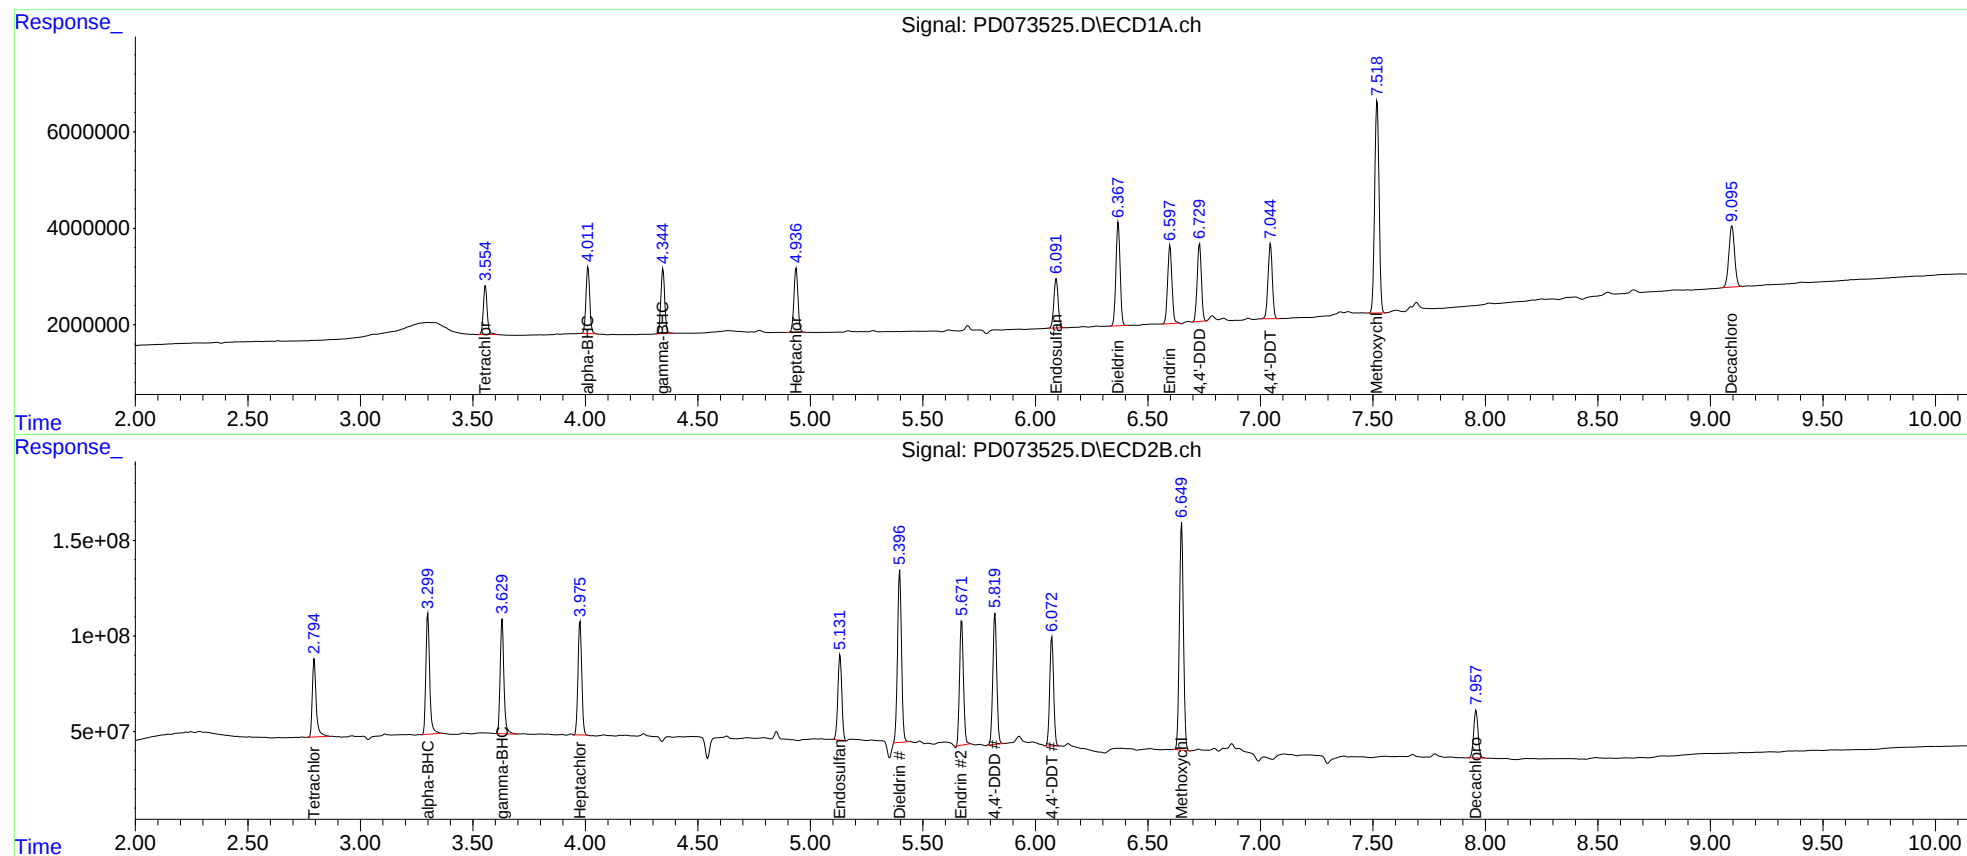

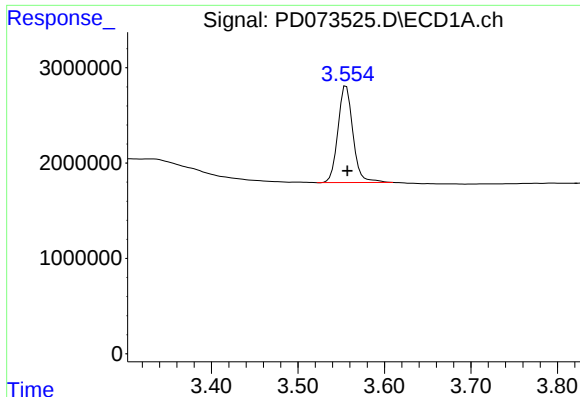


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: -0.001 min
Response: 12160847
Conc: 4.84 ng/ml

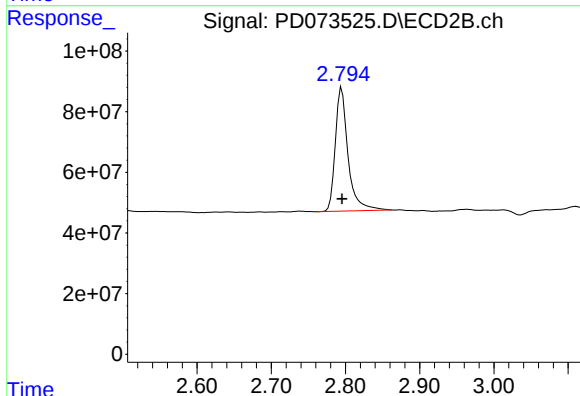


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 489086762
Conc: 5.37 ng/ml

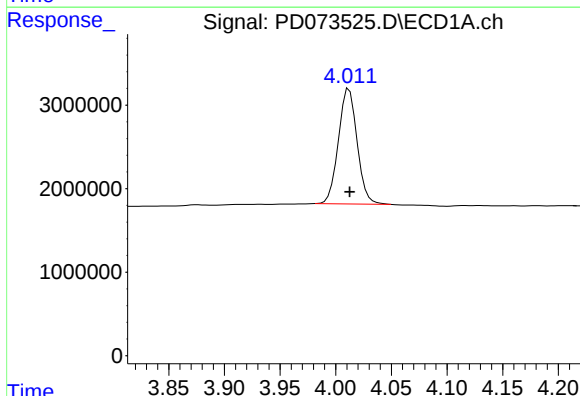


#2 alpha-BHC

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 16137532
Conc: 4.30 ng/ml

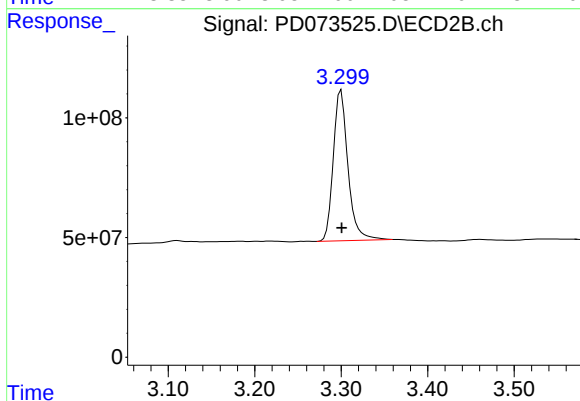


#2 alpha-BHC

R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 742069762
Conc: 5.09 ng/ml

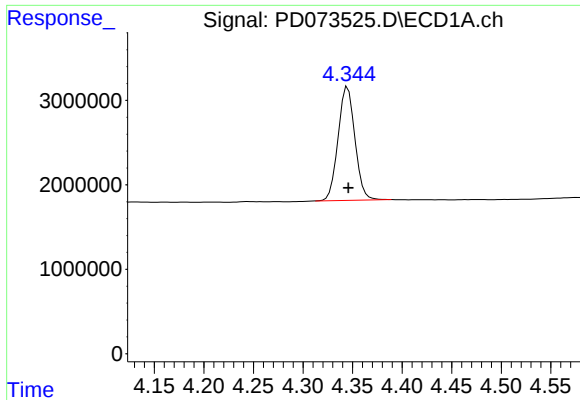


#3 gamma-BHC (Lindane)

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 15934887
Conc: 4.40 ng/ml

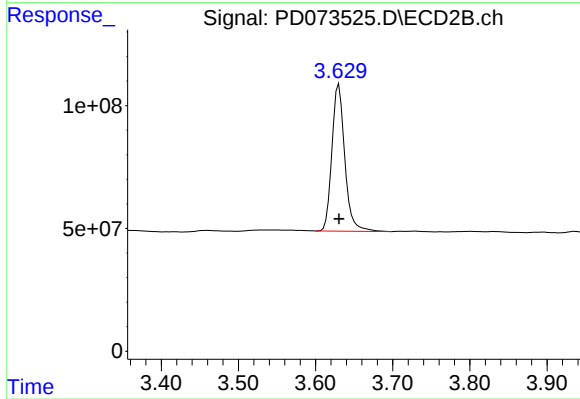


#3 gamma-BHC (Lindane)

R.T.: 3.630 min
Delta R.T.: 0.000 min
Response: 694743389
Conc: 5.12 ng/ml

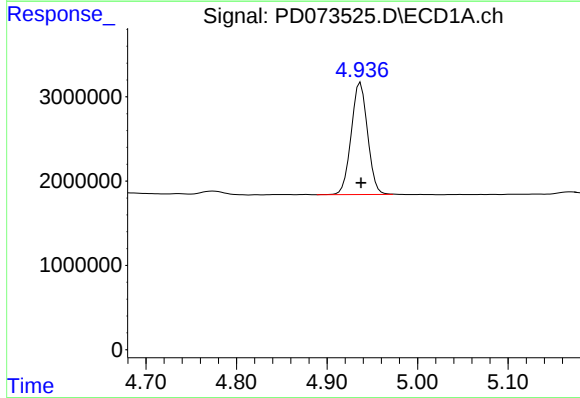


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 16708592
Conc: 4.56 ng/ml

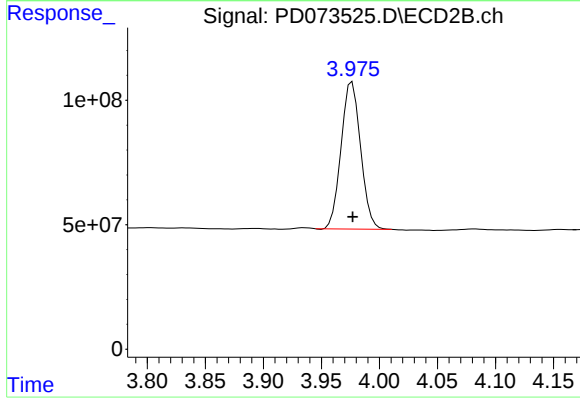


#4 Heptachlor

R.T.: 3.977 min
Delta R.T.: 0.000 min
Response: 691130255
Conc: 5.13 ng/ml

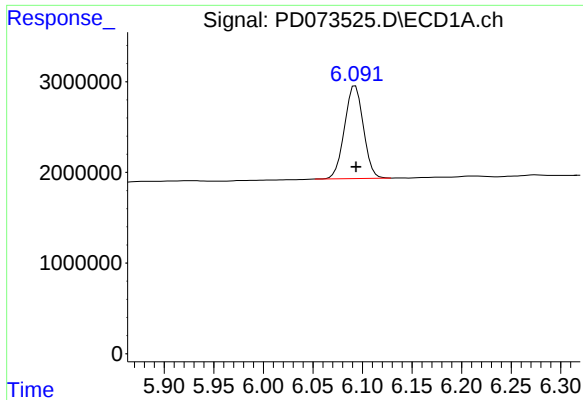


#9 Endosulfan I

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 13580966
Conc: 4.62 ng/ml

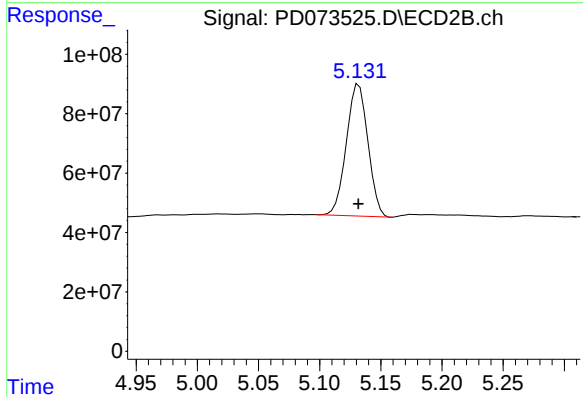


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 545450489
Conc: 5.31 ng/ml

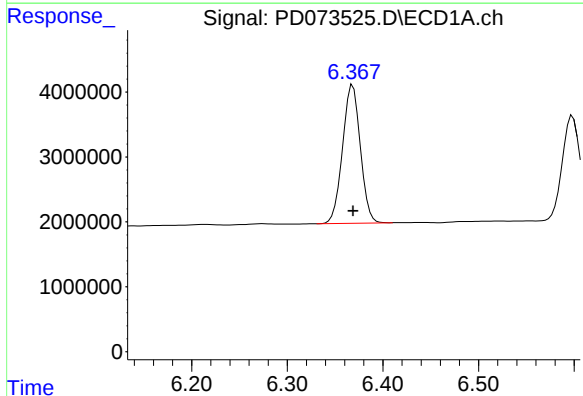


#13 Dieldrin

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 27662398
Conc: 8.66 ng/ml

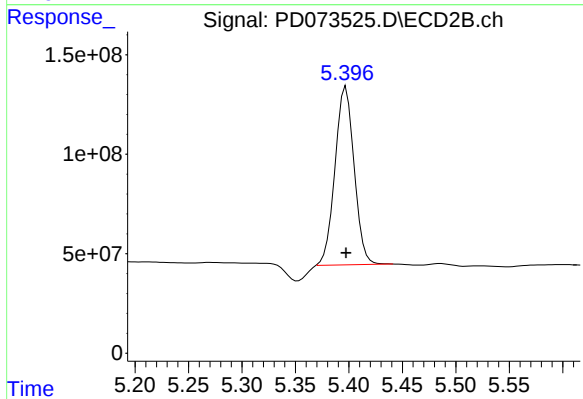


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 1117535870
Conc: 10.26 ng/ml

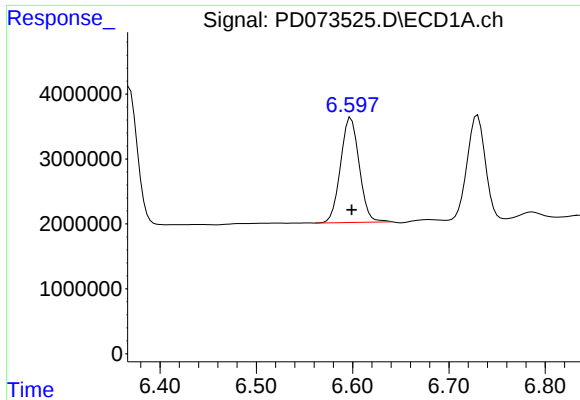


#14 Endrin

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 21728537
Conc: 8.64 ng/ml

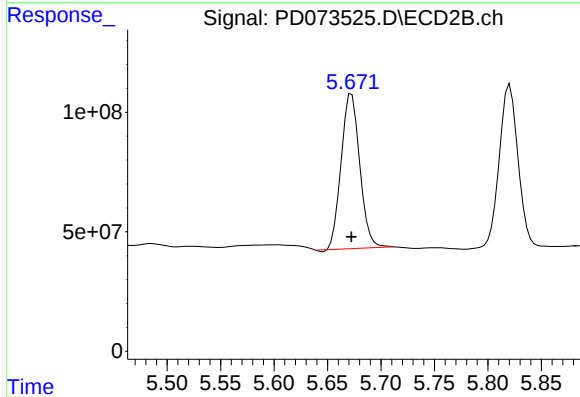


#14 Endrin

R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 786404955
Conc: 10.10 ng/ml

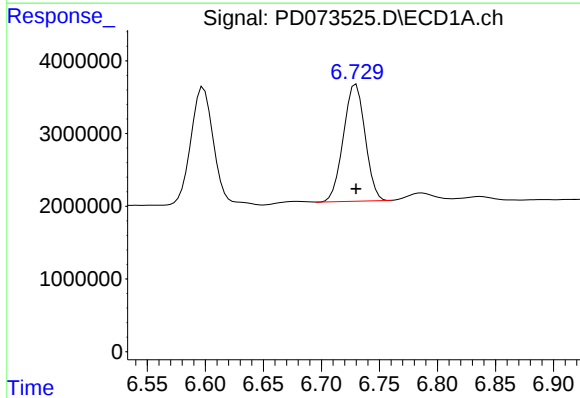


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 20914850
Conc: 8.62 ng/ml

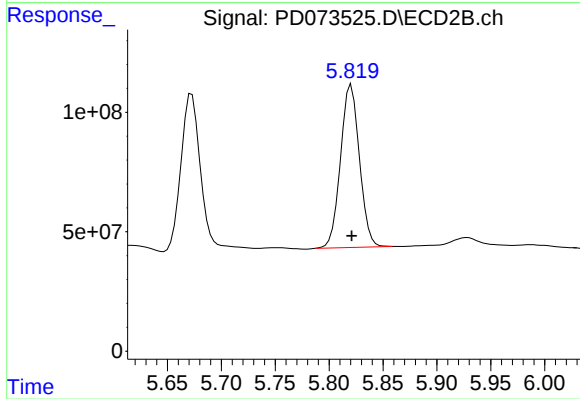


#16 4,4'-DDD

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 833625048
Conc: 10.31 ng/ml

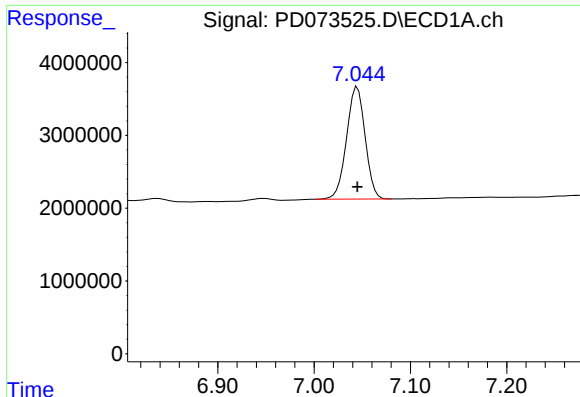


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 20601282
Conc: 8.73 ng/ml

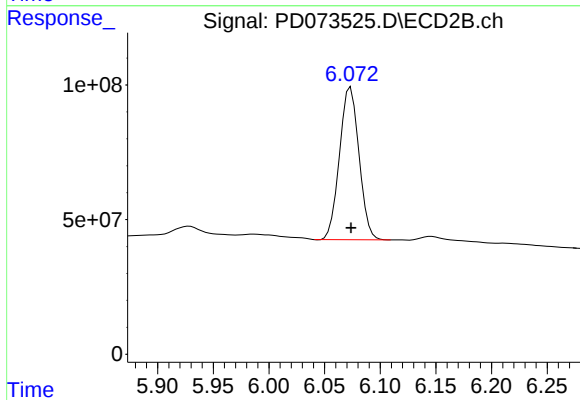


#17 4,4'-DDT

R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 690553425
Conc: 10.04 ng/ml

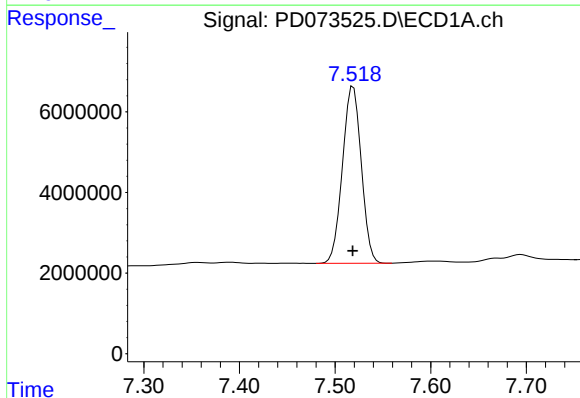


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 60170027
Conc: 45.20 ng/ml

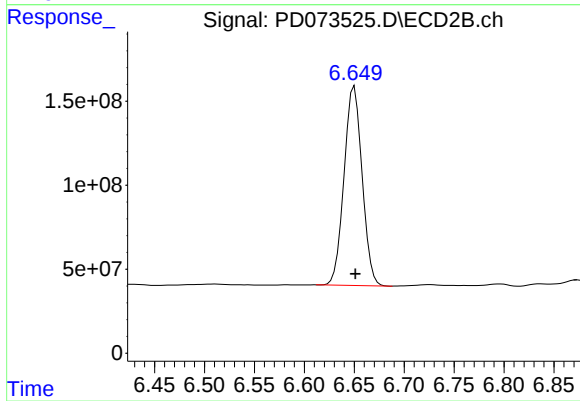

#20 Methoxychlor

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 1492953143
Conc: 52.33 ng/ml

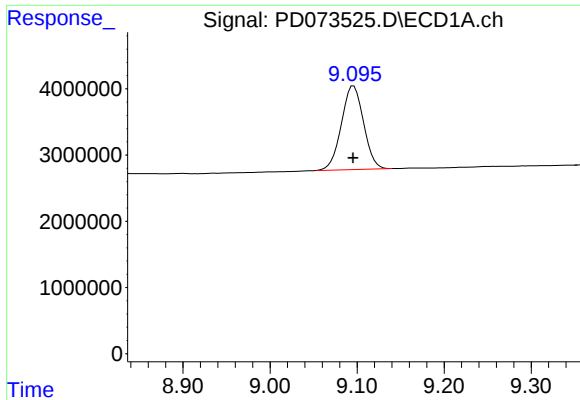


#27 Decachlorobiphenyl

R.T.: 9.096 min

Delta R.T.: 0.000 min

Response: 22455803

Conc: 9.84 ng/ml

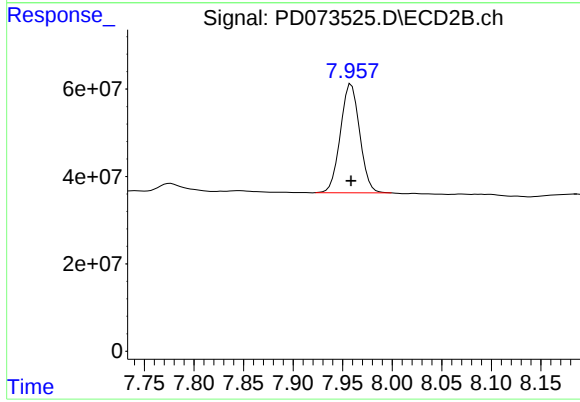

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 337586959

Conc: 10.29 ng/ml