

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 23:47
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:01:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 03:59:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	24937952	926.1E6	9.926	10.174
27)	SA Decachlor...	9.095	7.959	45502312	675.0E6	19.942	20.572
Target Compounds							
2)	A alpha-BHC	4.012	3.300	34786038	1447.7E6	9.278	9.926
3)	MA gamma-BHC...	4.345	3.630	33917489	1350.4E6	9.374	9.948
4)	MA Heptachlor	4.937	3.976	34673118	1345.4E6	9.462	9.993
9)	A Endosulfan I	6.092	5.132	28308341	1059.5E6	9.633	10.317
13)	MA Dieldrin	6.368	5.398	59317347	2177.4E6	18.562	19.995
14)	MA Endrin	6.598	5.672	45607218	1574.2E6	18.143	20.212
16)	A 4,4'-DDD	6.729	5.821	45321102	1647.1E6	18.677	20.367
17)	MA 4,4'-DDT	7.044	6.074	43821471	1404.2E6	18.578	20.408
20)	A Methoxychlor	7.519	6.651	126.3E6	2952.5E6	94.880	103.496


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 23:47
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:01:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 03:59:30 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

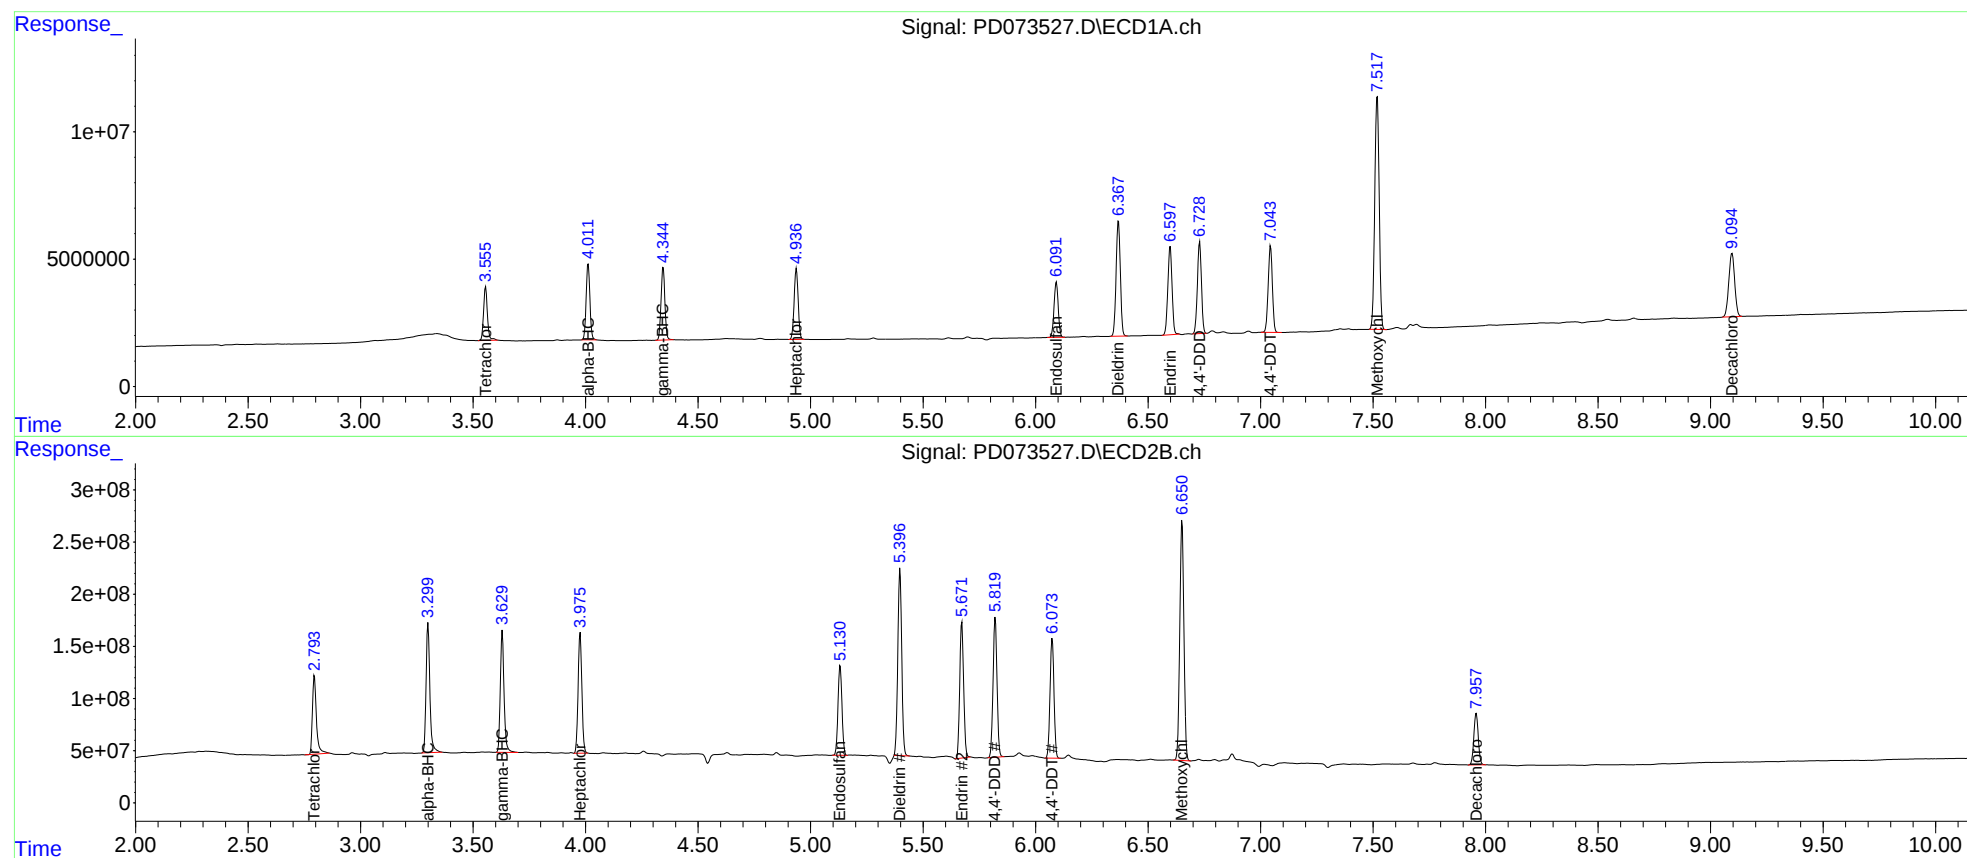

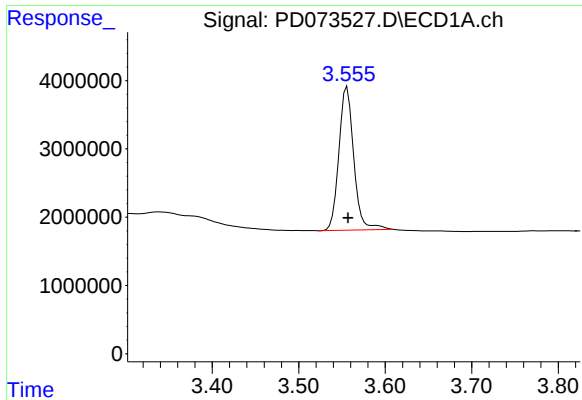


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 24937952
Conc: 9.93 ng/ml

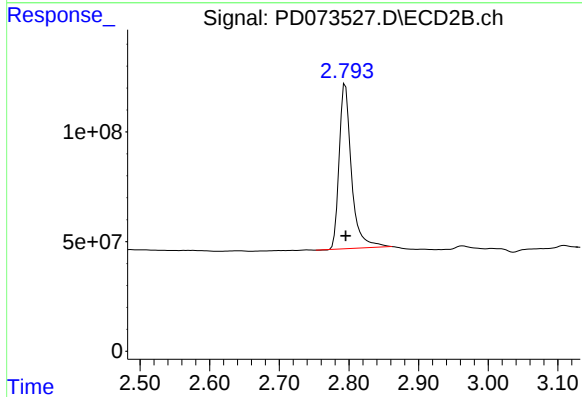


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 926137203
Conc: 10.17 ng/ml

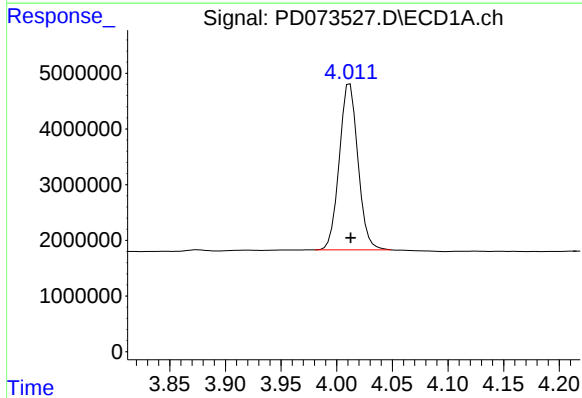


#2 alpha-BHC

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 34786038
Conc: 9.28 ng/ml

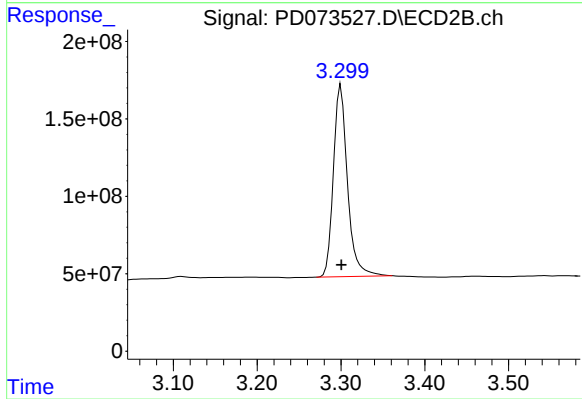


#2 alpha-BHC

R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 1447661480
Conc: 9.93 ng/ml

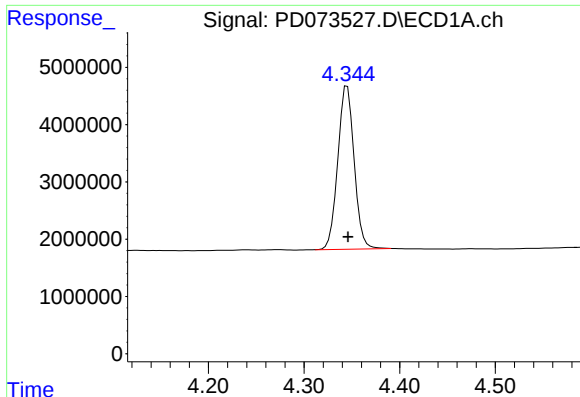


#3 gamma-BHC (Lindane)

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 33917489
Conc: 9.37 ng/ml

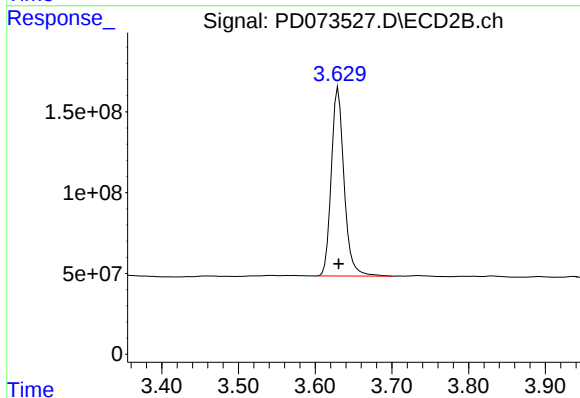


#3 gamma-BHC (Lindane)

R.T.: 3.630 min
Delta R.T.: 0.000 min
Response: 1350397882
Conc: 9.95 ng/ml

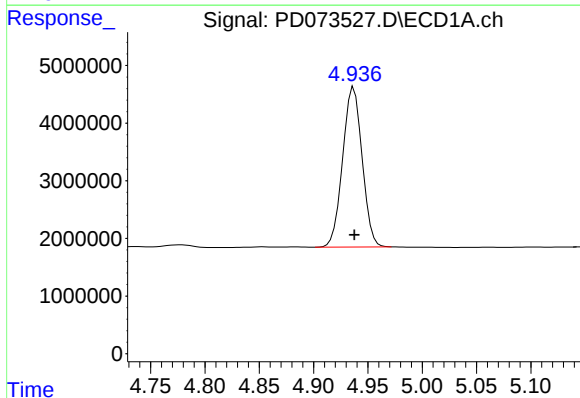


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 34673118
Conc: 9.46 ng/ml

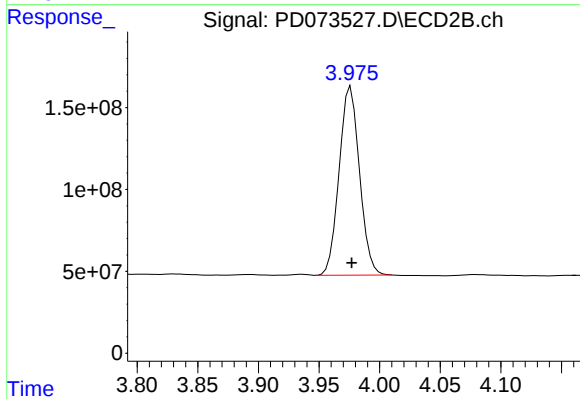


#4 Heptachlor

R.T.: 3.976 min
Delta R.T.: 0.000 min
Response: 1345402666
Conc: 9.99 ng/ml

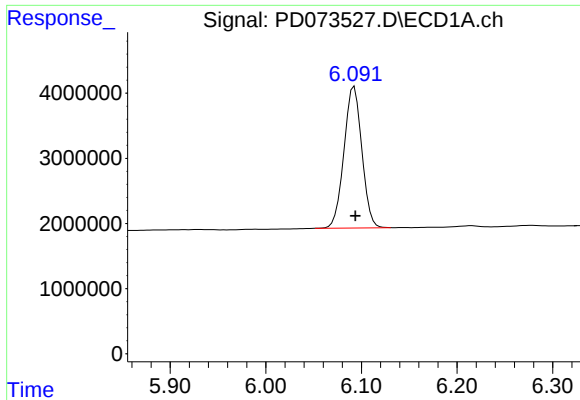


#9 Endosulfan I

R.T.: 6.092 min
Delta R.T.: -0.001 min
Response: 28308341
Conc: 9.63 ng/ml

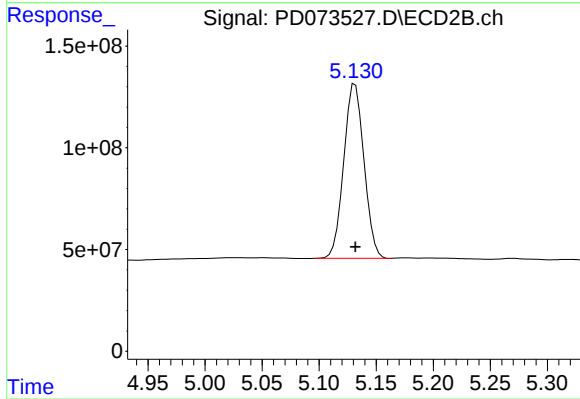


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 1059480054
Conc: 10.32 ng/ml

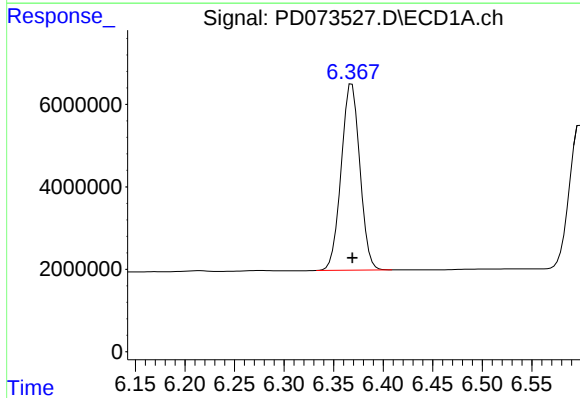


#13 Dieldrin

R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 59317347
Conc: 18.56 ng/ml

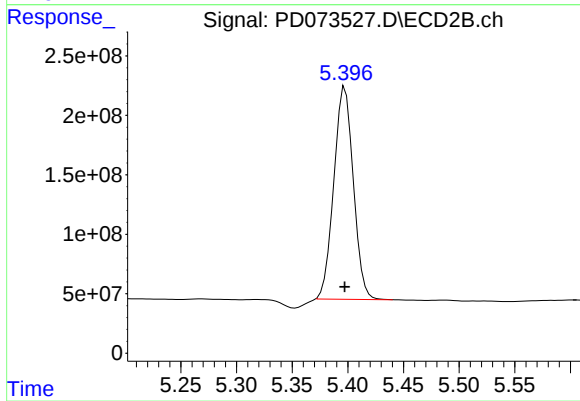


#13 Dieldrin

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 2177444177
Conc: 20.00 ng/ml

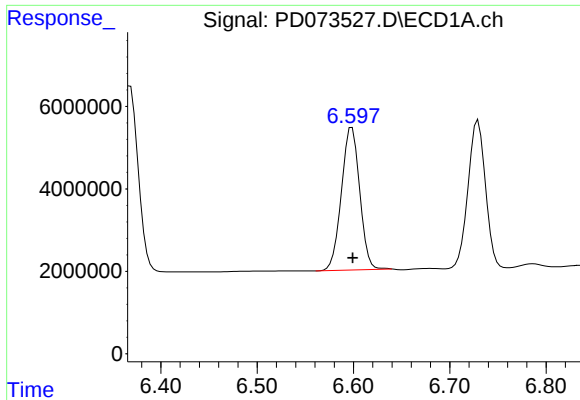


#14 Endrin

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 45607218
Conc: 18.14 ng/ml

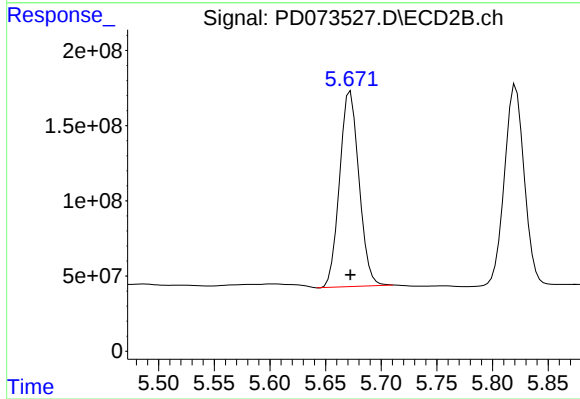


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 1574150770
Conc: 20.21 ng/ml

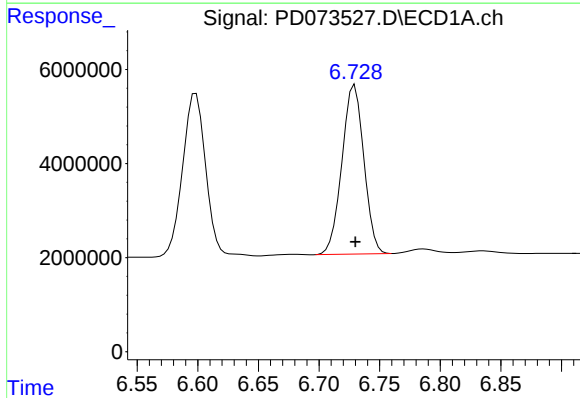


#16 4,4'-DDD

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 45321102
Conc: 18.68 ng/ml

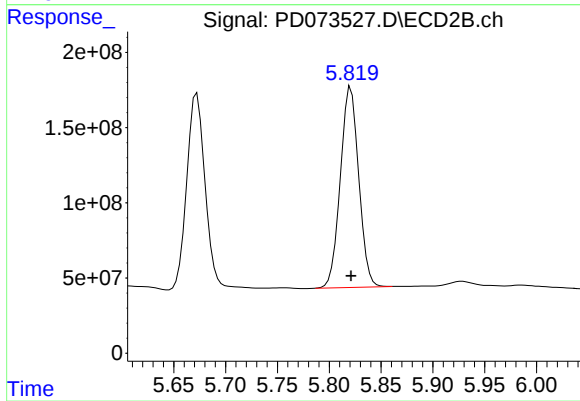


#16 4,4'-DDD

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 1647134984
Conc: 20.37 ng/ml

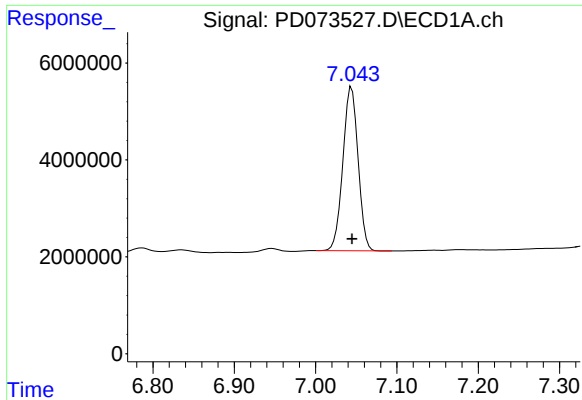


#17 4,4'-DDT

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 43821471
Conc: 18.58 ng/ml

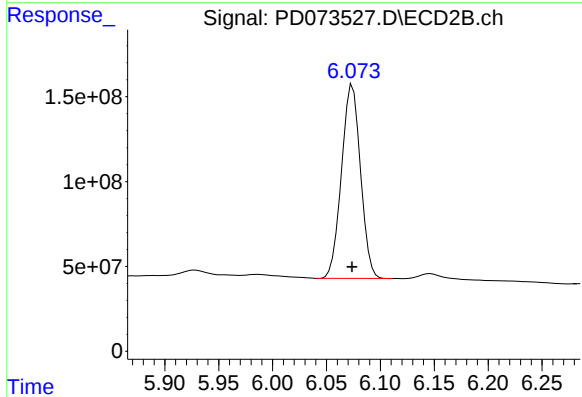


#17 4,4'-DDT

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1404223372
Conc: 20.41 ng/ml

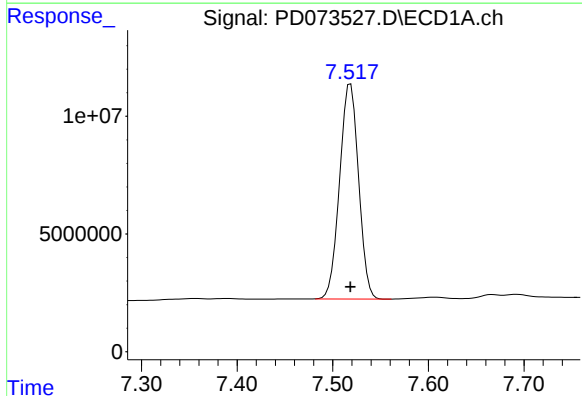


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 126312594
Conc: 94.88 ng/ml

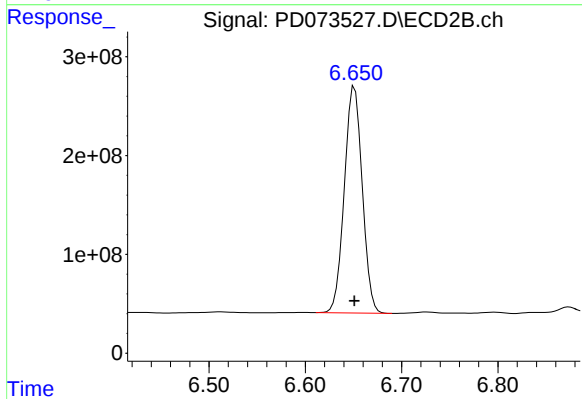


#20 Methoxychlor

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 2952475754
Conc: 103.50 ng/ml

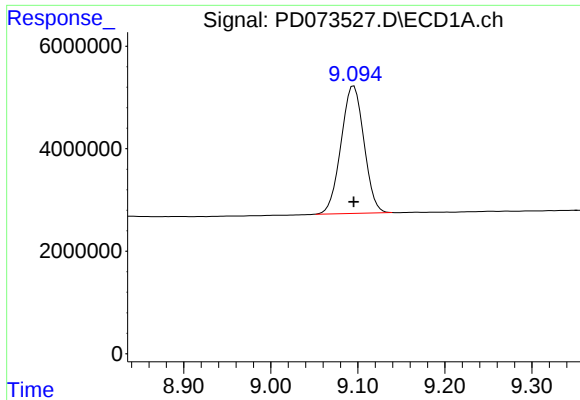

#27 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 45502312
Conc: 19.94 ng/ml

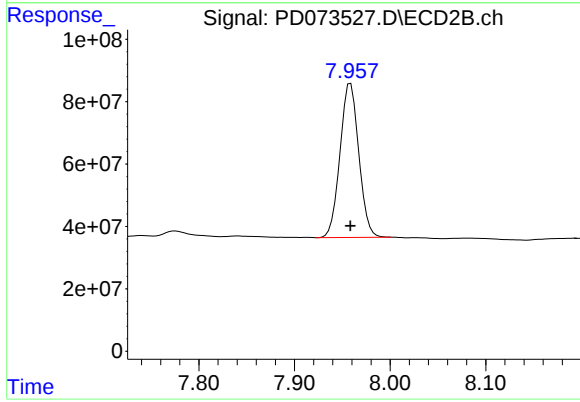

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 674991517
Conc: 20.57 ng/ml