

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 00:14
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:01:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 03:59:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.795	50249026	1820.6E6	20.000	20.000
27)	SA Decachlor...	9.095	7.959	91267382	1312.4E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.013	3.301	74989395	2916.8E6	20.000	20.000
3)	MA gamma-BHC...	4.346	3.631	72361831	2715.0E6	20.000	20.000
4)	MA Heptachlor	4.938	3.977	73291482	2692.6E6	20.000	20.000
9)	A Endosulfan I	6.094	5.132	58773008	2053.8E6	20.000	20.000
13)	MA Dieldrin	6.369	5.397	127.8E6	4355.9E6	40.000	40.000
14)	MA Endrin	6.599	5.672	100.6E6	3115.3E6	40.000	40.000
16)	A 4,4'-DDD	6.730	5.821	97062110	3235.0E6	40.000	40.000
17)	MA 4,4'-DDT	7.045	6.074	94351769	2752.3E6	40.000	40.000
20)	A Methoxychlor	7.519	6.651	266.3E6	5705.5E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 00:14
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:01:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 03:59:30 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

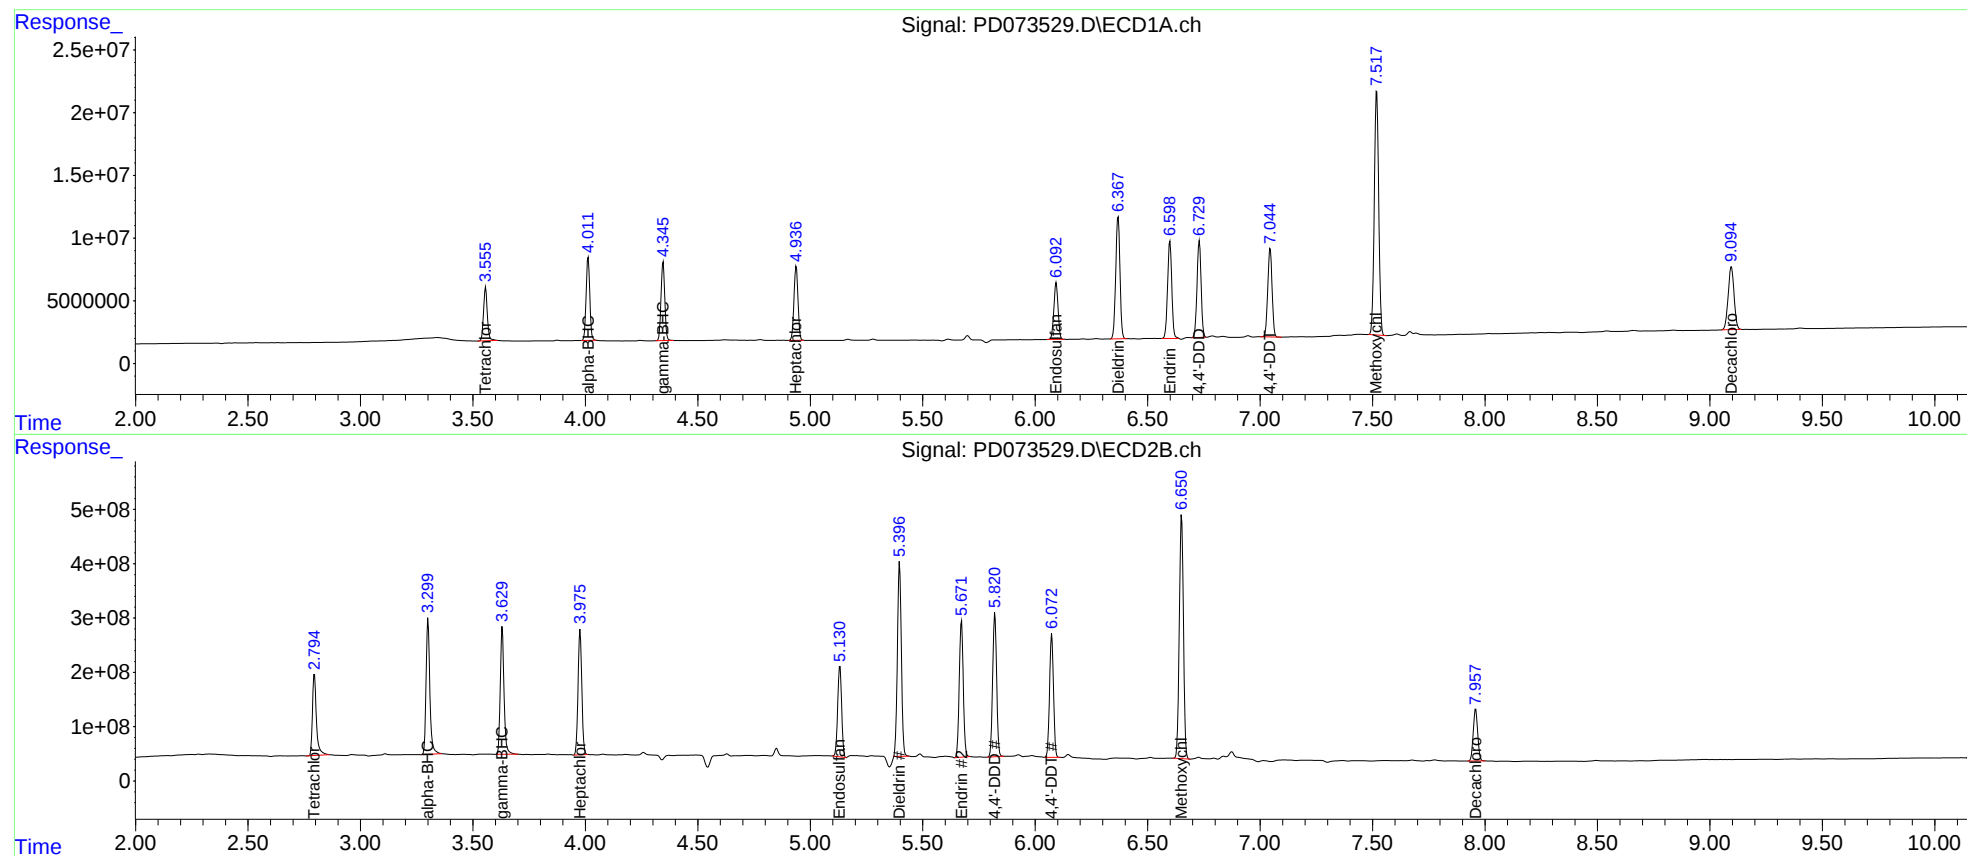

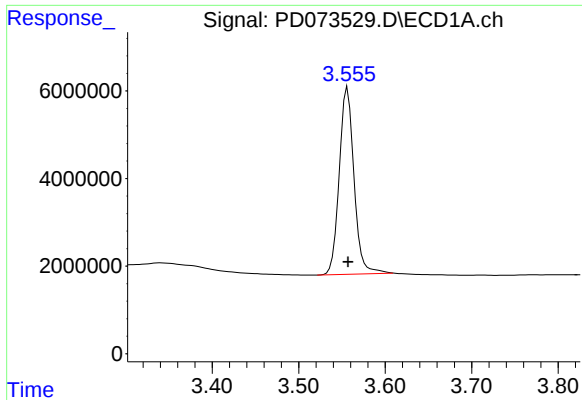


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 50249026
Conc: 20.00 ng/ml

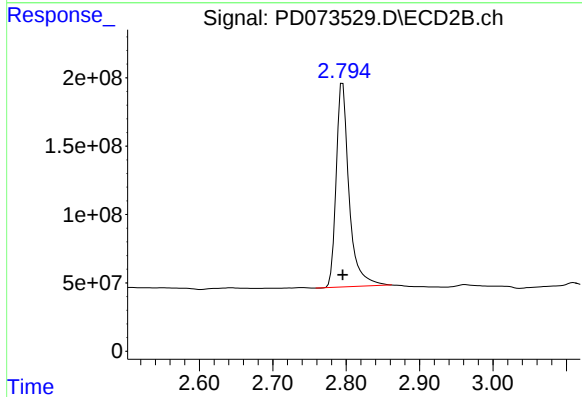


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 1820621228
Conc: 20.00 ng/ml

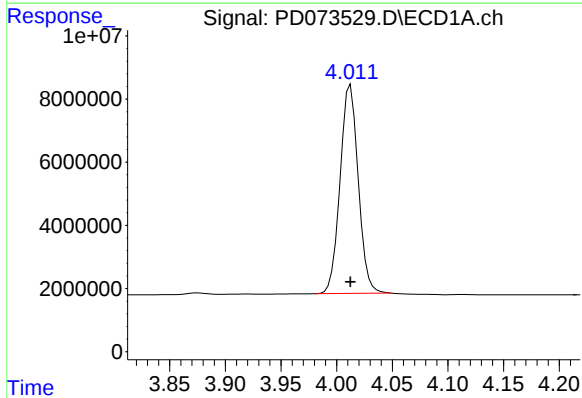


#2 alpha-BHC

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 74989395
Conc: 20.00 ng/ml

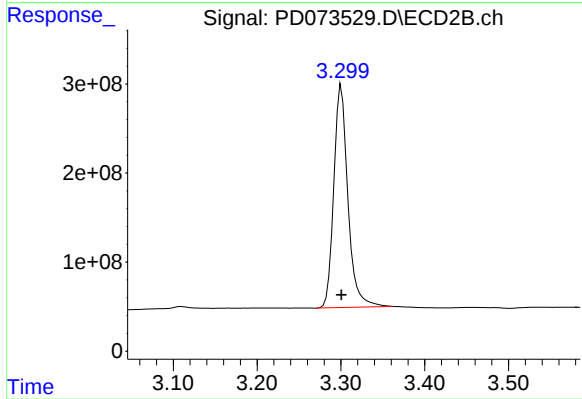


#2 alpha-BHC

R.T.: 3.301 min
Delta R.T.: 0.000 min
Response: 2916778815
Conc: 20.00 ng/ml

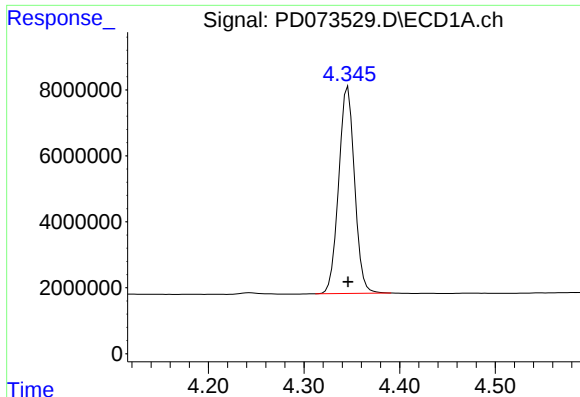


#3 gamma-BHC (Lindane)

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 72361831
Conc: 20.00 ng/ml

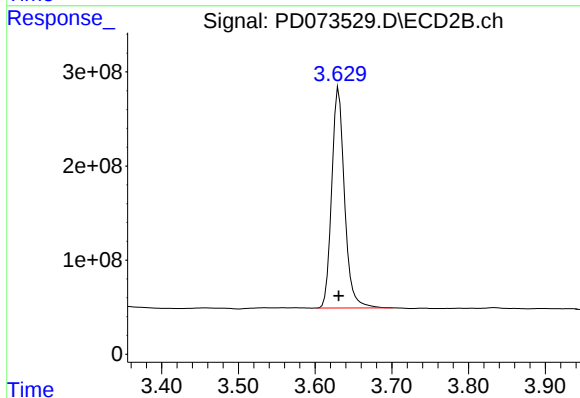


#3 gamma-BHC (Lindane)

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 2714950800
Conc: 20.00 ng/ml

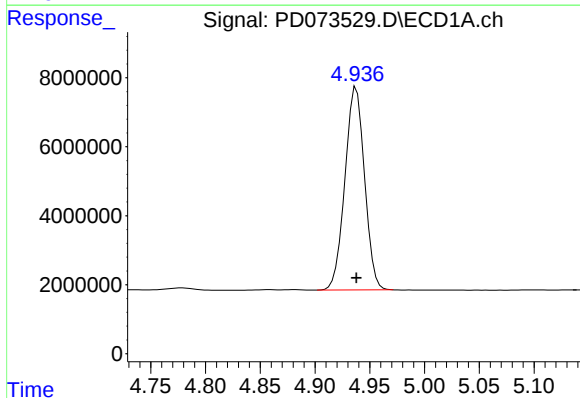


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 73291482
Conc: 20.00 ng/ml

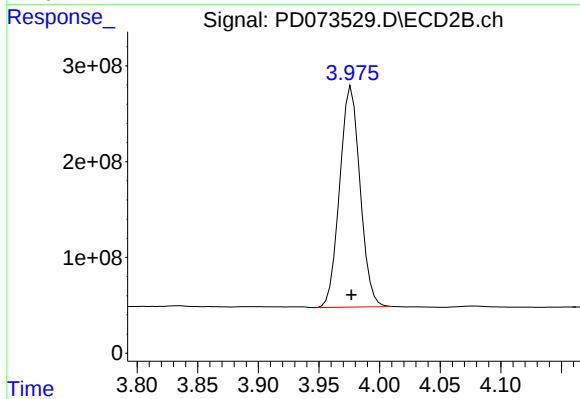


#4 Heptachlor

R.T.: 3.977 min
Delta R.T.: 0.000 min
Response: 2692619932
Conc: 20.00 ng/ml

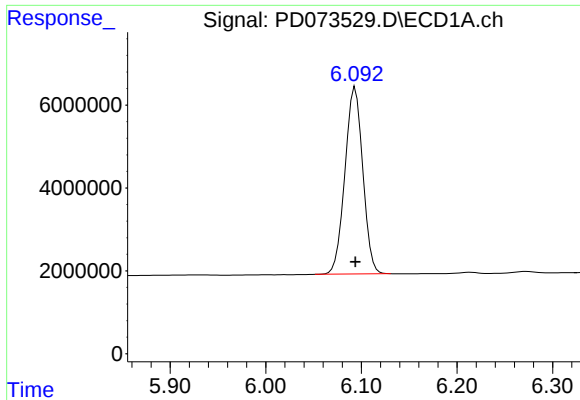


#9 Endosulfan I

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 58773008
Conc: 20.00 ng/ml

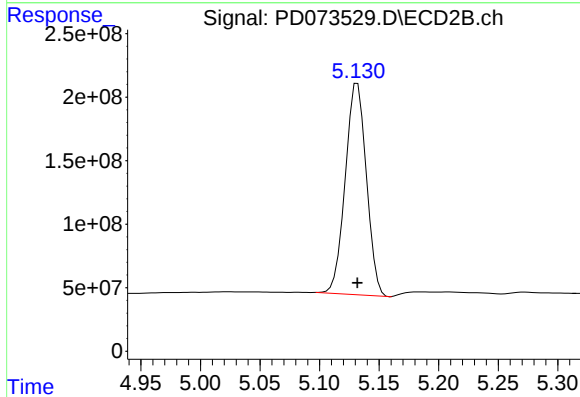


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 2053784084
Conc: 20.00 ng/ml

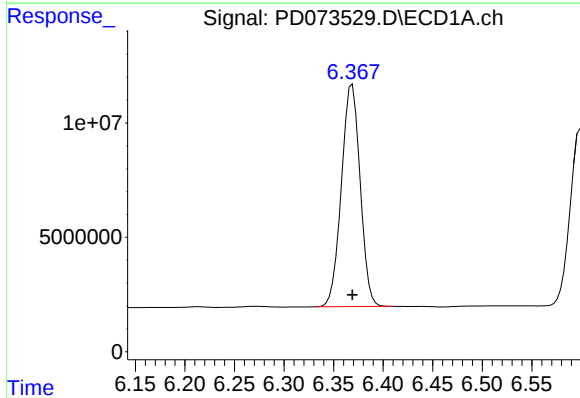


#13 Dieldrin

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 127825147
Conc: 40.00 ng/ml

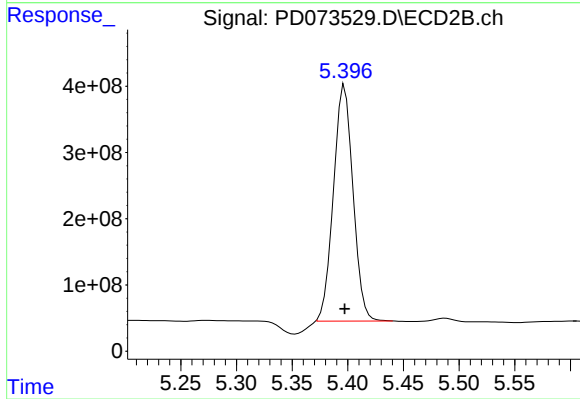


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 4355872550
Conc: 40.00 ng/ml

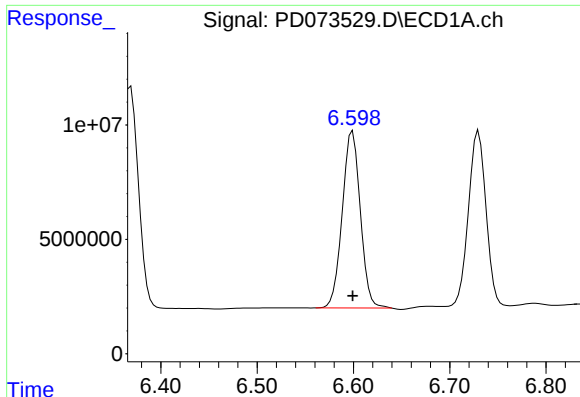


#14 Endrin

R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 100550460
Conc: 40.00 ng/ml

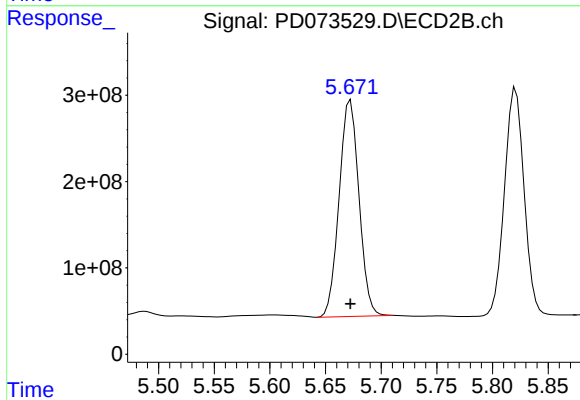


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 3115252776
Conc: 40.00 ng/ml

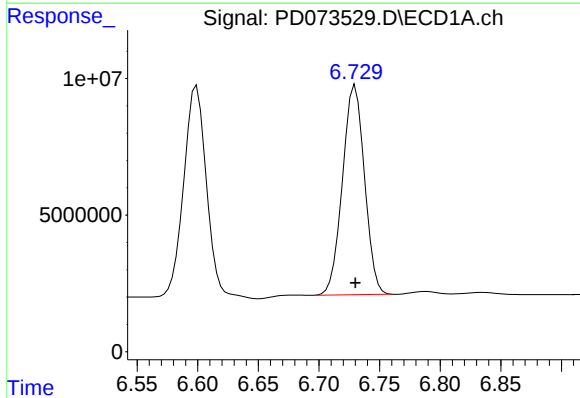


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 97062110
Conc: 40.00 ng/ml

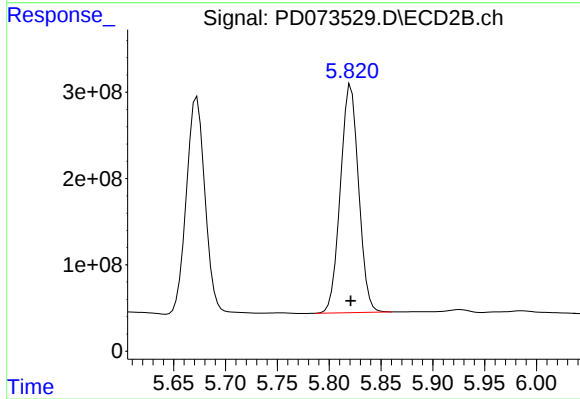


#16 4,4'-DDD

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 3234983723
Conc: 40.00 ng/ml

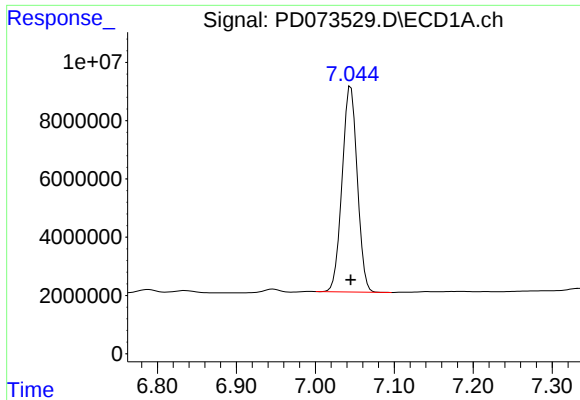


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 94351769
Conc: 40.00 ng/ml

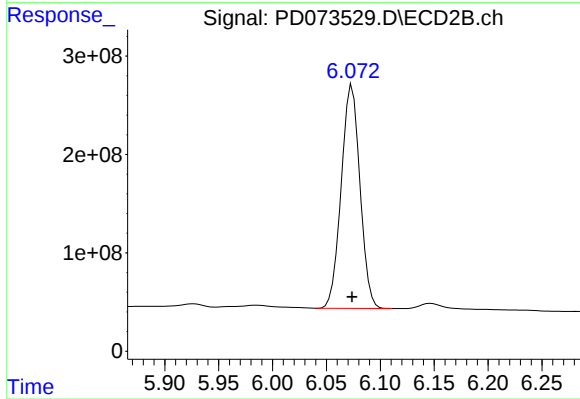


#17 4,4'-DDT

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 2752272009
Conc: 40.00 ng/ml

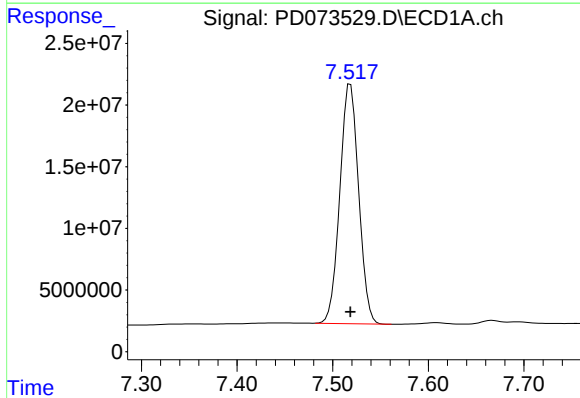


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 266256807
Conc: 200.00 ng/ml

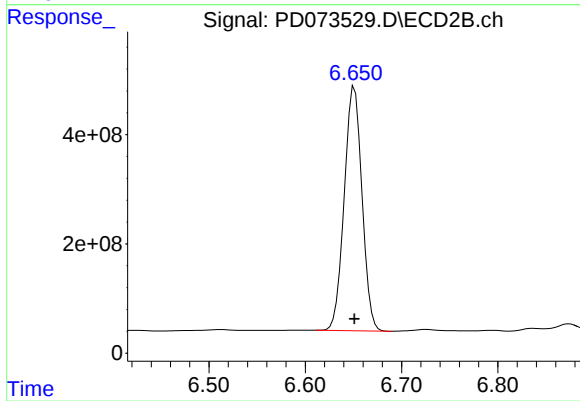

#20 Methoxychlor

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 5705503363
Conc: 200.00 ng/ml

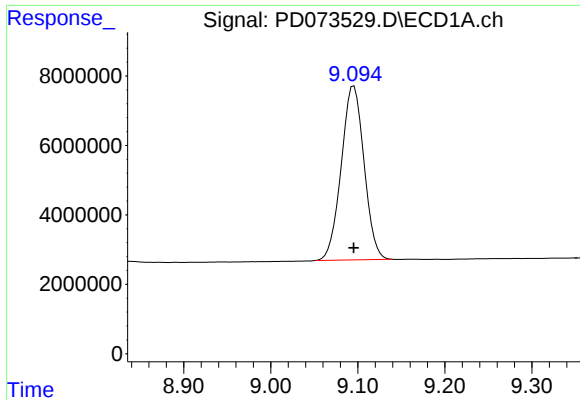


#27 Decachlorobiphenyl

R.T.: 9.095 min

Delta R.T.: 0.000 min

Response: 91267382

Conc: 40.00 ng/ml

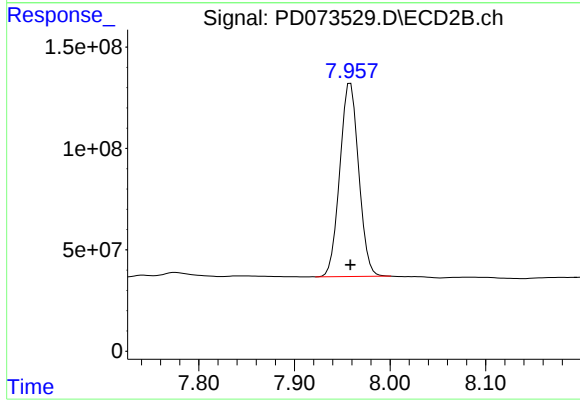

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 1312440777

Conc: 40.00 ng/ml