

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 00:41
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:02:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 03:59:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	98456035	3352.2E6	39.187	36.825
27)	SA Decachlor...	9.095	7.959	175.7E6	2502.1E6	77.009	76.258
Target Compounds							
2)	A alpha-BHC	4.013	3.300	156.2E6	5577.8E6	41.670	38.246
3)	MA gamma-BHC...	4.346	3.630	148.2E6	5161.8E6	40.961	38.025
4)	MA Heptachlor	4.938	3.977	149.6E6	5047.2E6	40.828	37.489
9)	A Endosulfan I	6.093	5.132	118.4E6	3952.7E6	40.304	38.492
13)	MA Dieldrin	6.369	5.397	267.0E6	8431.8E6	83.540	77.429
14)	MA Endrin	6.599	5.672	202.6E6	5716.2E6	80.577	73.397
16)	A 4,4'-DDD	6.730	5.820	201.1E6	6222.2E6	82.875	76.936
17)	MA 4,4'-DDT	7.045	6.074	195.0E6	5114.7E6	82.650	74.335
20)	A Methoxychlor	7.519	6.651	539.2E6	10559.4E6	405.032	370.148


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 00:41
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:02:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 03:59:30 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

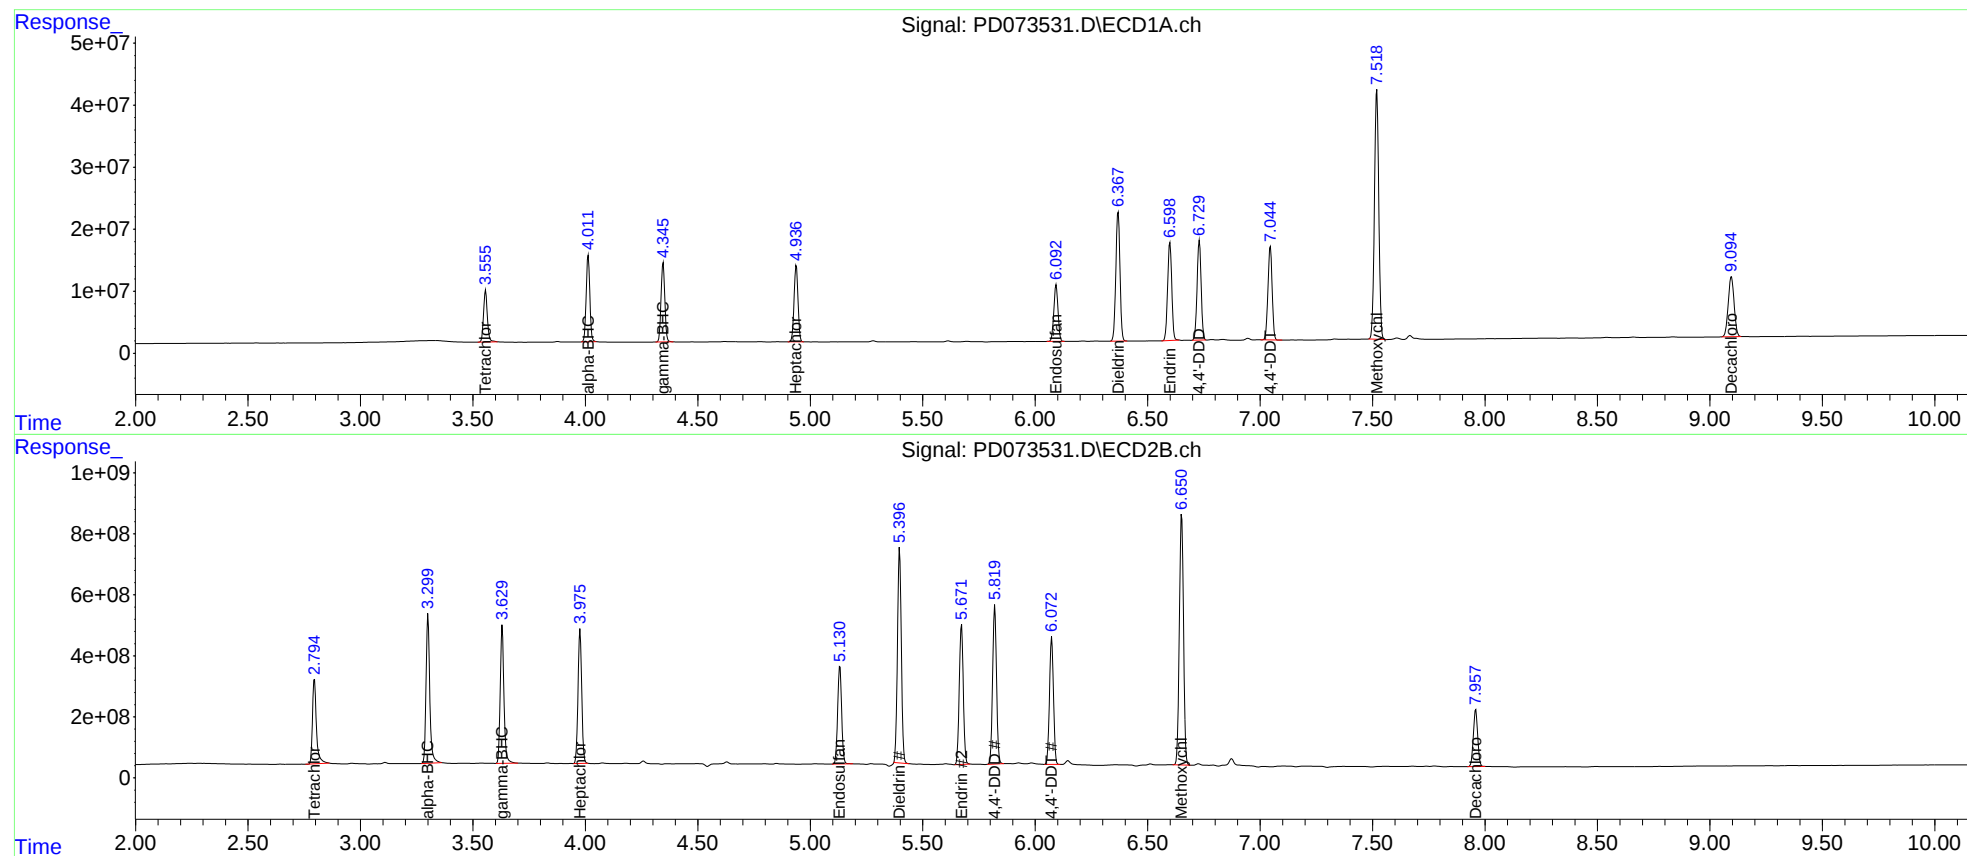

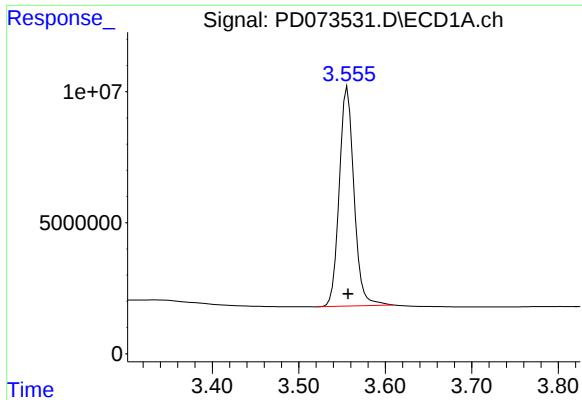


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 98456035
Conc: 39.19 ng/ml

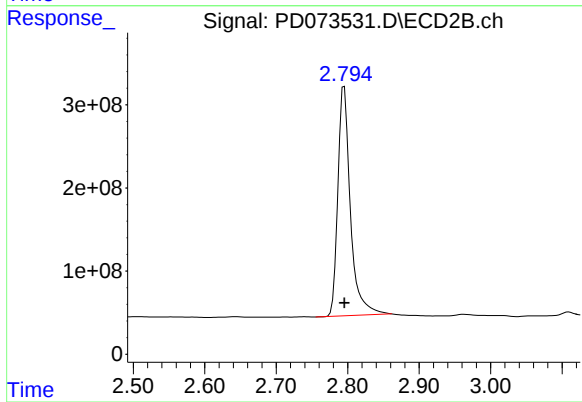


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 3352228189
Conc: 36.83 ng/ml

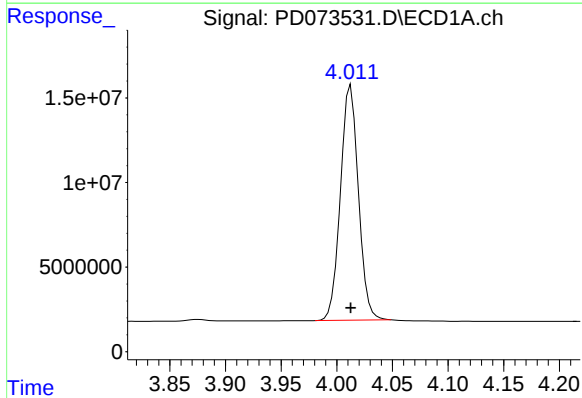


#2 alpha-BHC

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 156241004
Conc: 41.67 ng/ml

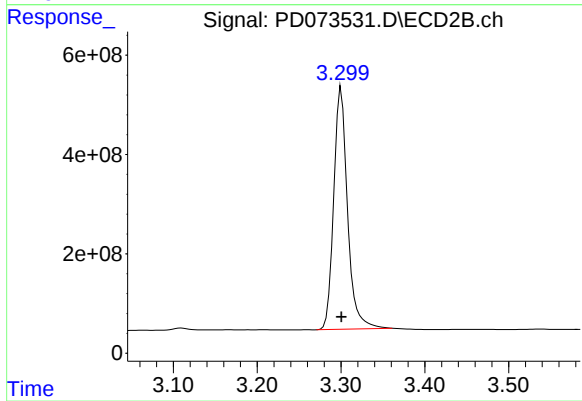


#2 alpha-BHC

R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 5577759626
Conc: 38.25 ng/ml

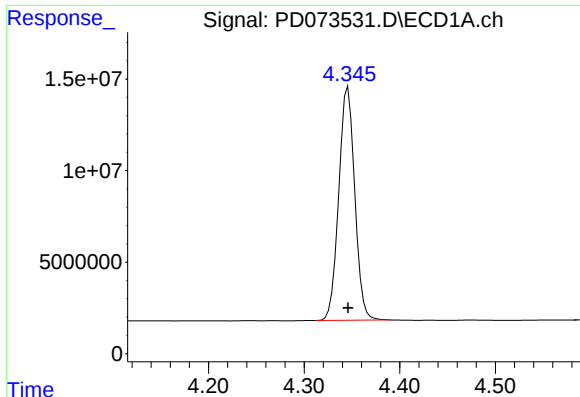


#3 gamma-BHC (Lindane)

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 148200081
Conc: 40.96 ng/ml

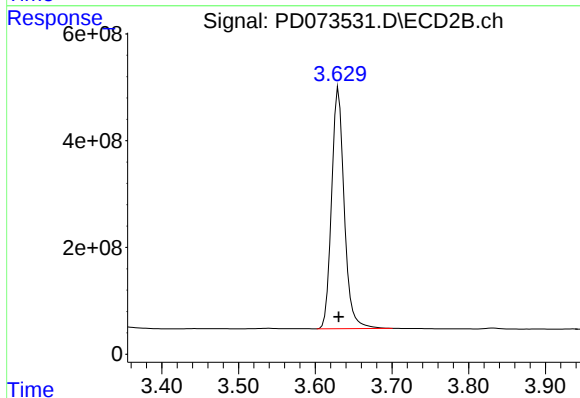


#3 gamma-BHC (Lindane)

R.T.: 3.630 min
Delta R.T.: 0.000 min
Response: 5161784215
Conc: 38.02 ng/ml

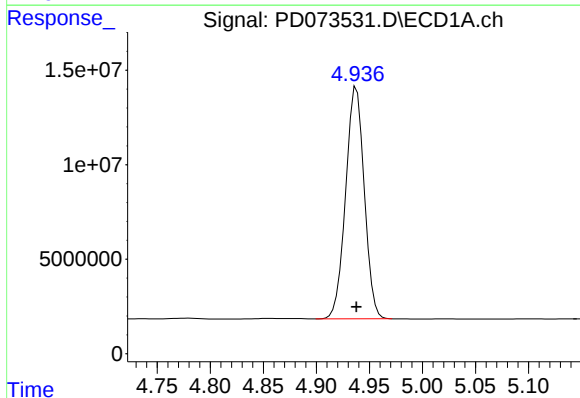


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 149616836
Conc: 40.83 ng/ml

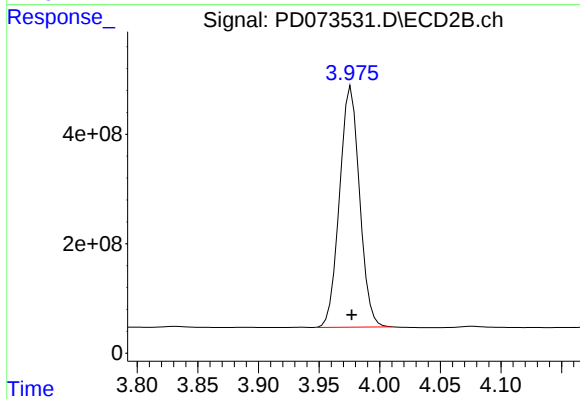


#4 Heptachlor

R.T.: 3.977 min
Delta R.T.: 0.000 min
Response: 5047170632
Conc: 37.49 ng/ml

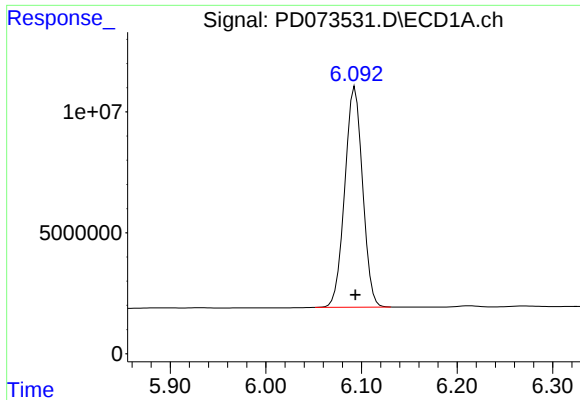


#9 Endosulfan I

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 118440808
Conc: 40.30 ng/ml

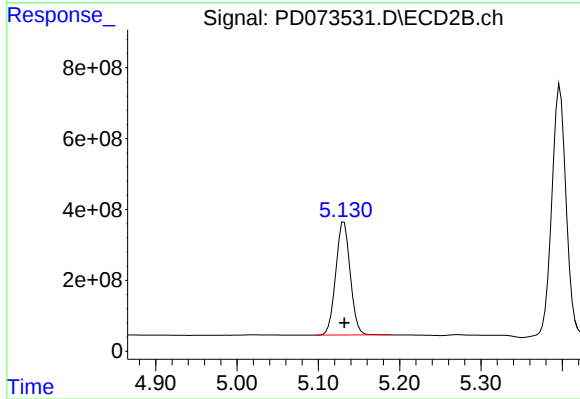


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 3952670799
Conc: 38.49 ng/ml

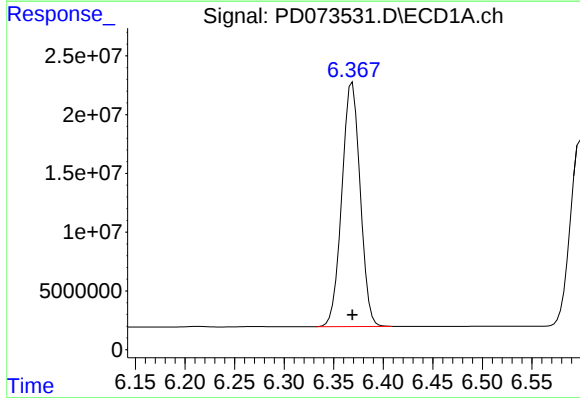


#13 Dieldrin

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 266962907
Conc: 83.54 ng/ml

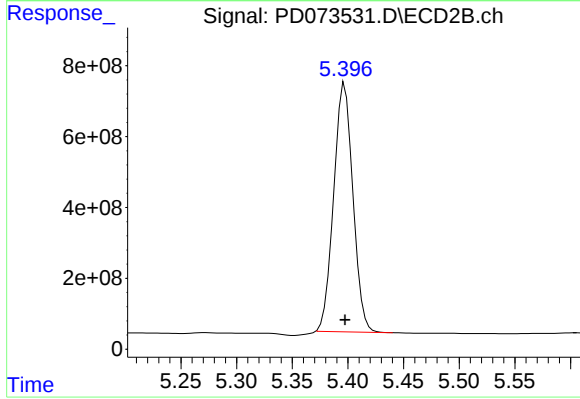


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 8431814893
Conc: 77.43 ng/ml

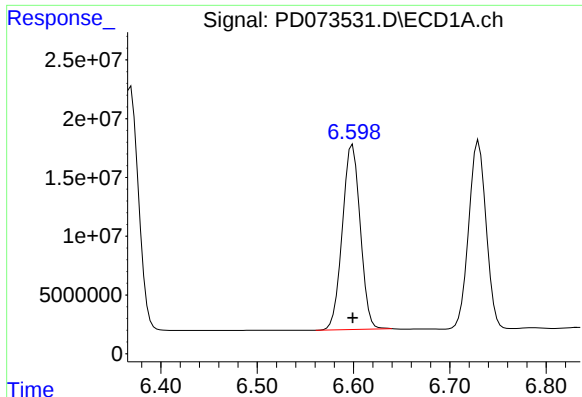


#14 Endrin

R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 202550744
Conc: 80.58 ng/ml

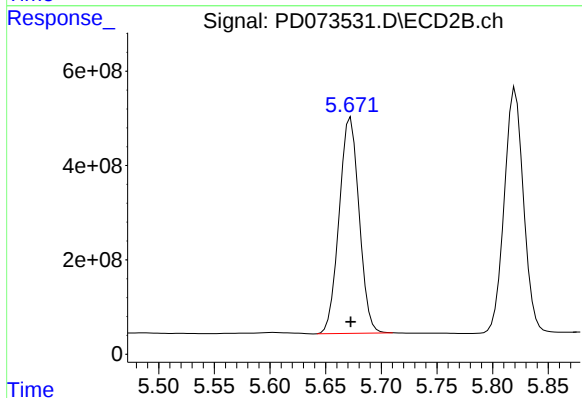


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 5716242326
Conc: 73.40 ng/ml

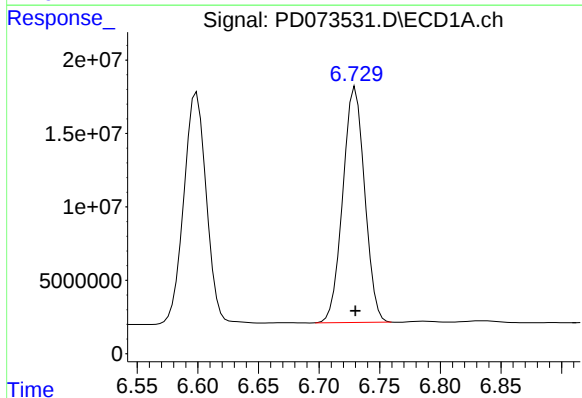


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 201101003
Conc: 82.88 ng/ml

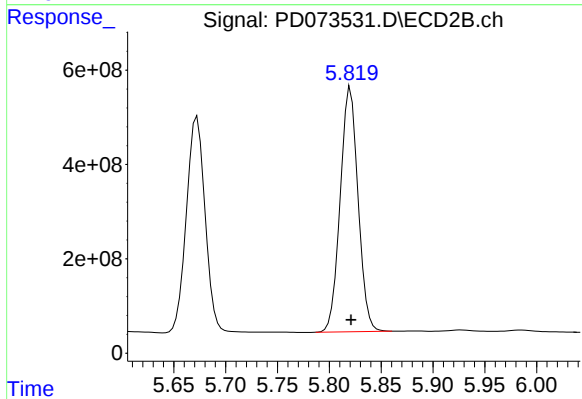


#16 4,4'-DDD

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 6222165410
Conc: 76.94 ng/ml

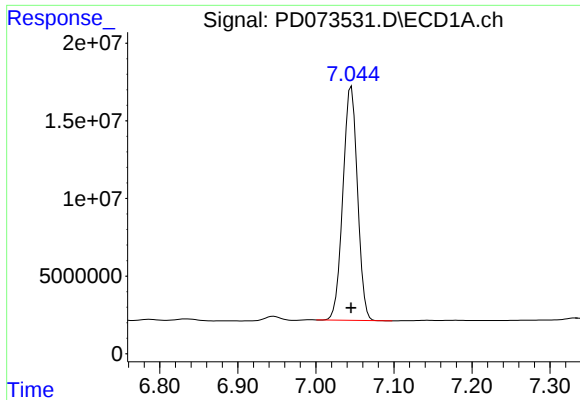


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 194953654
Conc: 82.65 ng/ml

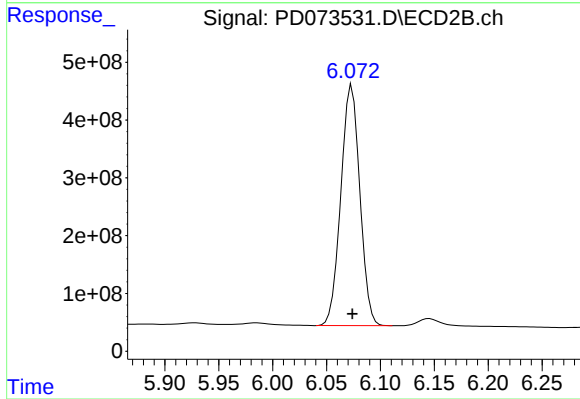


#17 4,4'-DDT

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 5114742026
Conc: 74.33 ng/ml

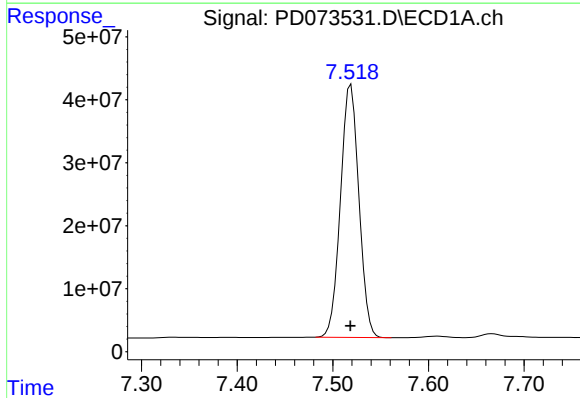


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 539212238
Conc: 405.03 ng/ml

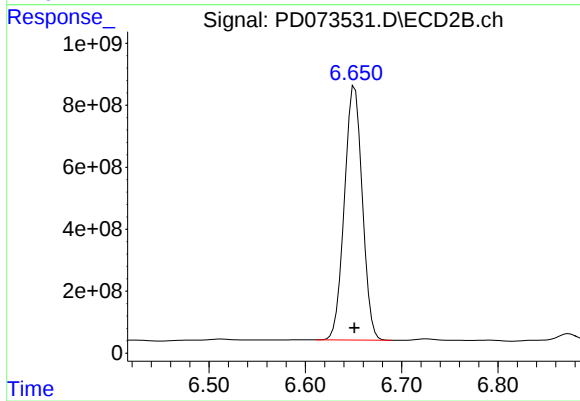

#20 Methoxychlor

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 10559394793
Conc: 370.15 ng/ml

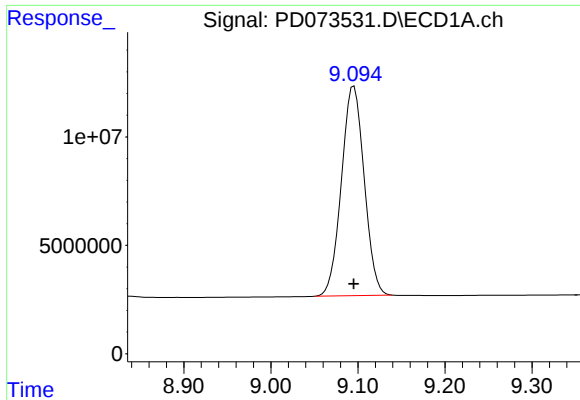


#27 Decachlorobiphenyl

R.T.: 9.095 min

Delta R.T.: 0.000 min

Response: 175709478

Conc: 77.01 ng/ml

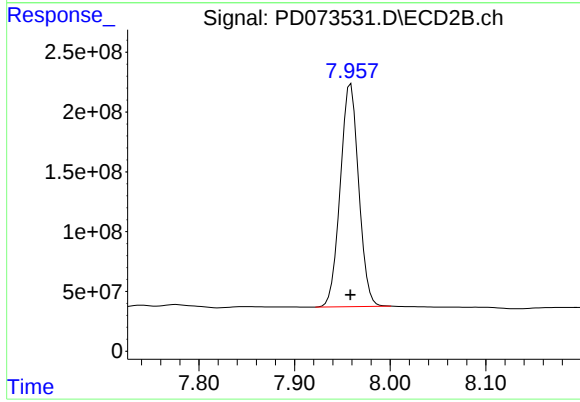

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 2502116588

Conc: 76.26 ng/ml