

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 00:54
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 03:03:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 02:59:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	95150454	3364.6E6	38.226	37.055
27)	SA Decachlor...	9.095	7.959	174.9E6	2530.0E6	75.344	76.059
Target Compounds							
5)	MB Aldrin	5.282	4.258	141.9E6	5235.6E6	39.842	37.446
6)	B beta-BHC	4.538	3.924	62526047	2056.0E6	37.464	36.673
7)	B delta-BHC	4.787	4.157	150.6E6	5421.2E6	40.094	38.051
8)	B Heptachlo...	5.707	4.761	129.6E6	4413.5E6	39.502	36.972
10)	B trans-Chl...	5.963	5.012	122.5E6	4482.4E6	39.389	37.739
11)	B cis-Chlor...	6.043	5.077	124.5E6	4415.0E6	38.995	37.531
12)	B 4,4'-DDE	6.213	5.267	243.9E6	7798.2E6	80.855	73.383
15)	B Endosulfa...	6.816	5.965	212.3E6	6133.1E6	79.328	76.227
18)	B Endrin al...	6.947	6.145	161.4E6	4597.8E6	77.569	74.478
19)	B Endosulfa...	7.181	6.368	196.3E6	5304.7E6	78.397	75.002
21)	B Endrin ke...	7.667	6.874	219.5E6	4813.9E6	77.990	75.442


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 00:54
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 03:03:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 02:59:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

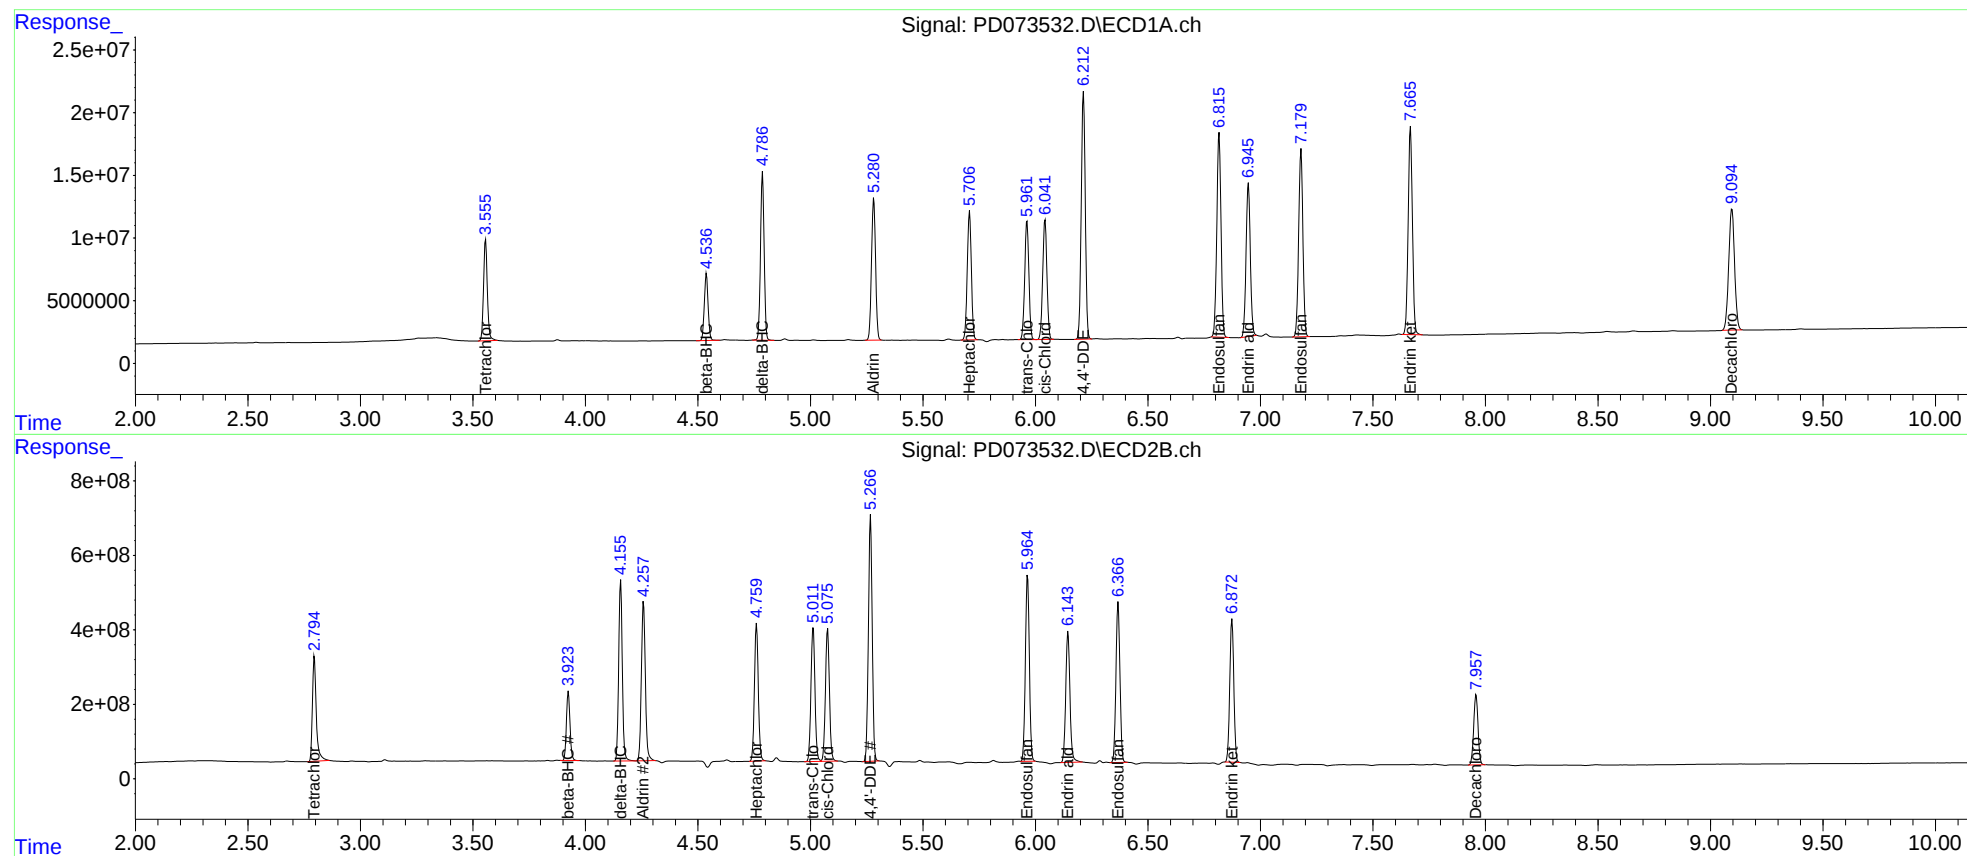

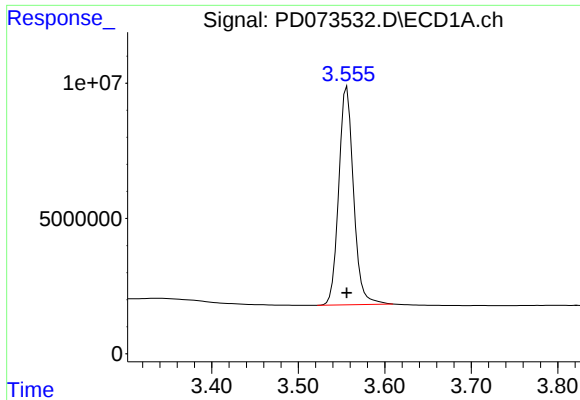


#1 Tetrachloro-m-xylene

R.T.: 3.556 min

Delta R.T.: 0.000 min

Response: 95150454

Conc: 38.23 ng/ml

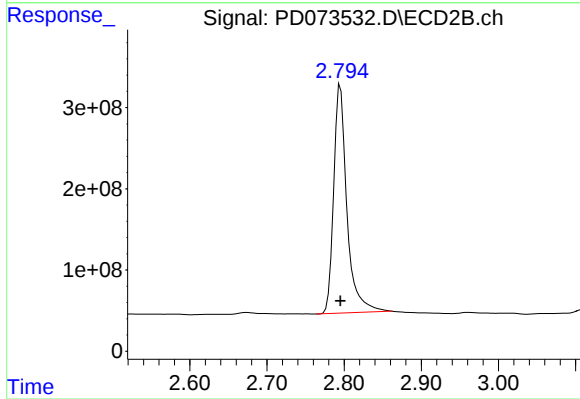


#1 Tetrachloro-m-xylene

R.T.: 2.795 min

Delta R.T.: 0.000 min

Response: 3364578420

Conc: 37.06 ng/ml

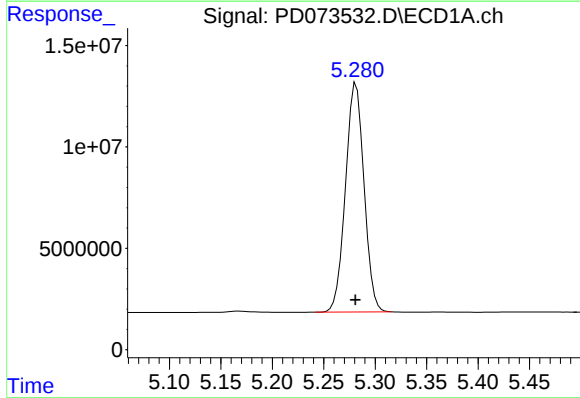


#5 Aldrin

R.T.: 5.282 min

Delta R.T.: 0.000 min

Response: 141895921

Conc: 39.84 ng/ml

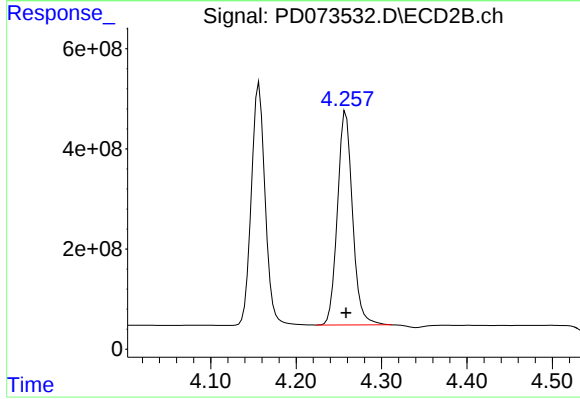


#5 Aldrin

R.T.: 4.258 min

Delta R.T.: 0.000 min


Response: 5235630481

Conc: 37.45 ng/ml

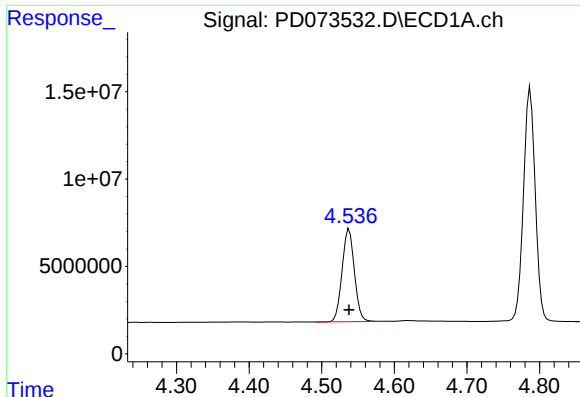


#6 beta-BHC

R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 62526047
Conc: 37.46 ng/ml

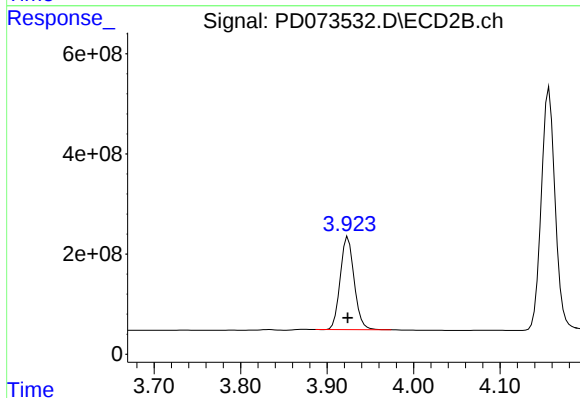


#6 beta-BHC

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 2056012204
Conc: 36.67 ng/ml

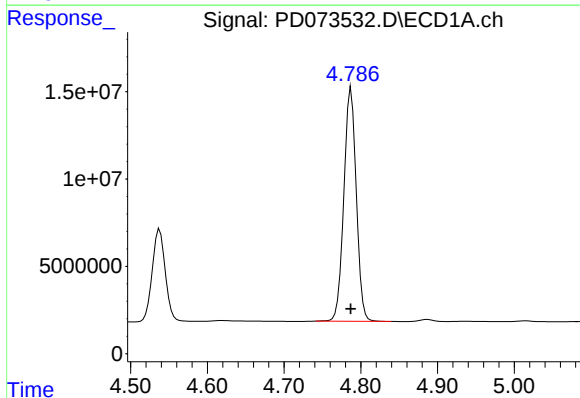


#7 delta-BHC

R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 150619335
Conc: 40.09 ng/ml

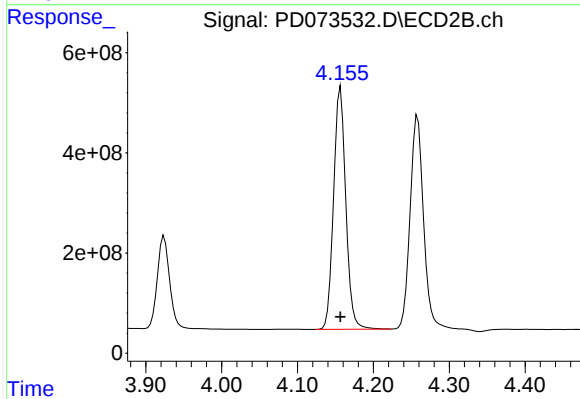


#7 delta-BHC

R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 5421218165
Conc: 38.05 ng/ml

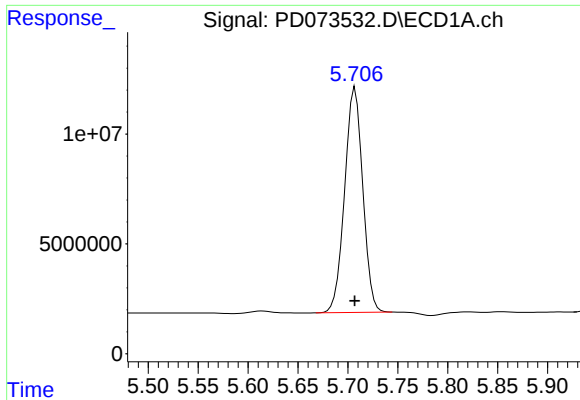


#8 Heptachlor epoxide

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 129633061
Conc: 39.50 ng/ml

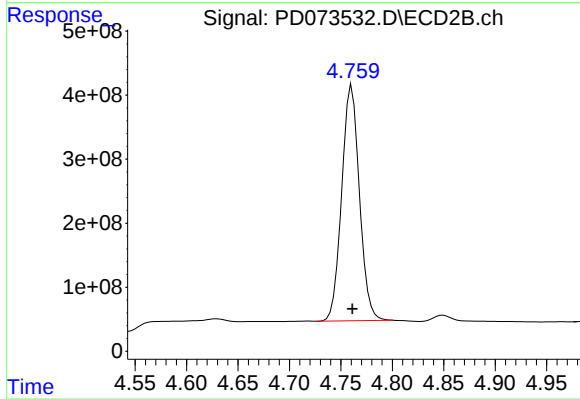


#8 Heptachlor epoxide

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 4413513501
Conc: 36.97 ng/ml

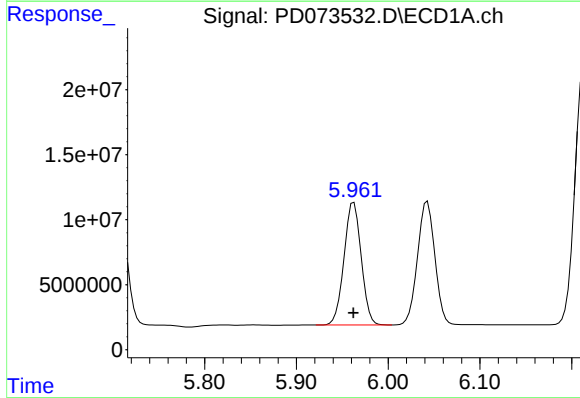


#10 trans-Chlordane

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 122483263
Conc: 39.39 ng/ml

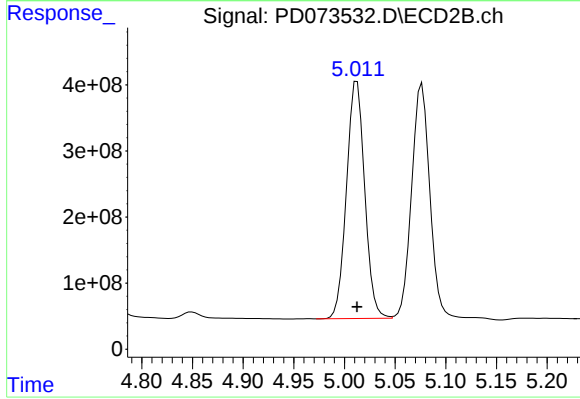


#10 trans-Chlordane

R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 4482395522
Conc: 37.74 ng/ml

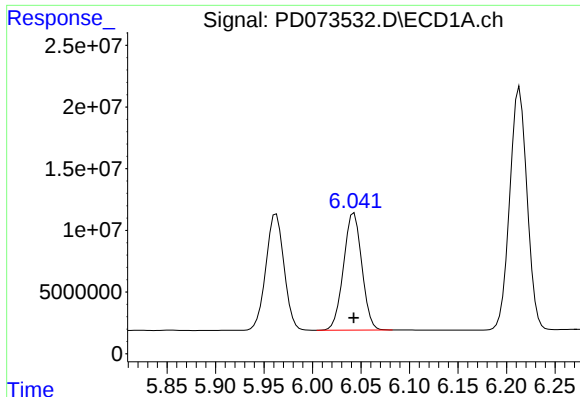


#11 cis-Chlordane

R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 124493450
Conc: 39.00 ng/ml

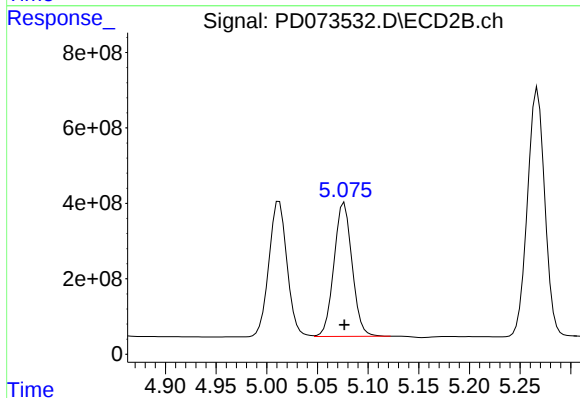


#11 cis-Chlordane

R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 4414953100
Conc: 37.53 ng/ml

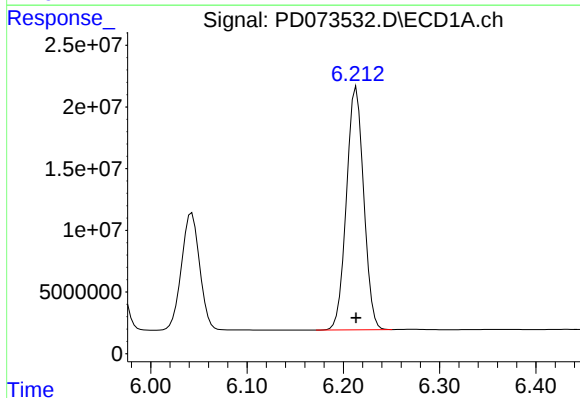


#12 4,4'-DDE

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 243904189
Conc: 80.85 ng/ml

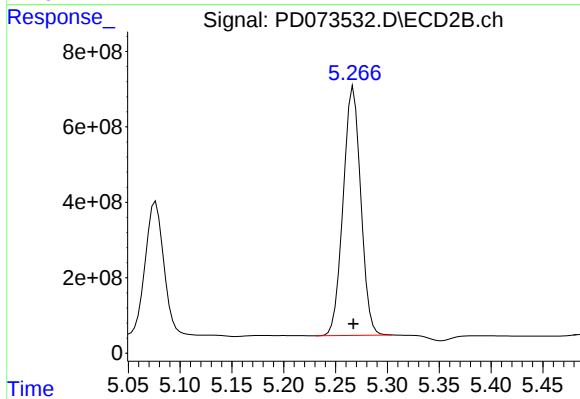


#12 4,4'-DDE

R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 7798211777
Conc: 73.38 ng/ml

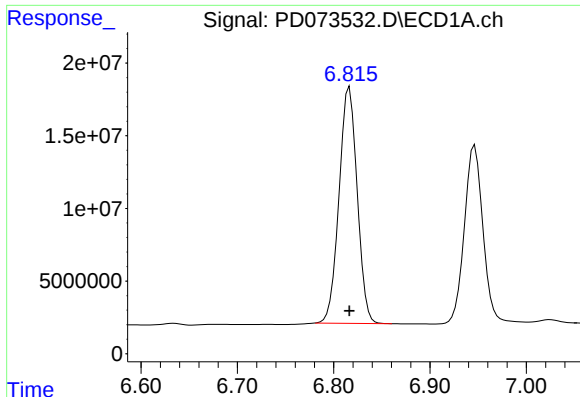


#15 Endosulfan II

R.T.: 6.816 min
Delta R.T.: 0.000 min
Response: 212310047
Conc: 79.33 ng/ml

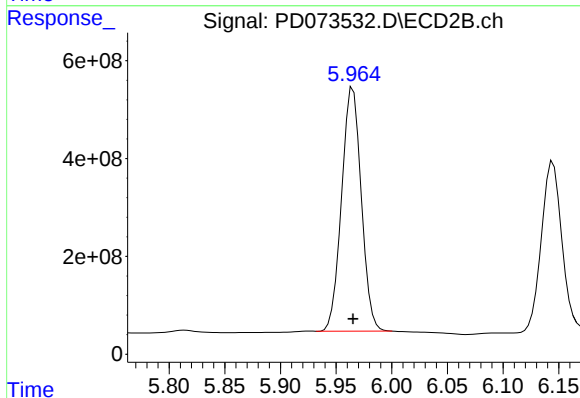


#15 Endosulfan II

R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 6133088452
Conc: 76.23 ng/ml

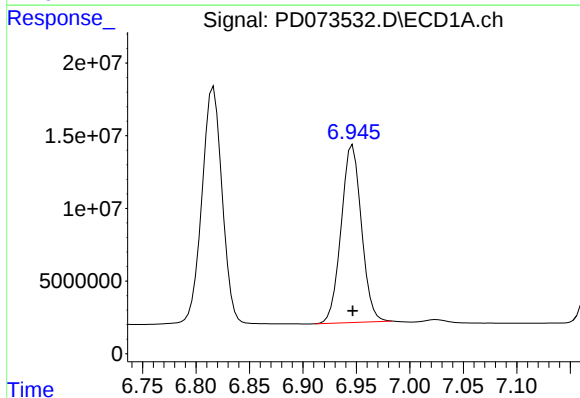


#18 Endrin aldehyde

R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 161436955
Conc: 77.57 ng/ml

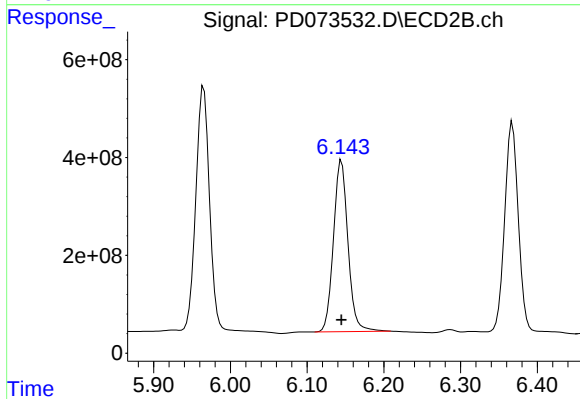


#18 Endrin aldehyde

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 4597795956
Conc: 74.48 ng/ml

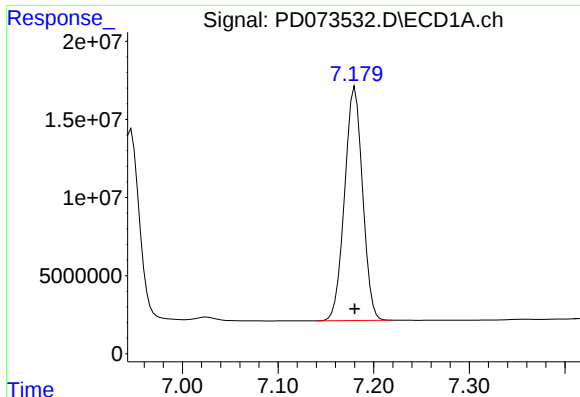


#19 Endosulfan Sulfate

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 196258303
Conc: 78.40 ng/ml

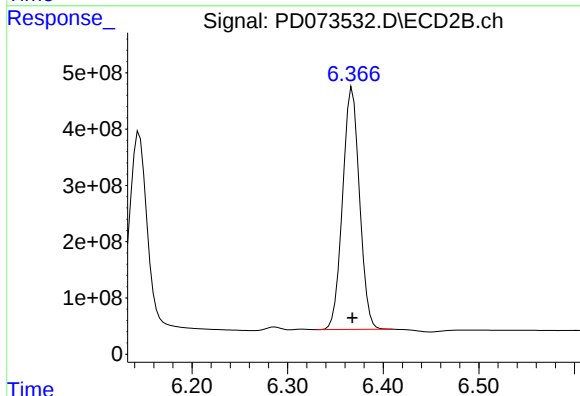


#19 Endosulfan Sulfate

R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 5304685224
Conc: 75.00 ng/ml

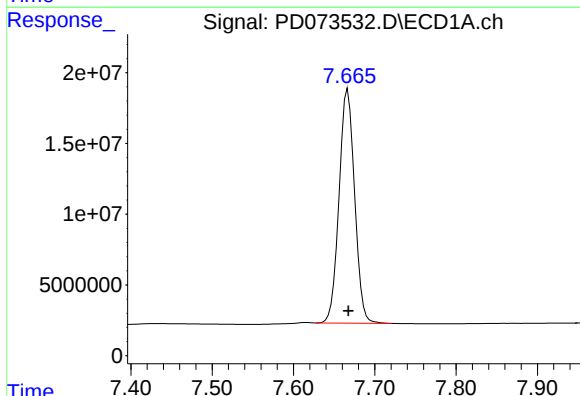


#21 Endrin ketone

R.T.: 7.667 min
Delta R.T.: 0.000 min
Response: 219529686
Conc: 77.99 ng/ml

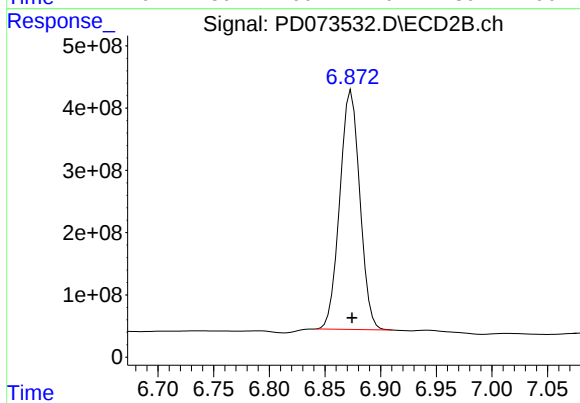

#21 Endrin ketone

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 4813905577
Conc: 75.44 ng/ml

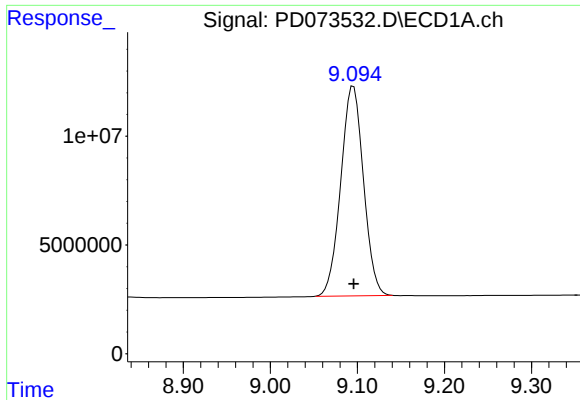


#27 Decachlorobiphenyl

R.T.: 9.095 min

Delta R.T.: 0.000 min

Response: 174897244

Conc: 75.34 ng/ml

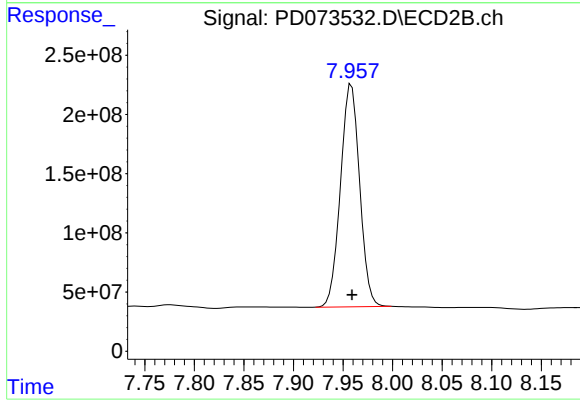

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 2529996375

Conc: 76.06 ng/ml