

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 01:07
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:02:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 03:59:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	195.1E6	6959.1E6	77.659	76.448
27)	SA Decachlor...	9.095	7.959	338.1E6	4882.9E6	148.182	148.818
Target Compounds							
2)	A alpha-BHC	4.013	3.304	326.0E6	9238.9E6	86.937	63.350 #
3)	MA gamma-BHC...	4.346	3.631	304.9E6	11649.8E6	84.283	85.820
4)	MA Heptachlor	4.938	3.977	306.6E6	10640.3E6	83.661	79.033
9)	A Endosulfan I	6.094	5.132	239.0E6	7986.5E6	81.346	77.773
13)	MA Dieldrin	6.369	5.399	549.1E6	15093.1E6	171.816	138.600
14)	MA Endrin	6.600	5.673	408.9E6	12123.8E6	162.653	155.670
16)	A 4,4'-DDD	6.730	5.821	411.6E6	12611.3E6	169.619	155.936
17)	MA 4,4'-DDT	7.046	6.074	400.8E6	11220.6E6	169.935	163.074
20)	A Methoxychlor	7.519	6.652	1071.4E6	15972.7E6	804.750	559.903 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 01:07
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:02:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 03:59:30 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

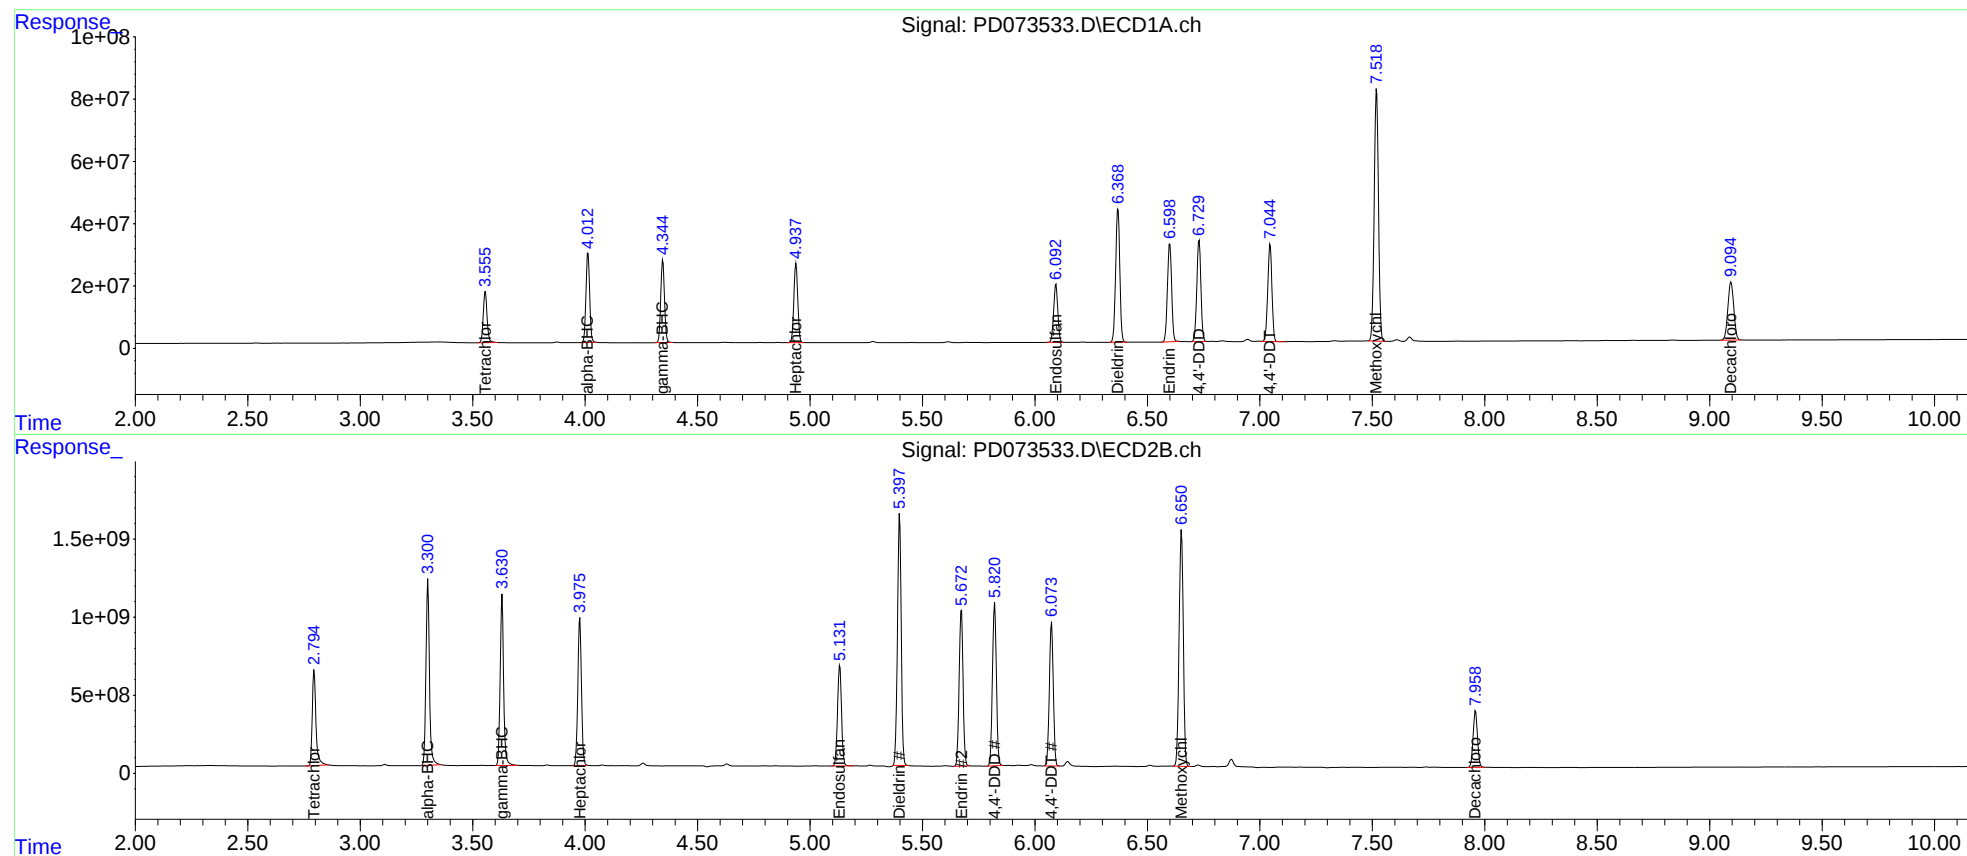

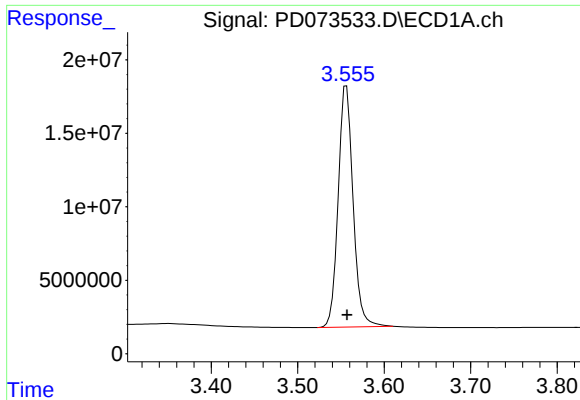


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 195114158
Conc: 77.66 ng/ml

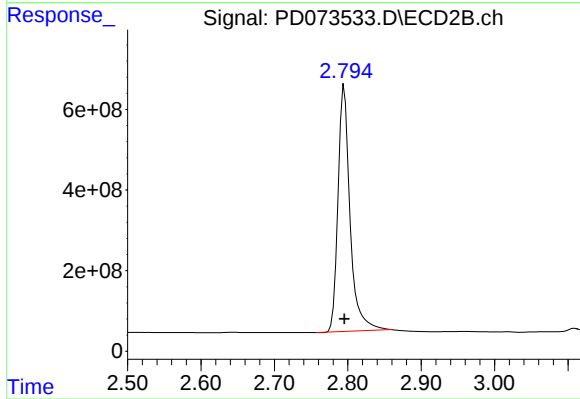


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 6959105439
Conc: 76.45 ng/ml

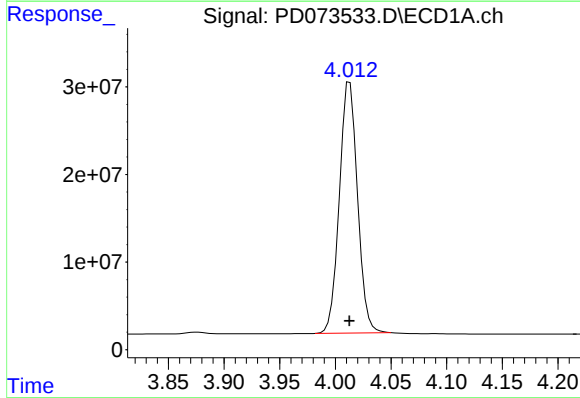


#2 alpha-BHC

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 325967765
Conc: 86.94 ng/ml

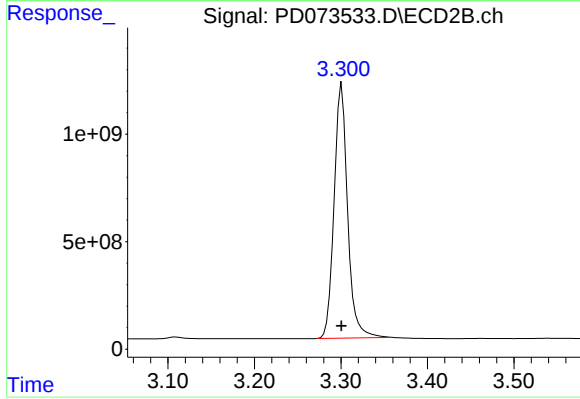


#2 alpha-BHC

R.T.: 3.304 min
Delta R.T.: 0.003 min
Response: 9238943404
Conc: 63.35 ng/ml

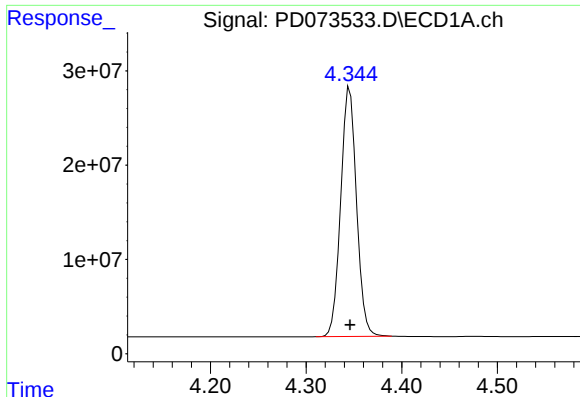


#3 gamma-BHC (Lindane)

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 304942510
Conc: 84.28 ng/ml

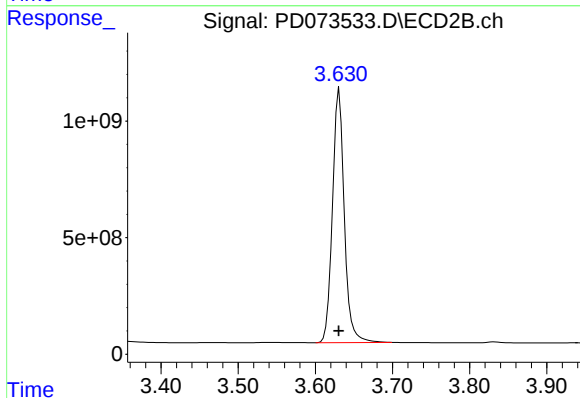


#3 gamma-BHC (Lindane)

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 11649805244
Conc: 85.82 ng/ml

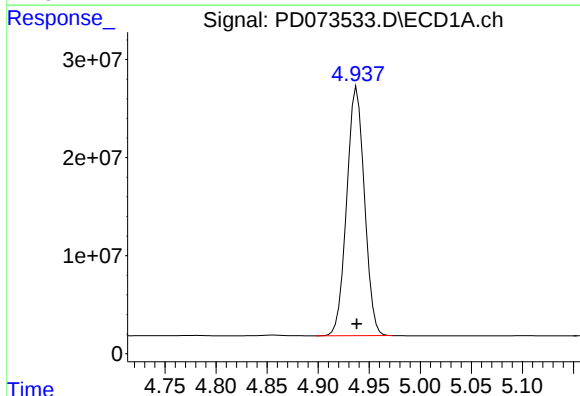


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 306581620
Conc: 83.66 ng/ml

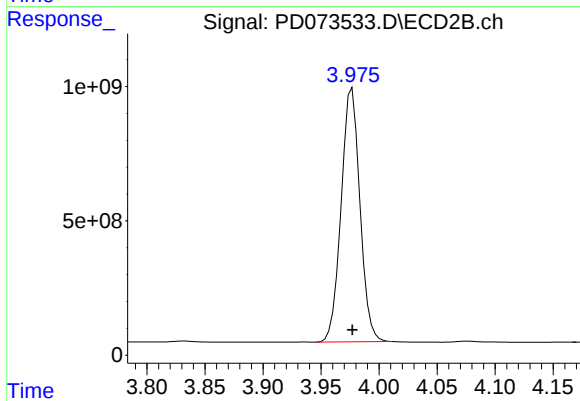


#4 Heptachlor

R.T.: 3.977 min
Delta R.T.: 0.000 min
Response: 10640252354
Conc: 79.03 ng/ml

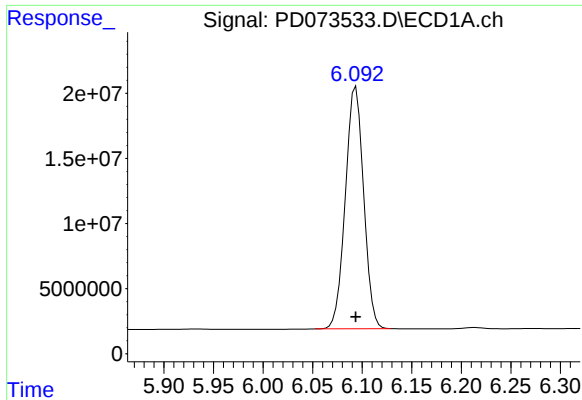


#9 Endosulfan I

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 239048809
Conc: 81.35 ng/ml

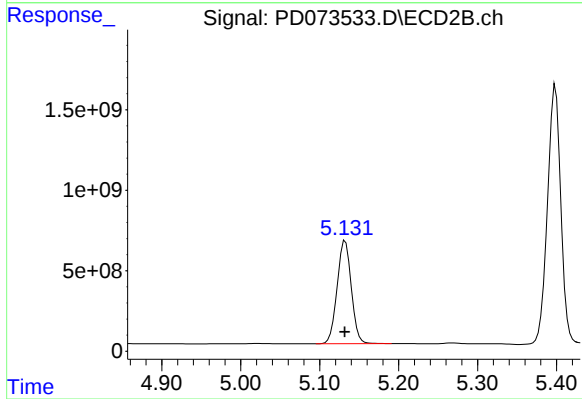


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 7986497300
Conc: 77.77 ng/ml

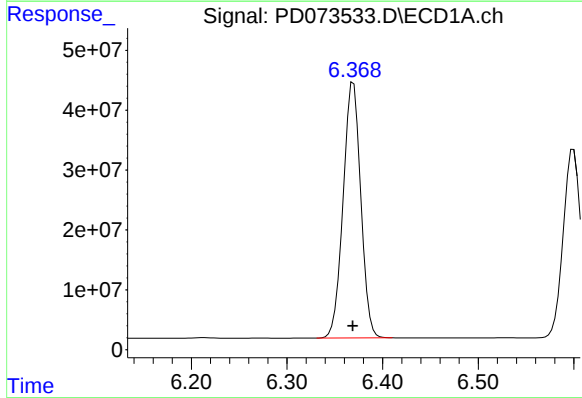


#13 Dieldrin

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 549060413
Conc: 171.82 ng/ml

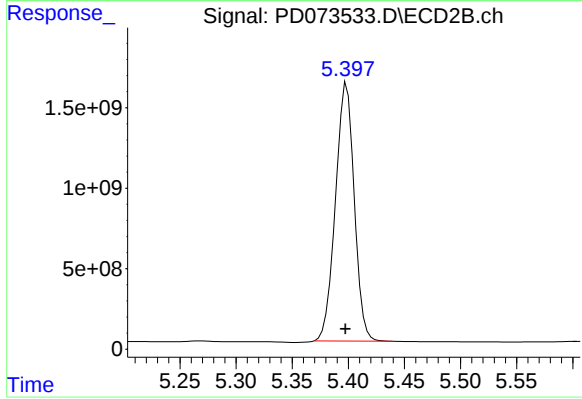


#13 Dieldrin

R.T.: 5.399 min
Delta R.T.: 0.001 min
Response: 15093137366
Conc: 138.60 ng/ml

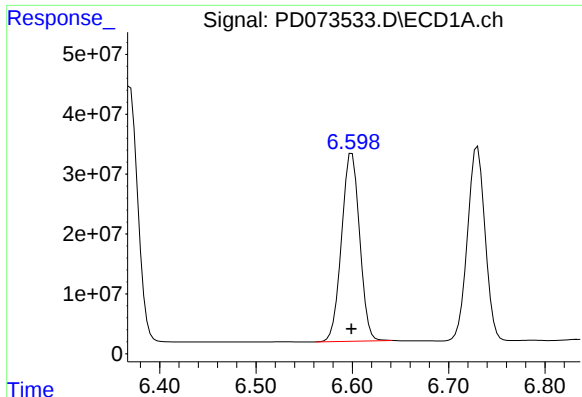


#14 Endrin

R.T.: 6.600 min
Delta R.T.: 0.000 min
Response: 408869906
Conc: 162.65 ng/ml

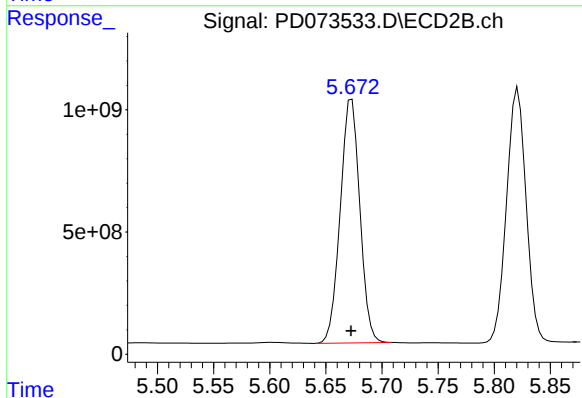


#14 Endrin

R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 12123771336
Conc: 155.67 ng/ml

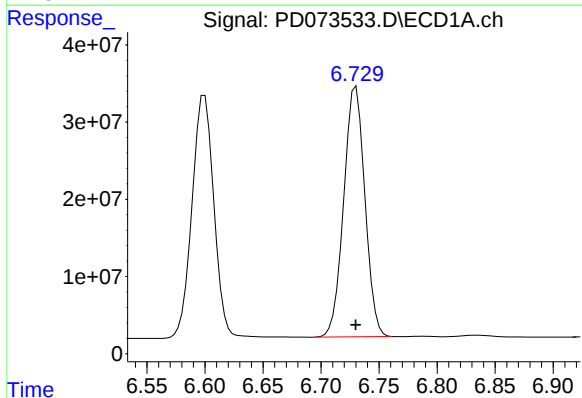


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 411588505
Conc: 169.62 ng/ml

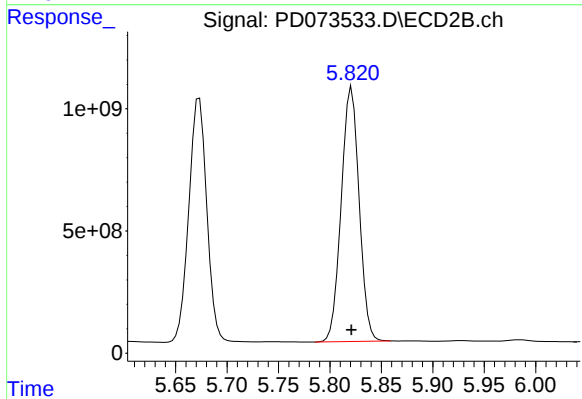


#16 4,4'-DDD

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 12611291466
Conc: 155.94 ng/ml

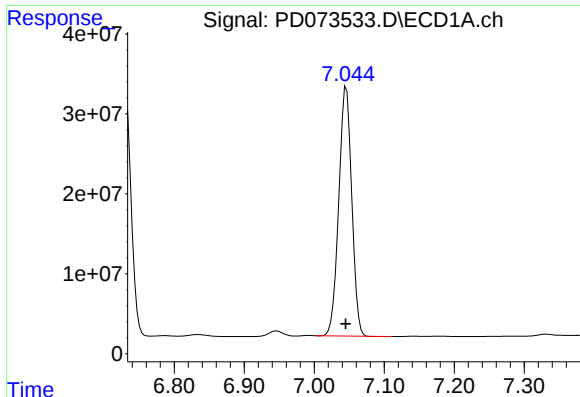


#17 4,4'-DDT

R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 400842156
Conc: 169.94 ng/ml

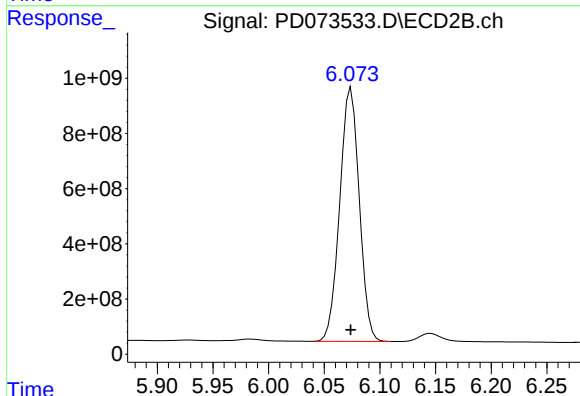


#17 4,4'-DDT

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 11220565762
Conc: 163.07 ng/ml

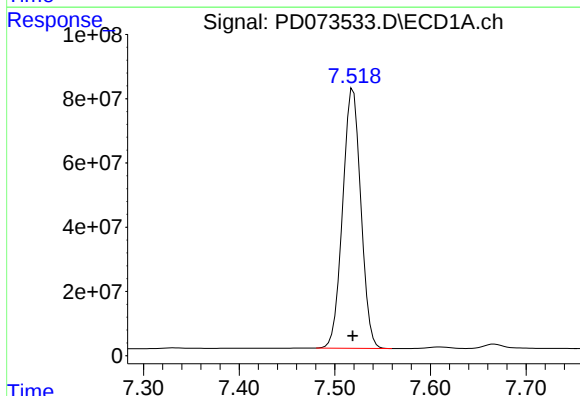


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 1071351047
Conc: 804.75 ng/ml

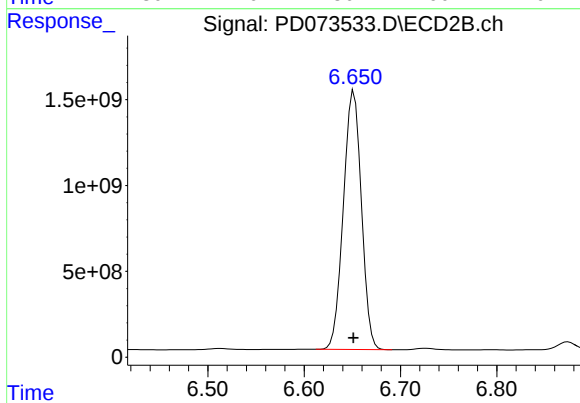


#20 Methoxychlor

R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 15972651195
Conc: 559.90 ng/ml

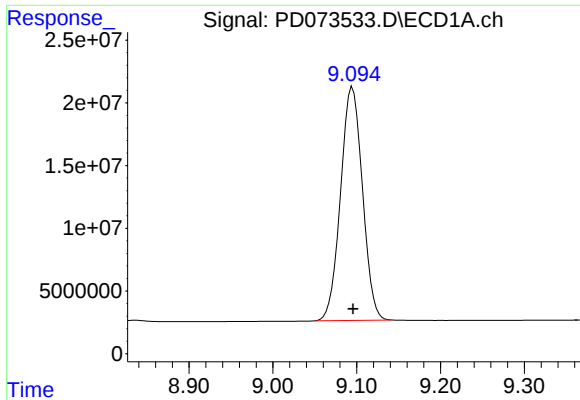

#27 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 338103906
Conc: 148.18 ng/ml

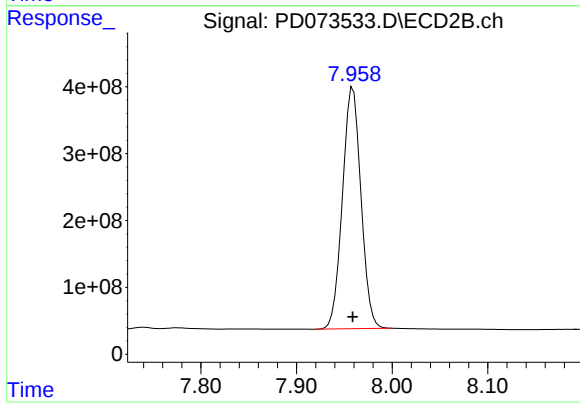

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 4882872207
Conc: 148.82 ng/ml