

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
 Data File : PD073542.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 03:08
 Operator : AR\AJ
 Sample : PB149858BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS858

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/29/2022
 Supervised By : Ankita Jodhani 12/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 05:48:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 29 05:46:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.795	52257134	1693.3E6	21.176	18.721
27)	SA Decachlor...	9.095	7.958	98238016	1414.5E6	44.204	43.627
Target Compounds							
2)	A alpha-BHC	4.012	3.300	16473710	644.4E6	4.468	4.643
3)	MA gamma-BHC...	4.345	3.630	16603051	655.2E6	4.687	4.786
4)	MA Heptachlor	4.937	3.976	17627024	661.6E6	4.884	4.962
5)	MB Aldrin	5.281	4.258	17294692	725.7E6	4.923	5.221
6)	B beta-BHC	4.538	3.923	9070323	268.5E6	5.569	4.824
7)	B delta-BHC	4.786	4.156	17132651	724.8E6	4.638	5.370
8)	B Heptachlo...	5.702	4.760	43658074	539.5E6	13.334	4.572 #
9)	A Endosulfan I	6.093	5.132	14746185	458.1E6	5.108	4.436
10)	B trans-Chl...	5.962	5.012	14443576	586.5E6	4.700	4.933
11)	B cis-Chlor...	6.042	5.076	16441260	521.9E6	5.206	4.445
12)	B 4,4'-DDE	6.213	5.267	26598360	817.7E6	8.963	8.153
13)	MA Dieldrin	6.369	5.395	30652341	1010.3E6	9.764	9.523m
14)	MA Endrin	6.599	5.673	28198598	821.9E6	11.696	10.745
15)	B Endosulfa...	6.816	5.963	25714846	829.5E6	9.741	10.434m
16)	A 4,4'-DDD	6.730	5.820	22501627	786.6E6	9.478	9.755
17)	MA 4,4'-DDT	7.045	6.073	24237191	503.8E6	10.490	7.362 #
18)	B Endrin al...	6.946	6.144	20817818	619.6E6	10.124	10.128
19)	B Endosulfa...	7.180	6.367	24348846	740.5E6	9.833	10.538
20)	A Methoxychlor	7.517	6.650	63588657	1588.6E6	49.027m	59.156
21)	B Endrin ke...	7.667	6.871	28641093	617.3E6	10.223	9.756m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122822\
Data File : PD073542.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 03:08
Operator : AR\AJ
Sample : PB149858BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 05:48:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122822CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 29 05:46:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

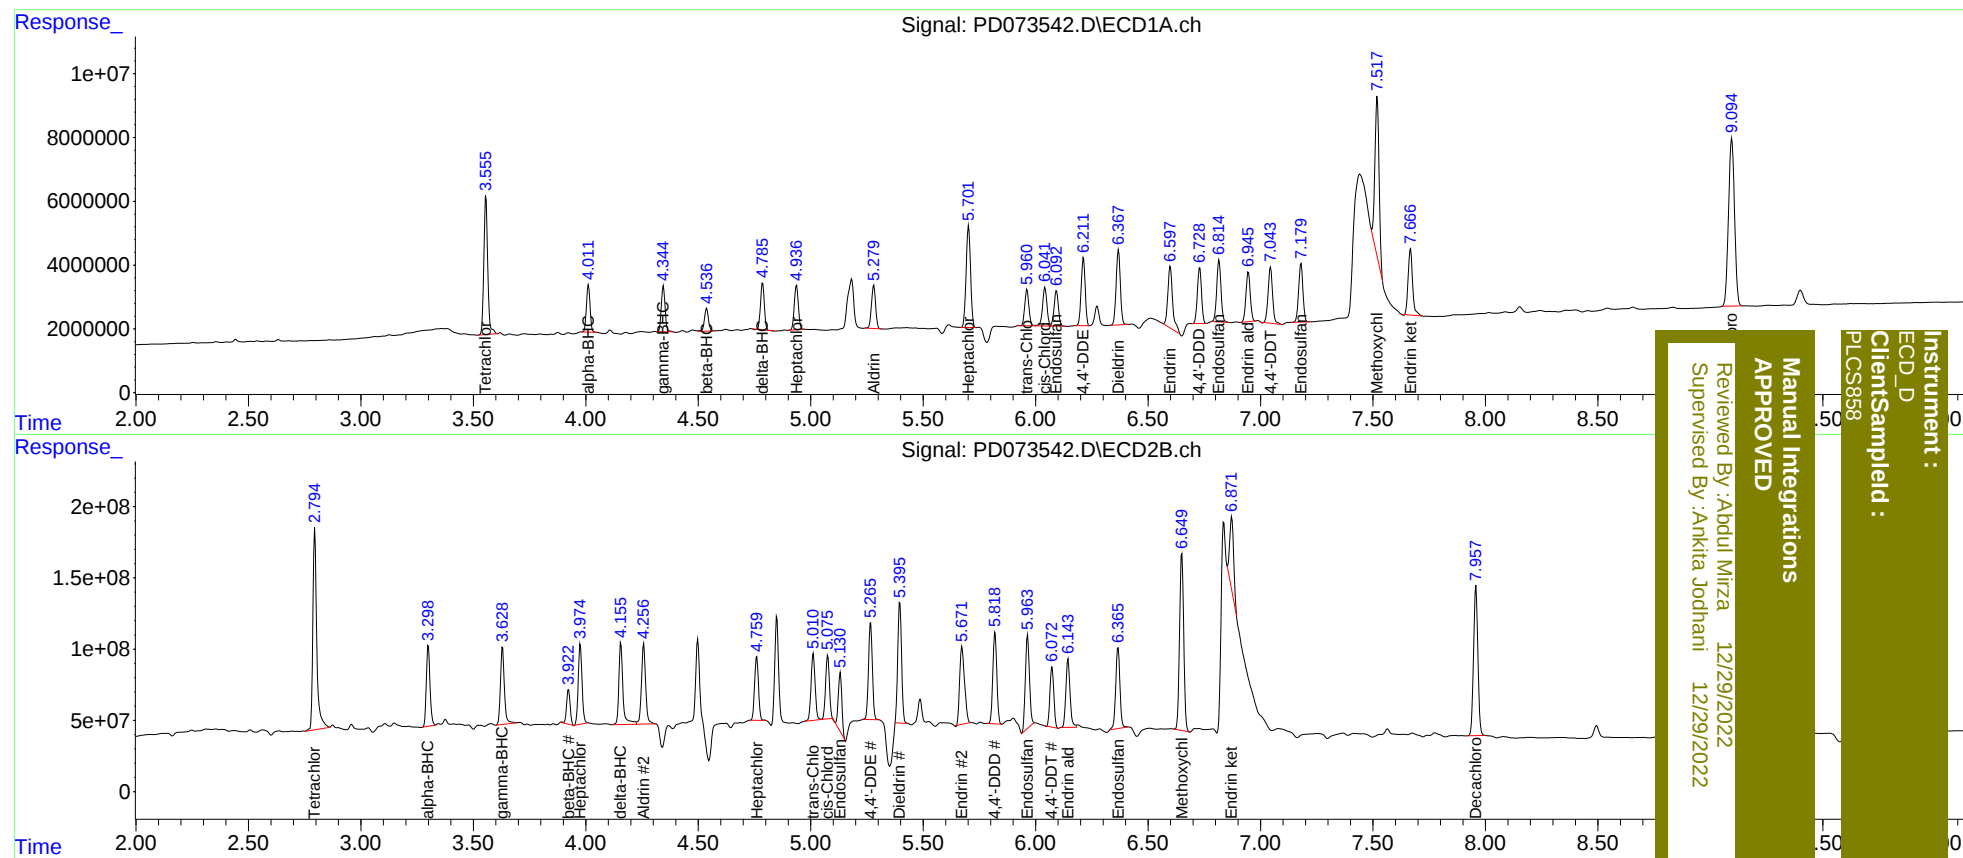

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 12/29/2022
Supervised By: Ankita Jodhani 12/29/2022

Instrument :
ECD_D
Client Sampled :
PLCS858