

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122823\
 Data File : PD080561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2023 13:10
 Operator : AR\AJ
 Sample : 06022-11MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSL2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 20:41:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.799	25272220	43085232	19.794	19.377
2)	SA Decachlor...	9.113	7.938	37500757	51000863	23.325	21.248
Target Compounds							
2)	A alpha-BHC	4.023	3.301	117.3E6	192.2E6	56.910	56.359
3)	MA gamma-BHC...	4.356	3.630	109.9E6	178.0E6	55.327	55.299
4)	MA Heptachlor	4.949	3.971	111.4E6	177.2E6	53.345	55.322
5)	MB Aldrin	5.293	4.252	106.8E6	173.9E6	47.757	49.227
6)	B beta-BHC	4.550	3.925	48152936	77111658	46.390	44.910
7)	B delta-BHC	4.800	4.156	115.5E6	186.3E6	50.277	47.918
8)	B Heptachlo...	5.720	4.753	98645499	161.2E6	45.920	47.554
9)	A Endosulfan I	6.106	5.124	93438167	149.4E6	52.452	54.498
10)	B trans-Chl...	5.976	5.004	96525406	159.0E6	47.035	48.306
11)	B cis-Chlor...	6.055	5.068	99036919	160.9E6	47.182	47.856
12)	B 4,4'-DDE	6.226	5.257	188.2E6	312.4E6	97.419	99.474
13)	MA Dieldrin	6.382	5.388	203.4E6	336.0E6	109.306	112.121
14)	MA Endrin	6.612	5.663	169.1E6	293.5E6	107.968	111.546
15)	B Endosulfa...	6.830	5.955	173.5E6	284.0E6	92.546	97.957
16)	A 4,4'-DDD	6.743	5.810	153.8E6	254.8E6	110.912	110.824
17)	MA 4,4'-DDT	7.058	6.061	163.9E6	262.6E6	110.880	108.891
18)	B Endrin al...	6.960	6.135	125.6E6	202.6E6	84.189	87.842
19)	B Endosulfa...	7.194	6.357	167.7E6	268.1E6	91.417	95.571
20)	A Methoxychlor	7.532	6.635	403.9E6	625.8E6	510.084	497.142
21)	B Endrin ke...	7.681	6.864	184.6E6	308.6E6	94.859	96.434

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122823\
Data File : PD080561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2023 13:10
Operator : AR\AJ
Sample : 06022-11MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 20:41:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

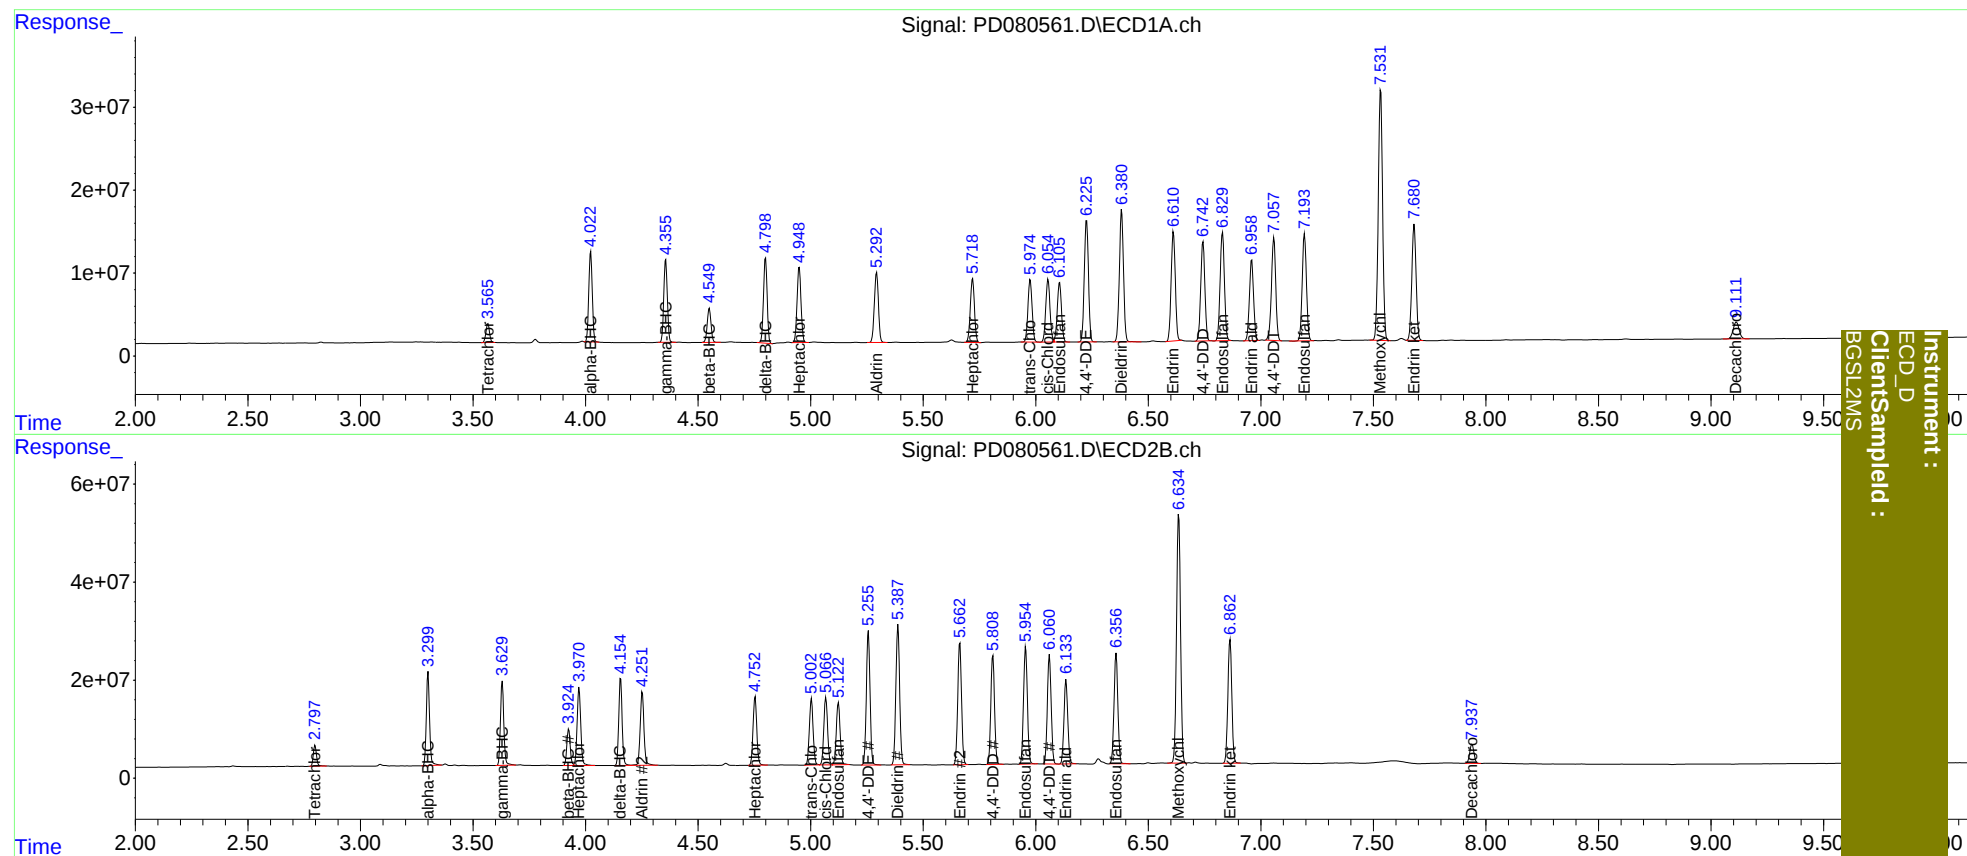

Instrument :
ECD_D
ClientSampled :
BSL2MS