

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 11:52
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 13:10:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:09:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	6135416	25707663	5.420	5.151
27)	SA Decachlor...	8.283	9.104	15103492	42759453	10.945	10.754
Target Compounds							
2)	A alpha-BHC	3.941	4.411	8445484	37063168	5.254	5.052
3)	MA gamma-BHC...	4.226	4.697	8178854	33469161	5.320	5.023
4)	MA Heptachlor	4.531	5.208	8597373	34742259	5.246	5.230
9)	A Endosulfan I	5.569	6.259	7467355	27813000	5.367	5.167
13)	MA Dieldrin	5.814	6.516	15389748	58483232	10.140	10.073
14)	MA Endrin	6.072	6.735	13672033	47889145	10.706	10.333
16)	A 4,4'-DDD	6.196	6.854	12392862	46254858	10.245	10.246
17)	MA 4,4'-DDT	6.439	7.154	12694056	45436010	9.932	10.062
20)	A Methoxychlor	6.986	7.610	35199017	120.4E6	53.500	54.303

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 11:52
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 13:10:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:09:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

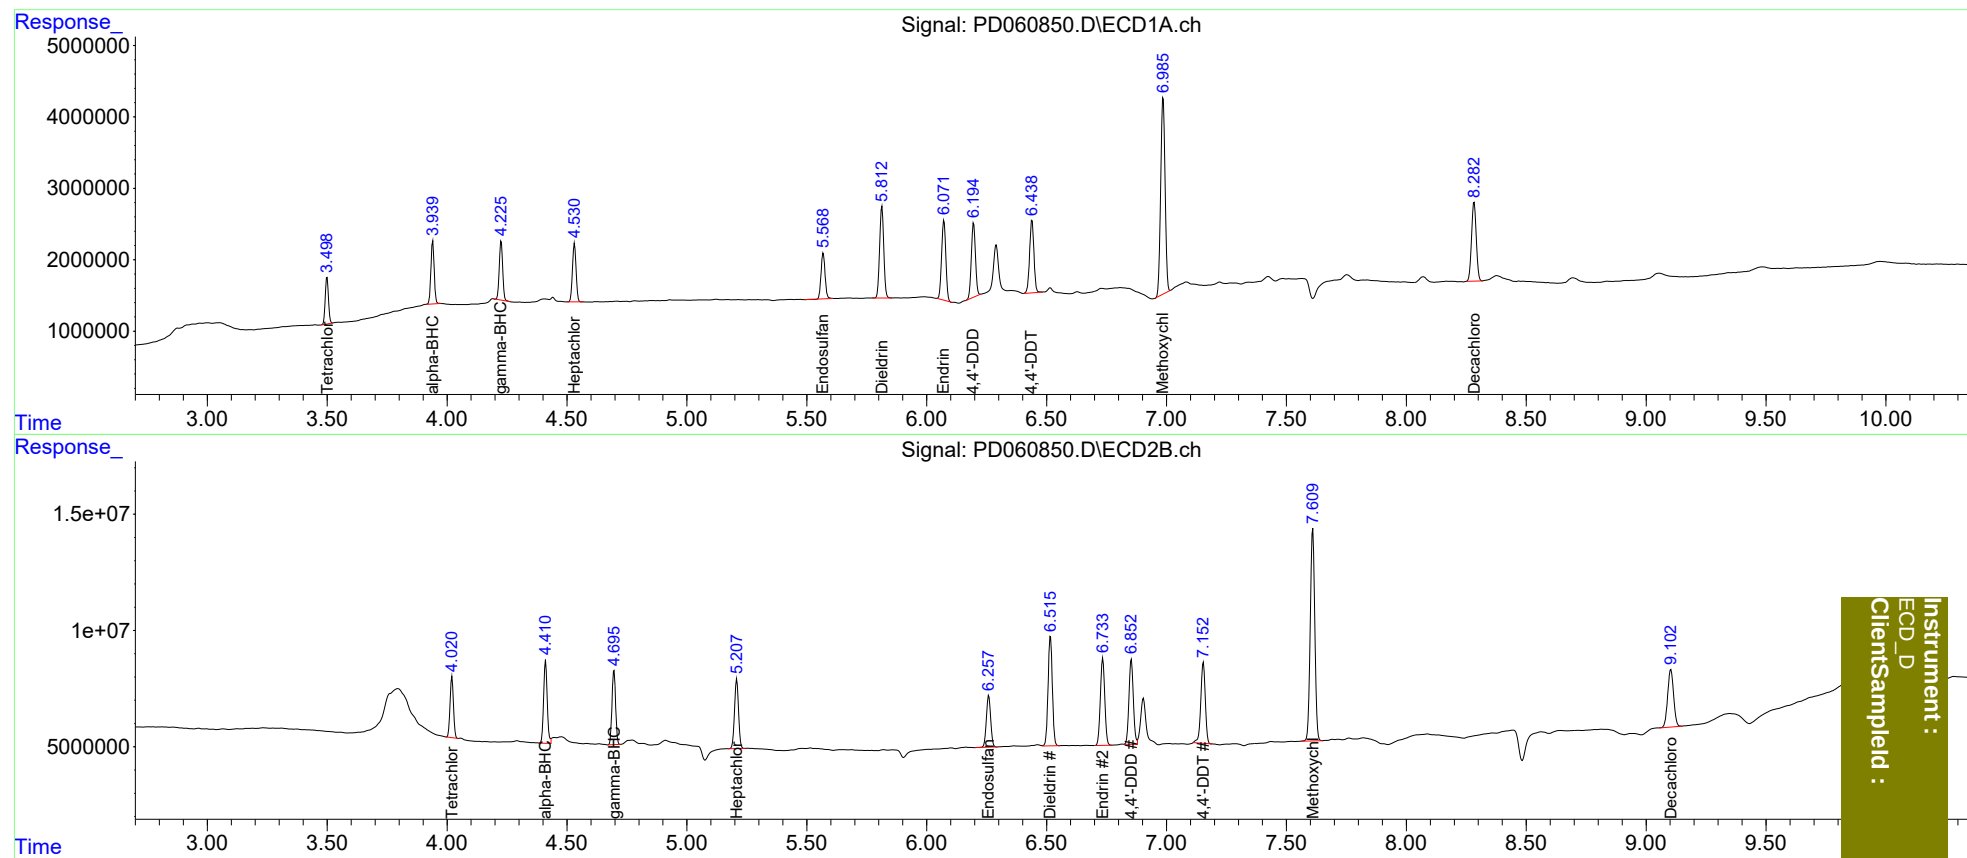


Instrument :
ECD_D
ClientSampled :

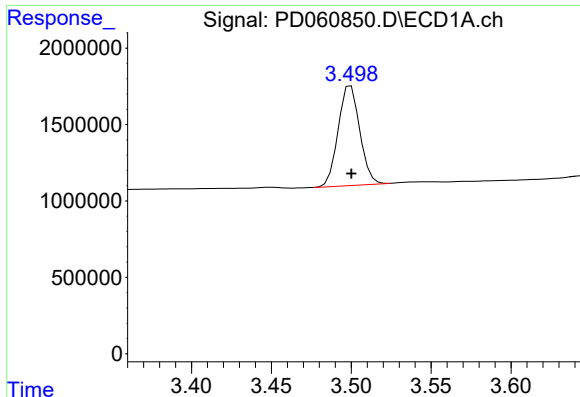

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 6135416
Conc: 5.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

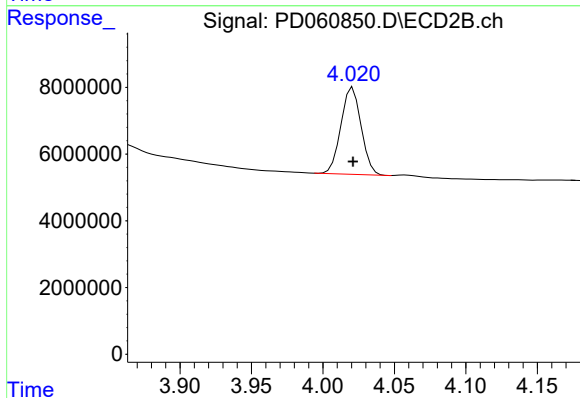


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 25707663
Conc: 5.15 ng/ml

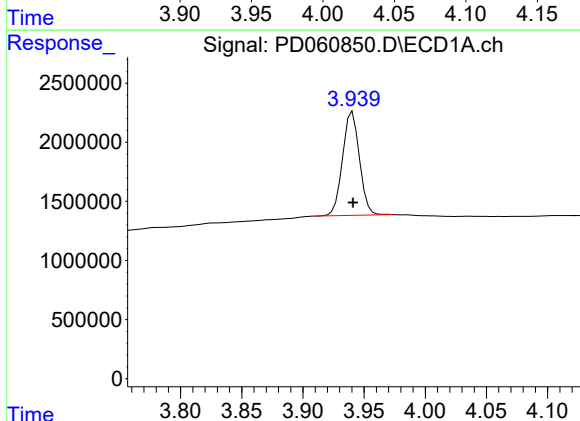


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 8445484
Conc: 5.25 ng/ml

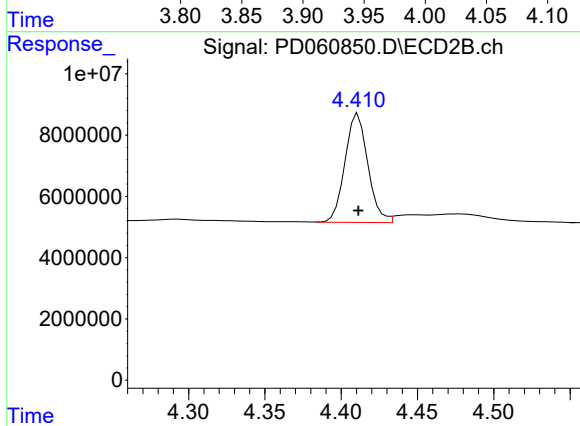

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 37063168
Conc: 5.05 ng/ml

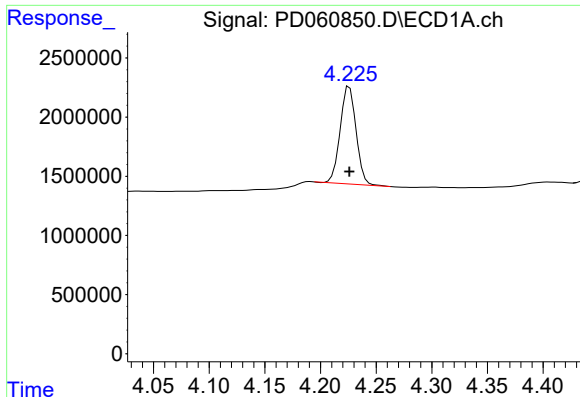

#3 gamma-BHC (Lindane)


R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 8178854
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

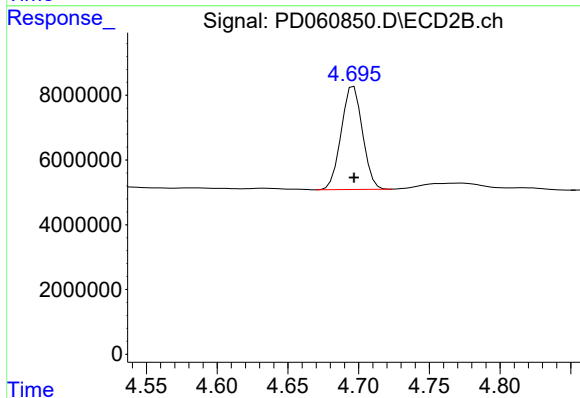


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 33469161
Conc: 5.02 ng/ml

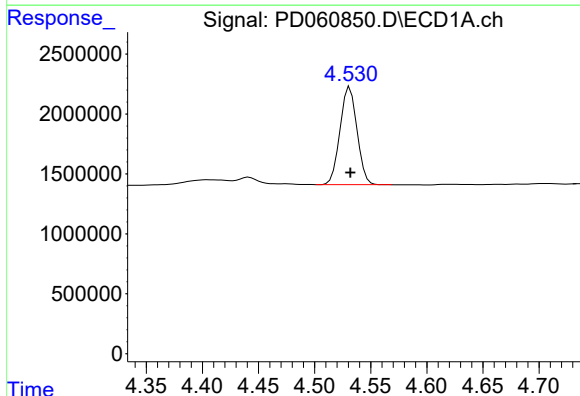


#4 Heptachlor

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 8597373
Conc: 5.25 ng/ml

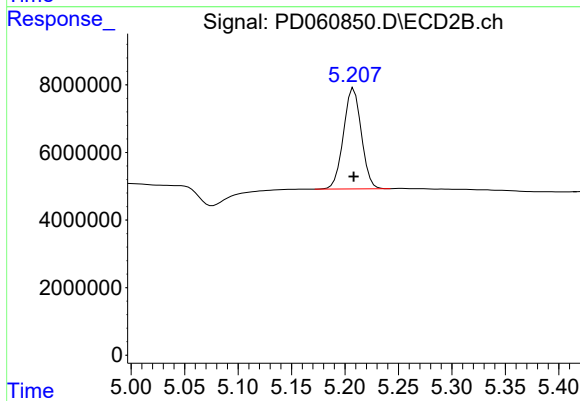

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 34742259
Conc: 5.23 ng/ml

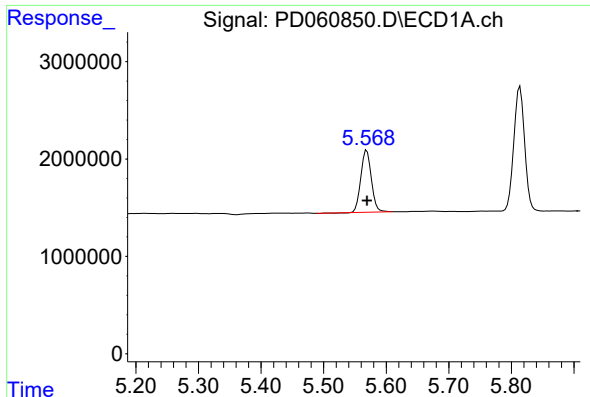

#9 Endosulfan I


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 7467355
Conc: 5.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

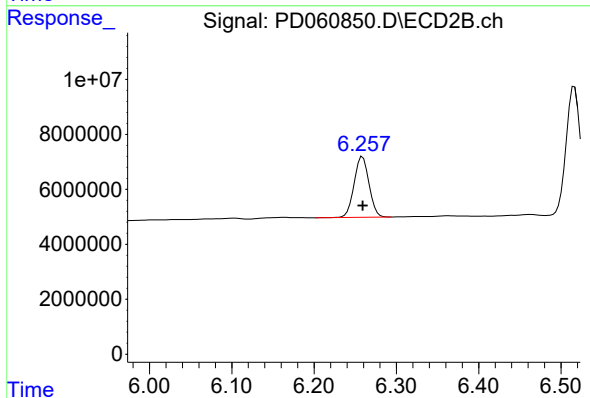


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 27813000
Conc: 5.17 ng/ml

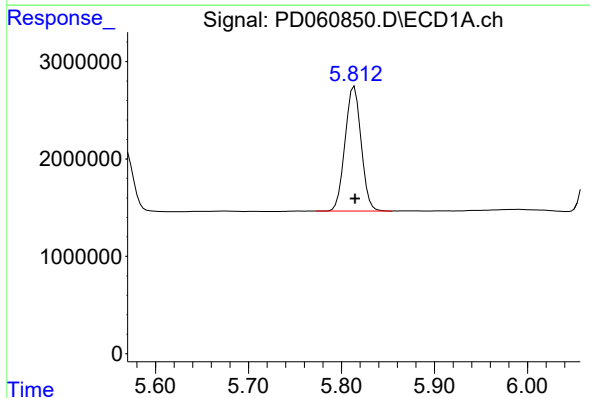


#13 Dieldrin

R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 15389748
Conc: 10.14 ng/ml

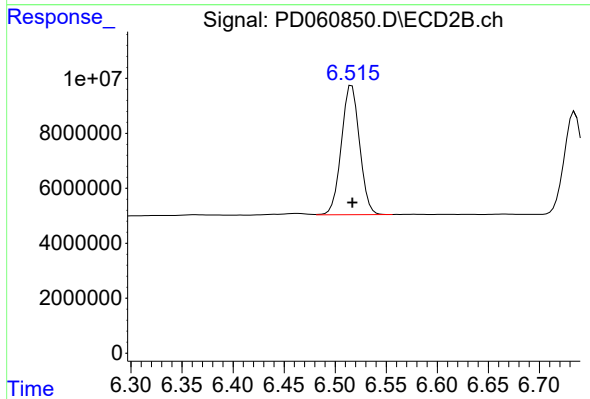

#13 Dieldrin


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 58483232
Conc: 10.07 ng/ml

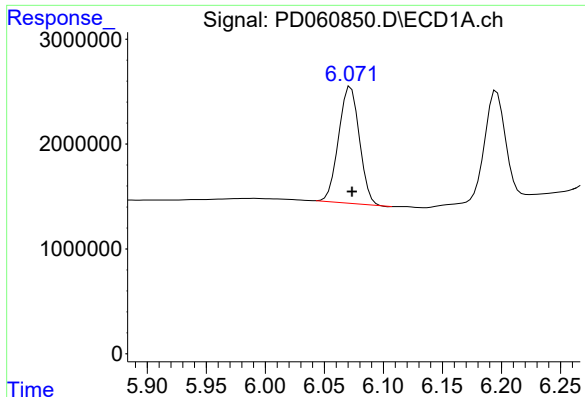

#14 Endrin


R.T.: 6.072 min
Delta R.T.: -0.001 min
Response: 13672033
Conc: 10.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

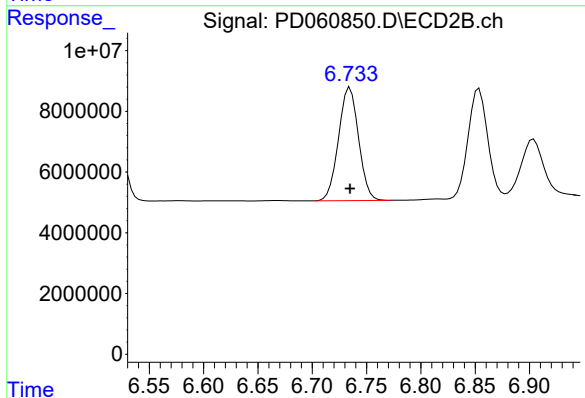


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 47889145
Conc: 10.33 ng/ml

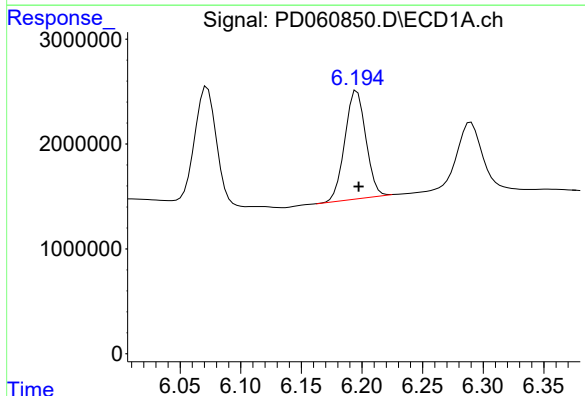


#16 4,4'-DDD

R.T.: 6.196 min
Delta R.T.: -0.001 min
Response: 12392862
Conc: 10.25 ng/ml

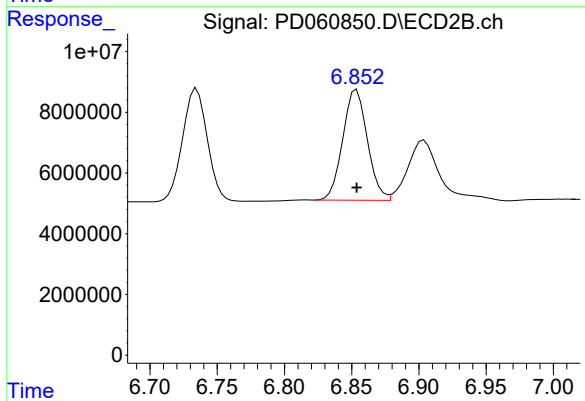

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 46254858
Conc: 10.25 ng/ml

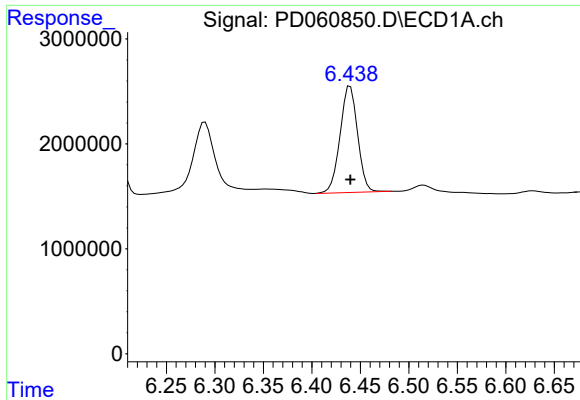

#17 4,4'-DDT


R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 12694056
Conc: 9.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

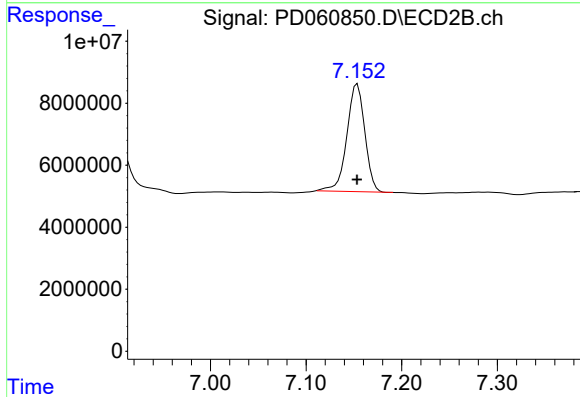


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 45436010
Conc: 10.06 ng/ml

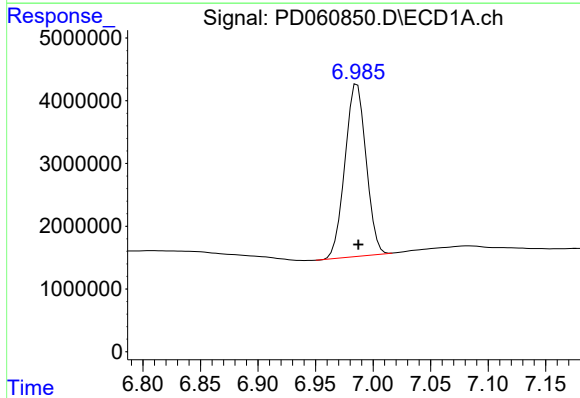


#20 Methoxychlor

R.T.: 6.986 min
Delta R.T.: -0.001 min
Response: 35199017
Conc: 53.50 ng/ml

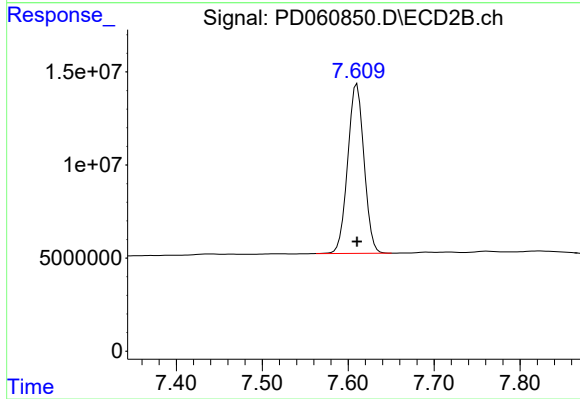

#20 Methoxychlor


R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 120352506
Conc: 54.30 ng/ml

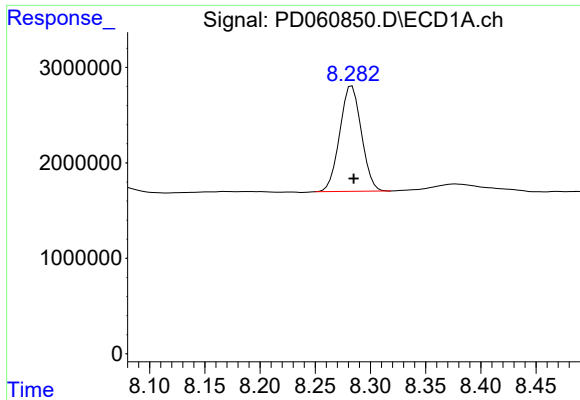

#27 Decachlorobiphenyl

R.T.: 8.283 min
Delta R.T.: -0.002 min
Response: 15103492
Conc: 10.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

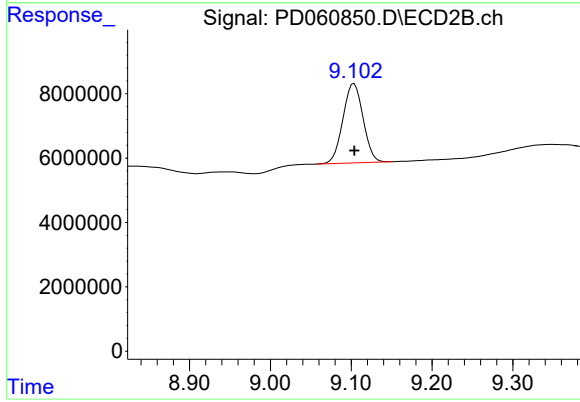

#27 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 42759453
Conc: 10.75 ng/ml