

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 12:21
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 13:10:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:09:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	11768089	50522345	10.396	10.123
27)	SA Decachlor...	8.284	9.103	29190269	83319892	21.154	20.955
Target Compounds							
2)	A alpha-BHC	3.941	4.411	16337130	73645760	10.163	10.038
3)	MA gamma-BHC...	4.226	4.697	15557072	66915673	10.120	10.043
4)	MA Heptachlor	4.532	5.208	16861021	67759279	10.288	10.199
9)	A Endosulfan I	5.570	6.259	14337348	54898834	10.304	10.199
13)	MA Dieldrin	5.815	6.516	30542143	116.8E6	20.124	20.111
14)	MA Endrin	6.073	6.735	26333213	94614965	20.621	20.415
16)	A 4,4'-DDD	6.197	6.854	24300375	92045733	20.089	20.389
17)	MA 4,4'-DDT	6.440	7.154	25312939	91664699	19.805	20.299
20)	A Methoxychlor	6.986	7.610	68700408	235.1E6	104.419	106.088

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 12:21
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 13:10:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:09:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

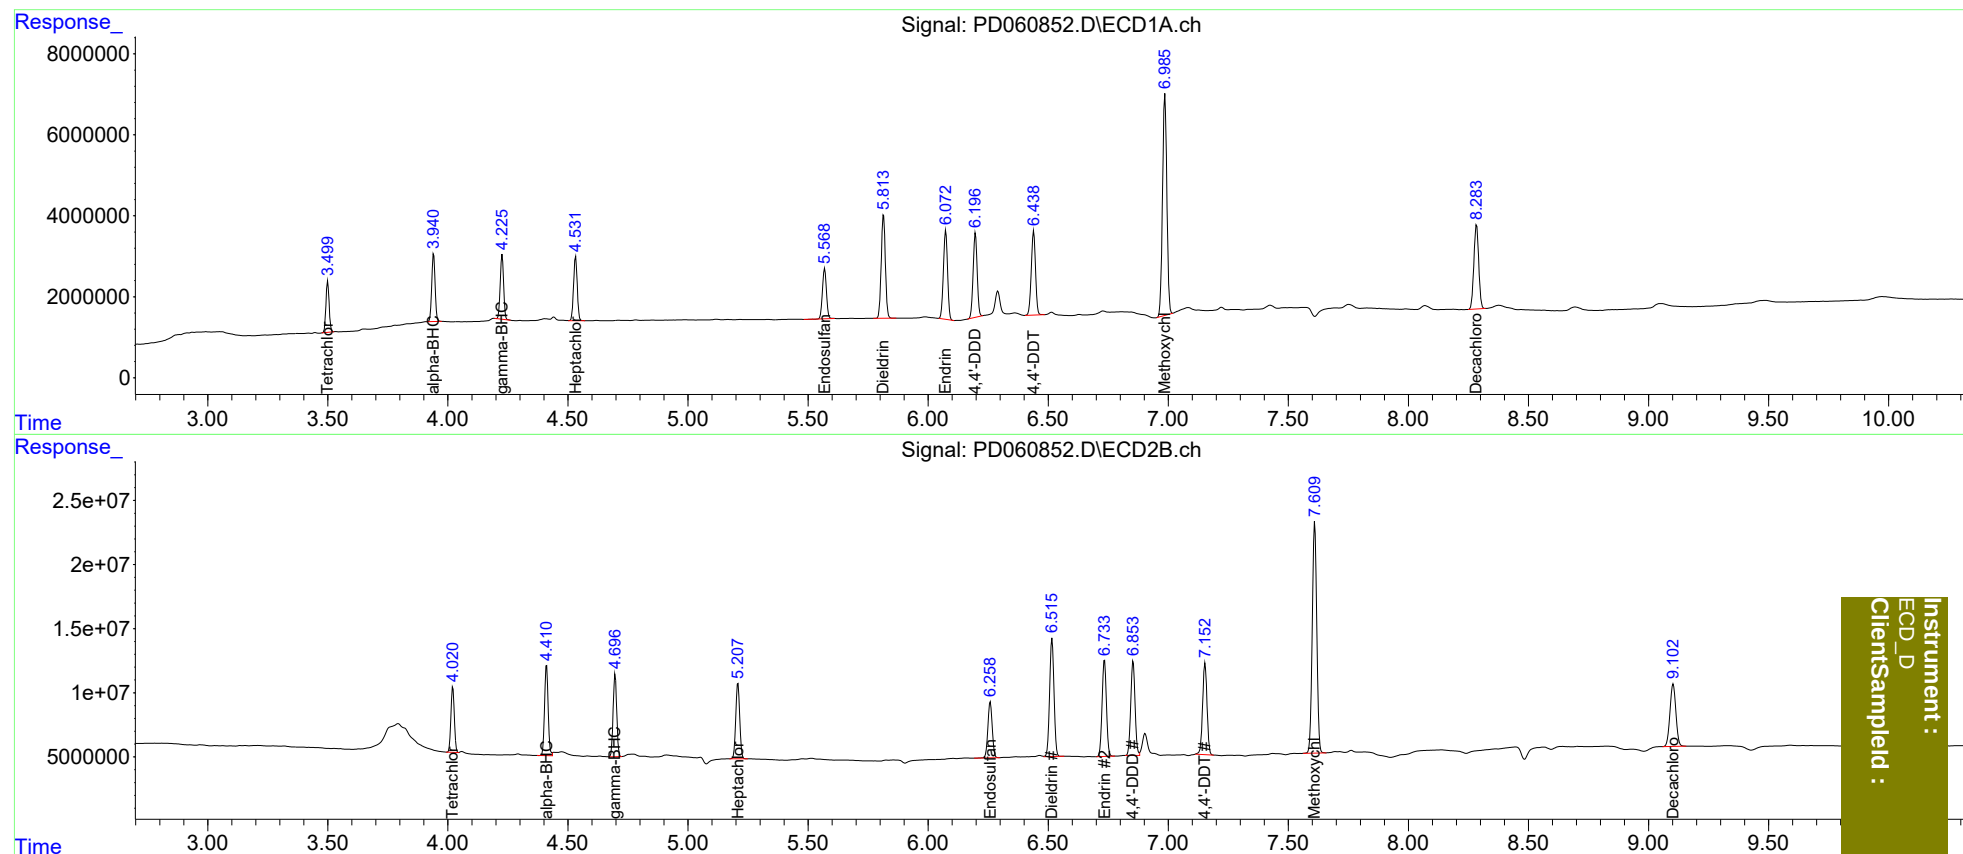


Instrument :
ECD_D
ClientSampled :

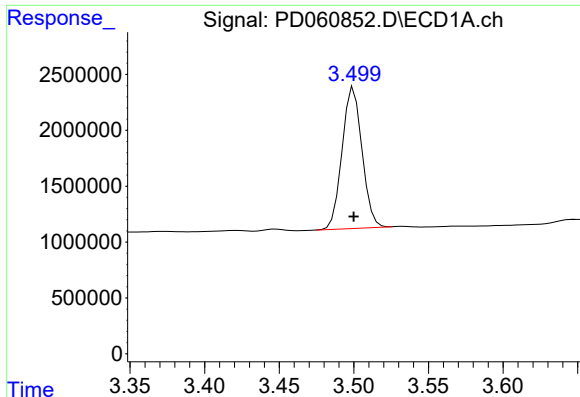

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 11768089
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

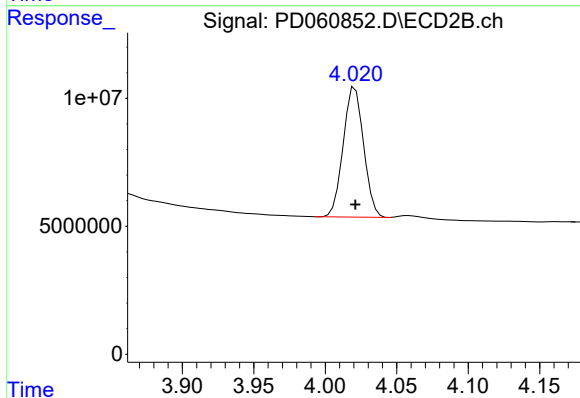


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 50522345
Conc: 10.12 ng/ml

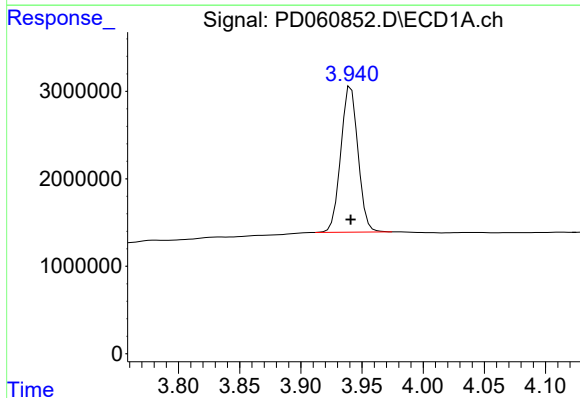


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 16337130
Conc: 10.16 ng/ml

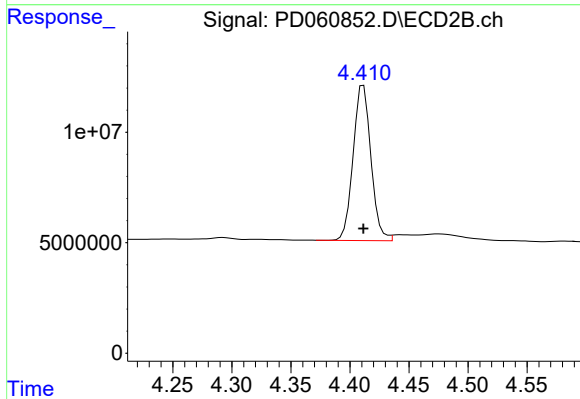

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 73645760
Conc: 10.04 ng/ml

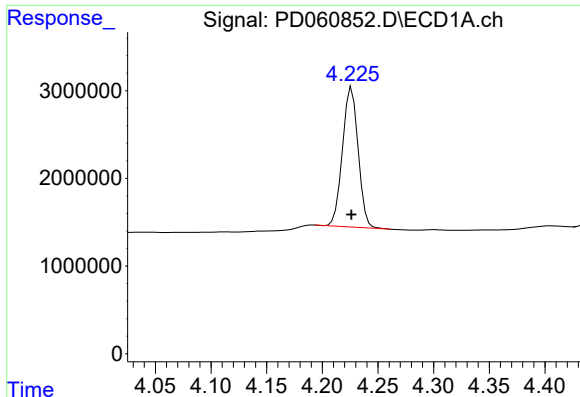

#3 gamma-BHC (Lindane)


R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 15557072
Conc: 10.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

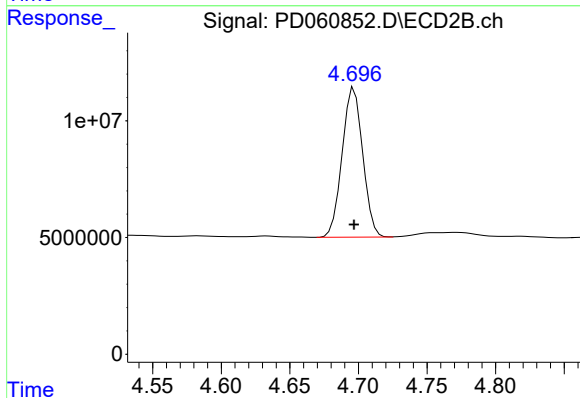


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 66915673
Conc: 10.04 ng/ml

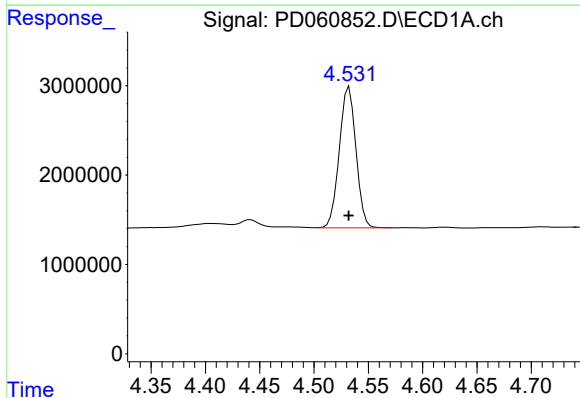


#4 Heptachlor

R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 16861021
Conc: 10.29 ng/ml

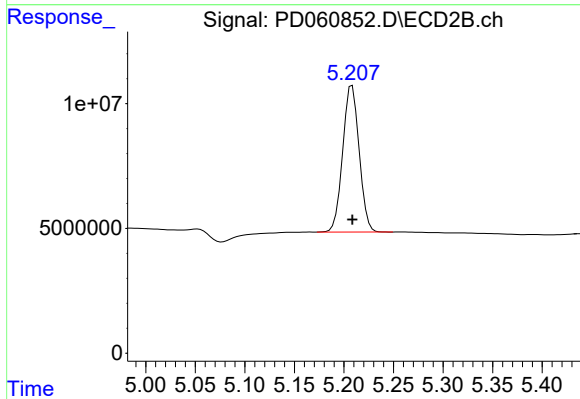

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 67759279
Conc: 10.20 ng/ml

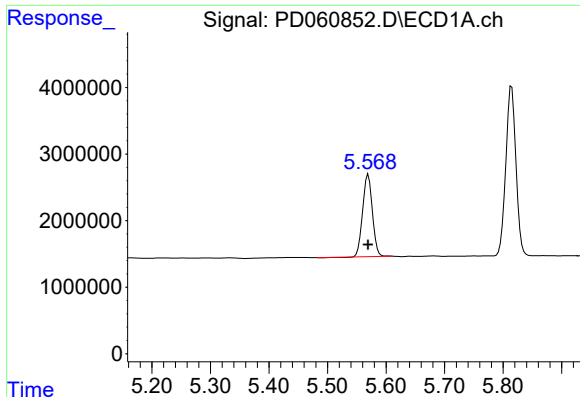

#9 Endosulfan I


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 14337348
Conc: 10.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

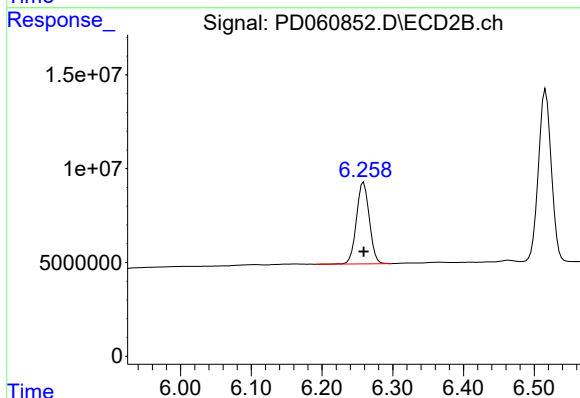


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 54898834
Conc: 10.20 ng/ml

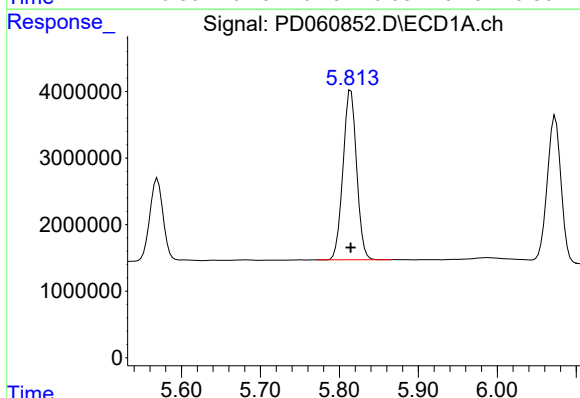


#13 Dieldrin

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 30542143
Conc: 20.12 ng/ml

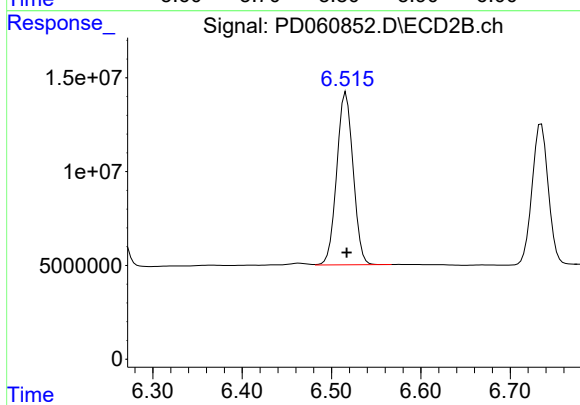

#13 Dieldrin


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 116766688
Conc: 20.11 ng/ml

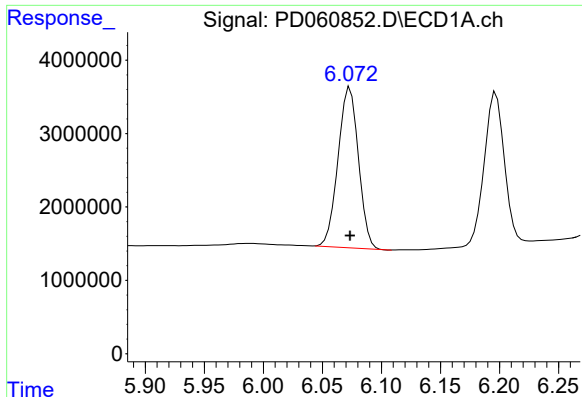

#14 Endrin


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 26333213
Conc: 20.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

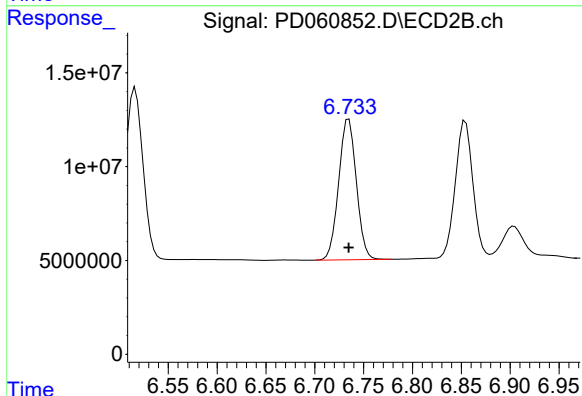


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 94614965
Conc: 20.42 ng/ml

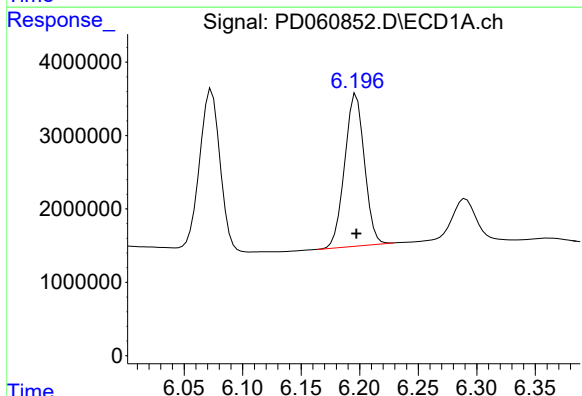


#16 4,4'-DDD

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 24300375
Conc: 20.09 ng/ml

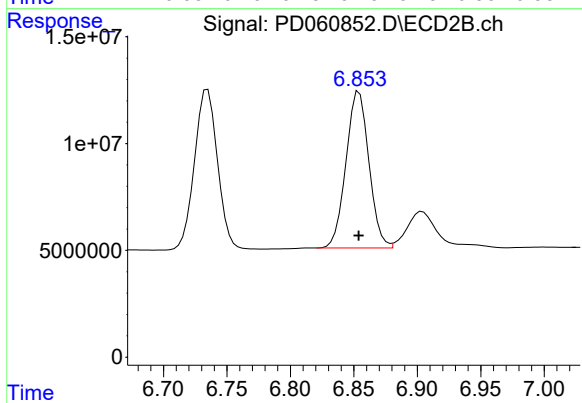

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 92045733
Conc: 20.39 ng/ml

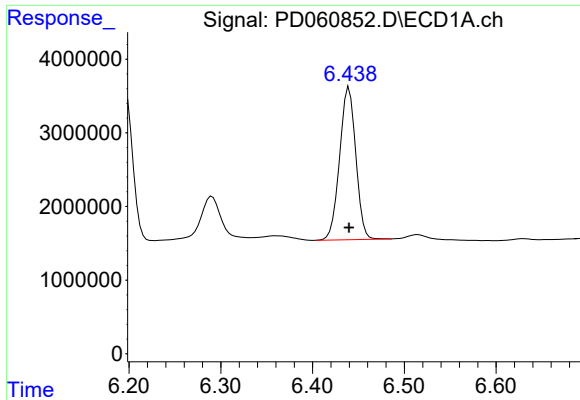

#17 4,4'-DDT


R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 25312939
Conc: 19.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

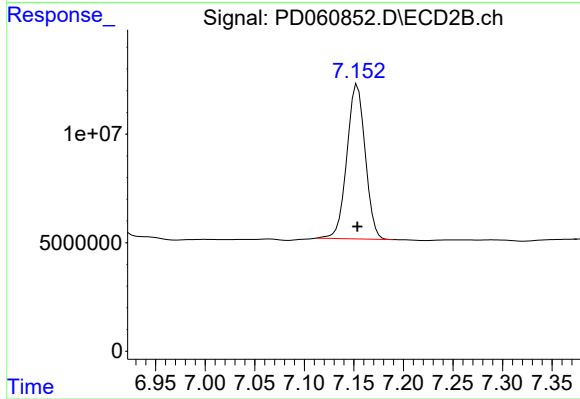


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 91664699
Conc: 20.30 ng/ml

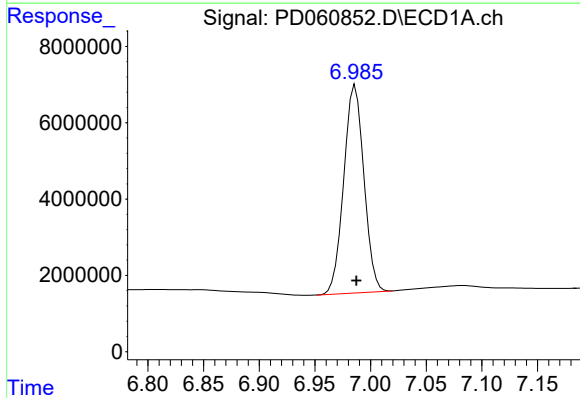


#20 Methoxychlor

R.T.: 6.986 min
Delta R.T.: 0.000 min
Response: 68700408
Conc: 104.42 ng/ml

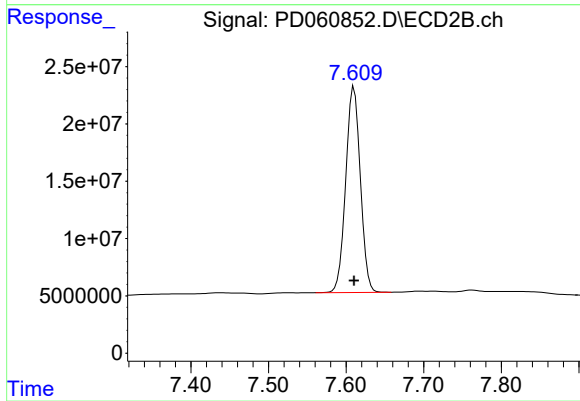

#20 Methoxychlor


R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 235123516
Conc: 106.09 ng/ml

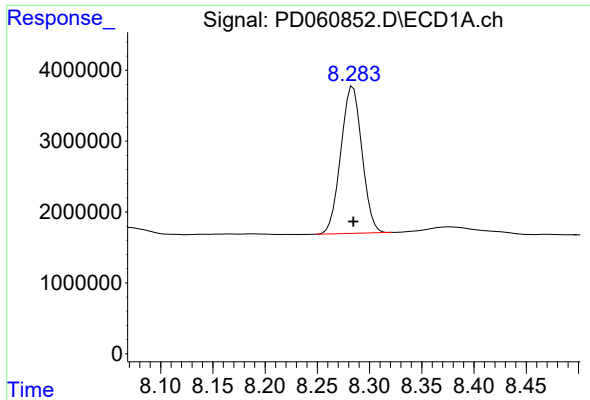

#27 Decachlorobiphenyl

R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 29190269
Conc: 21.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

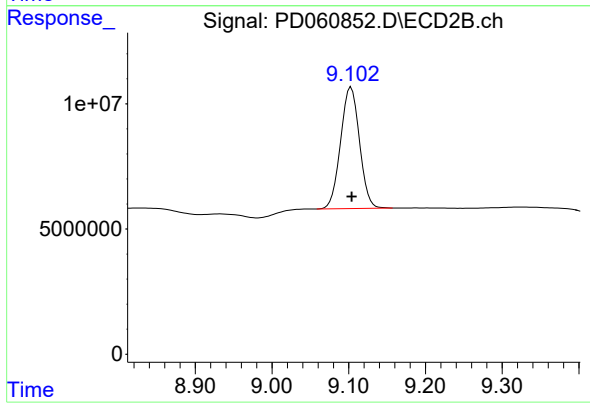

#27 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.000 min
Response: 83319892
Conc: 20.96 ng/ml