

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 12:49
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 13:09:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:09:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	22639366	99817749	20.000	20.000
27)	SA Decachlor...	8.285	9.104	55195468	159.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.941	4.411	32150541	146.7E6	20.000	20.000
3)	MA gamma-BHC...	4.226	4.697	30746187	133.3E6	20.000	20.000
4)	MA Heptachlor	4.532	5.208	32778646	132.9E6	20.000	20.000
9)	A Endosulfan I	5.569	6.259	27828756	107.7E6	20.000	20.000
13)	MA Dieldrin	5.815	6.517	60707101	232.2E6	40.000	40.000
14)	MA Endrin	6.073	6.735	51079773	185.4E6	40.000	40.000
16)	A 4,4'-DDD	6.197	6.854	48385910	180.6E6	40.000	40.000
17)	MA 4,4'-DDT	6.440	7.153	51125194	180.6E6	40.000	40.000
20)	A Methoxychlor	6.987	7.610	131.6E6	443.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 12:49
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 13:09:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:09:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

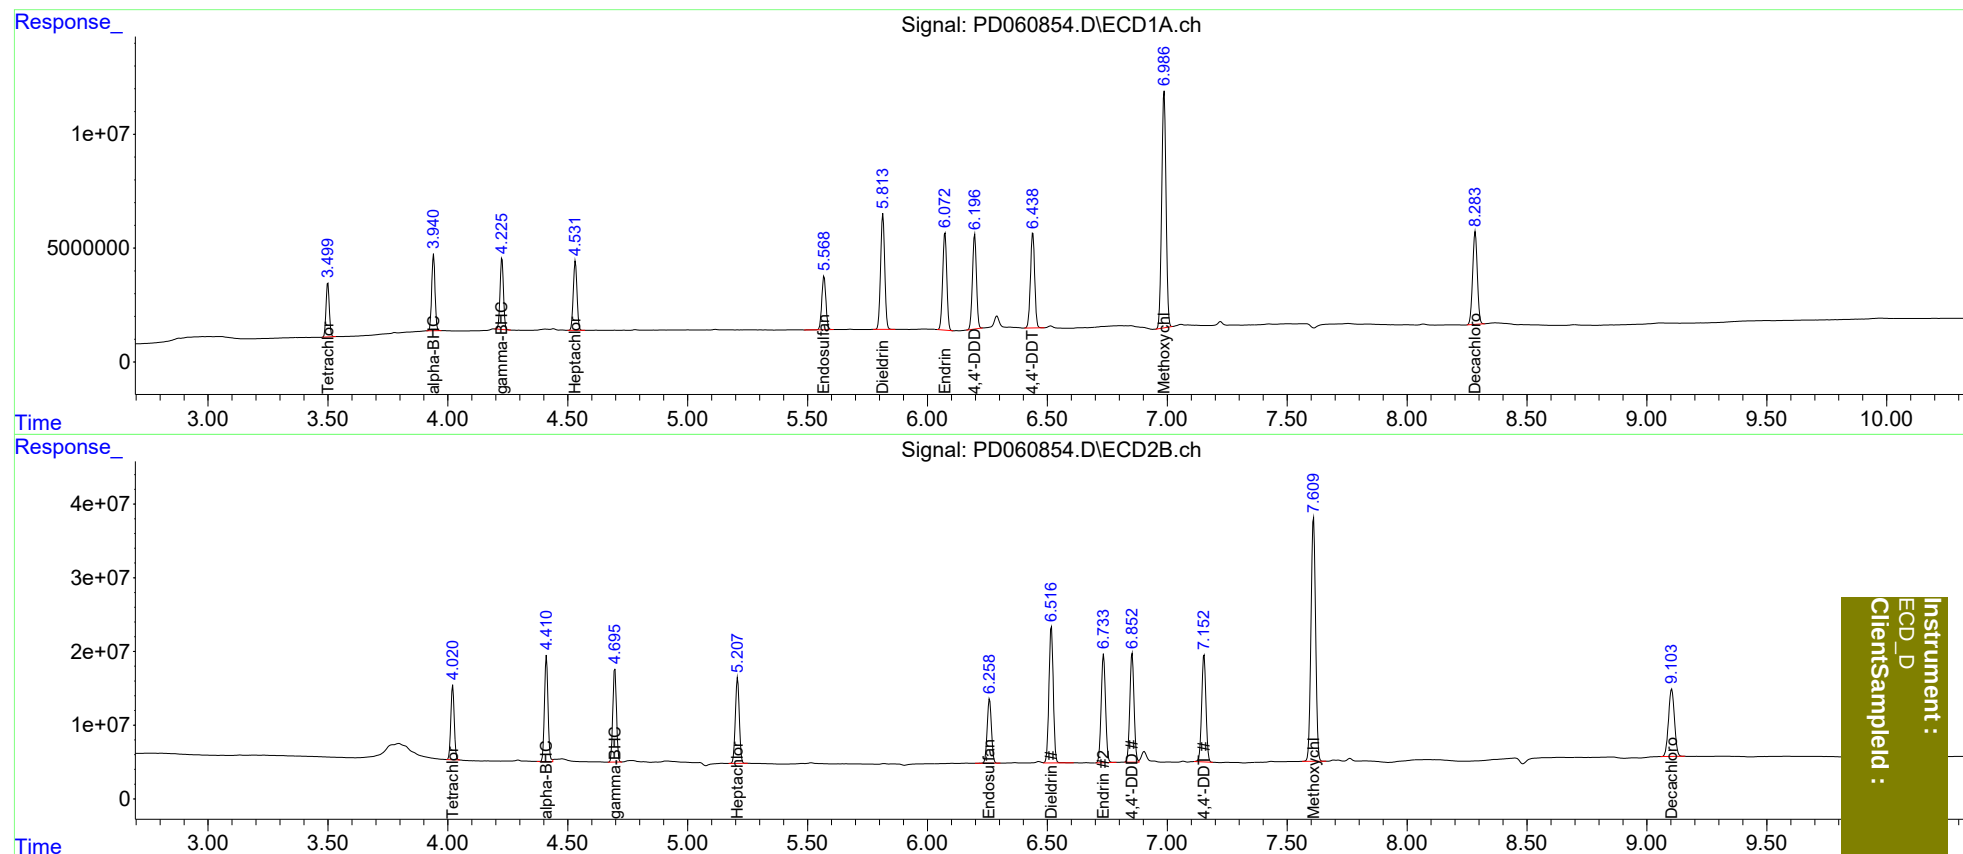


Instrument :
ECD_D
ClientSampled :

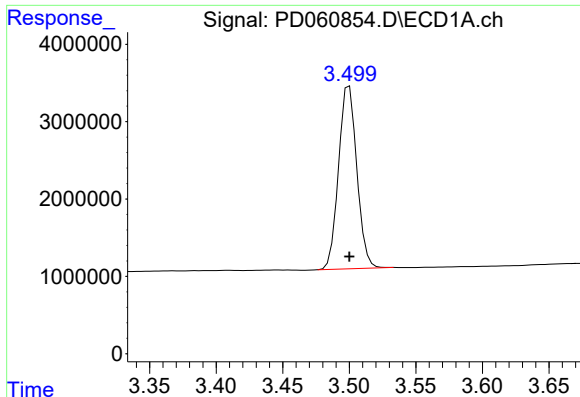

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 22639366
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

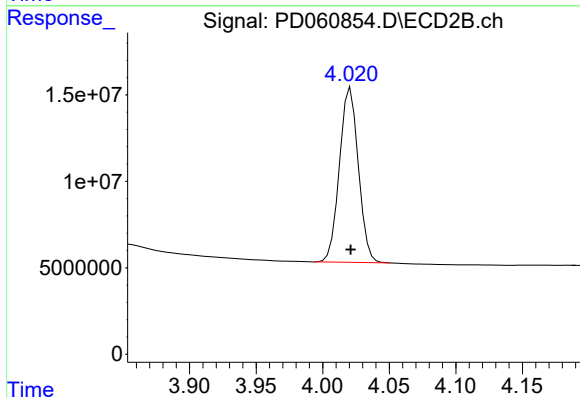


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 99817749
Conc: 20.00 ng/ml

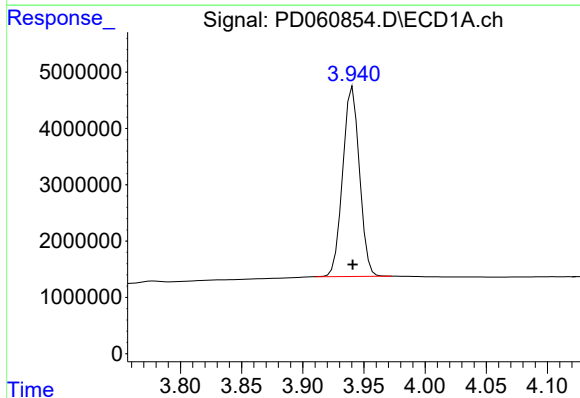


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 32150541
Conc: 20.00 ng/ml

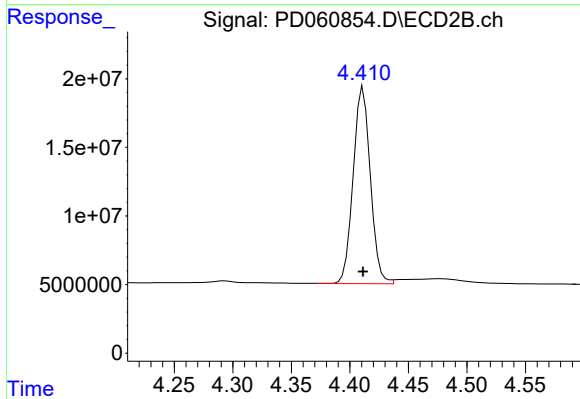

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 146726798
Conc: 20.00 ng/ml

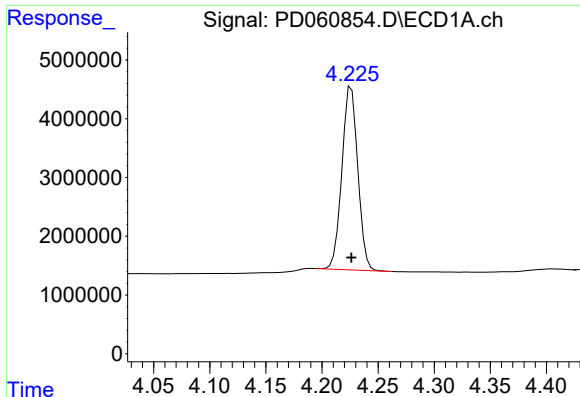

#3 gamma-BHC (Lindane)


R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 30746187
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

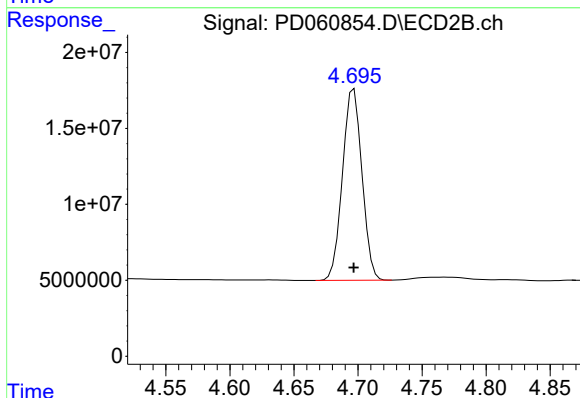


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 133260365
Conc: 20.00 ng/ml

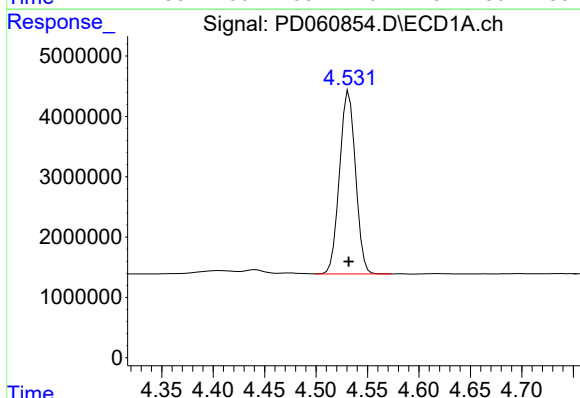


#4 Heptachlor

R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 32778646
Conc: 20.00 ng/ml

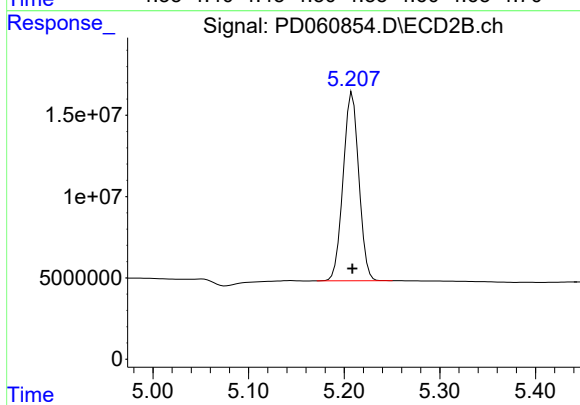

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 132868305
Conc: 20.00 ng/ml

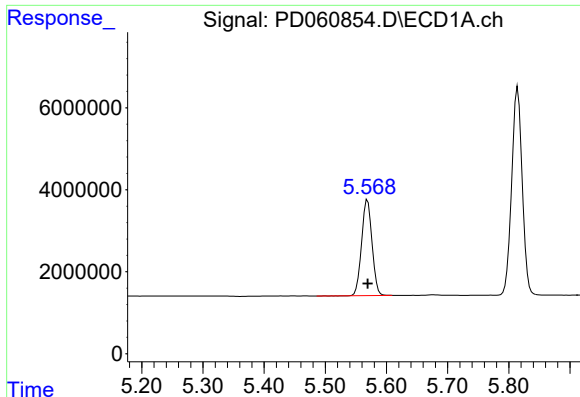

#9 Endosulfan I


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 27828756
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

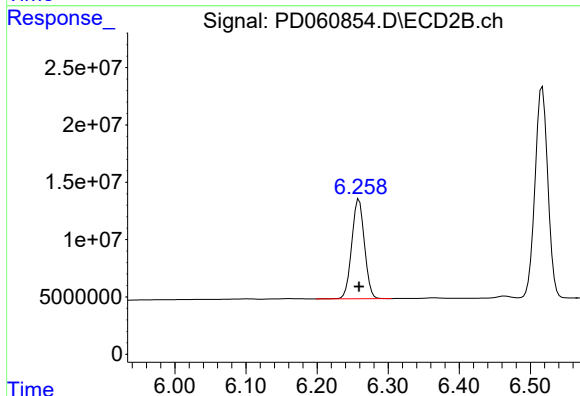


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 107658573
Conc: 20.00 ng/ml

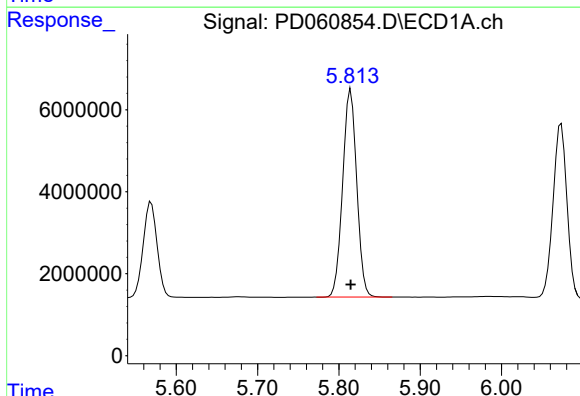


#13 Dieldrin

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 60707101
Conc: 40.00 ng/ml

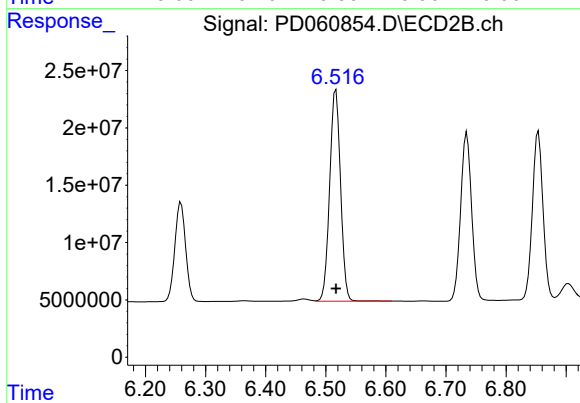

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 232238879
Conc: 40.00 ng/ml

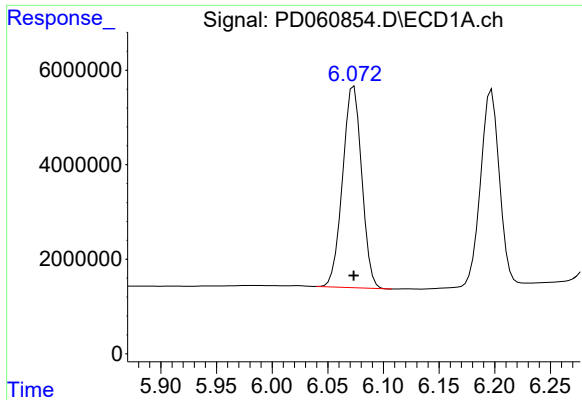

#14 Endrin


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 51079773
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

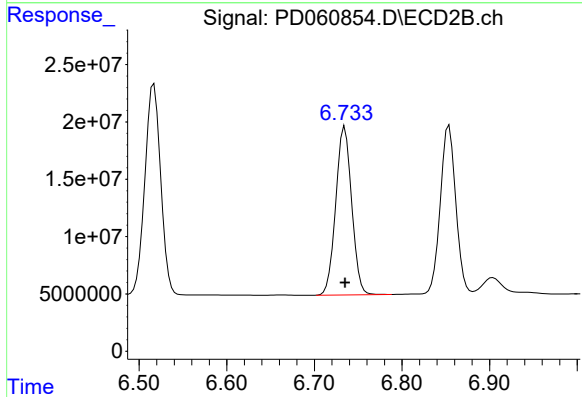


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 185381828
Conc: 40.00 ng/ml

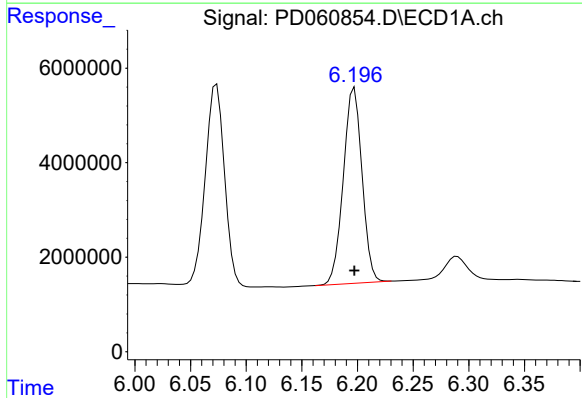


#16 4,4'-DDD

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 48385910
Conc: 40.00 ng/ml

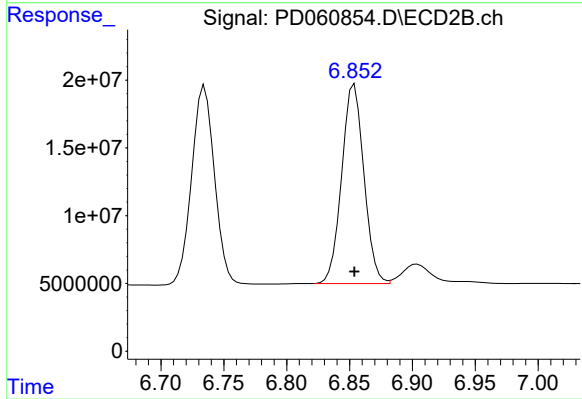

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 180583405
Conc: 40.00 ng/ml

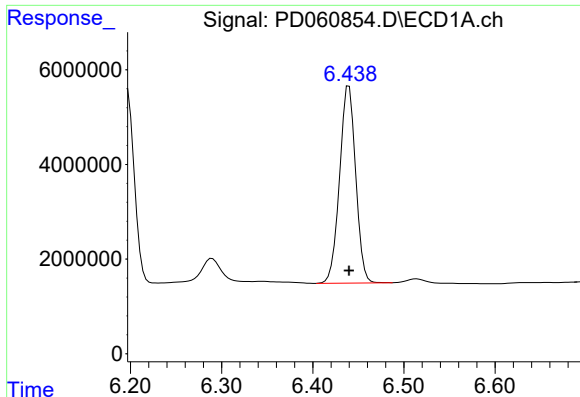

#17 4,4'-DDT


R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 51125194
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

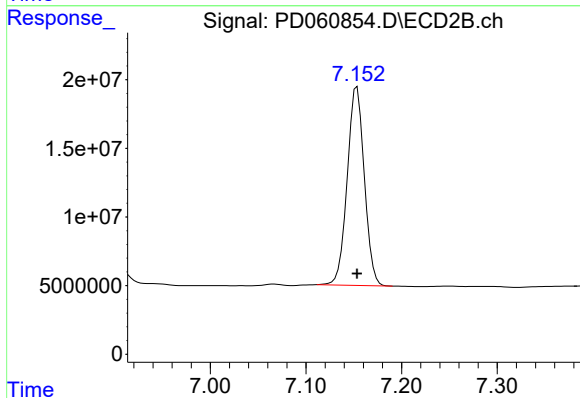


#17 4,4'-DDT

R.T.: 7.153 min
Delta R.T.: 0.000 min
Response: 180632163
Conc: 40.00 ng/ml

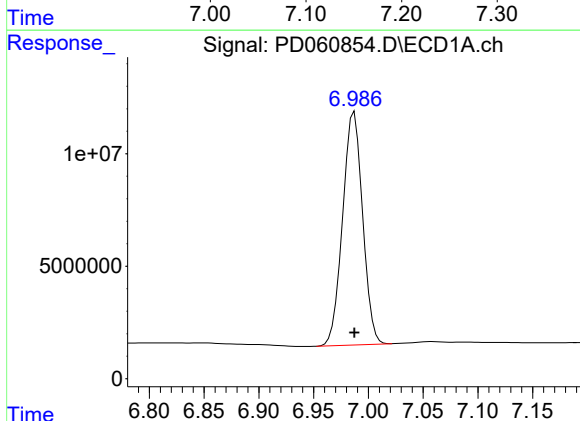


#20 Methoxychlor

R.T.: 6.987 min
Delta R.T.: 0.000 min
Response: 131586091
Conc: 200.00 ng/ml

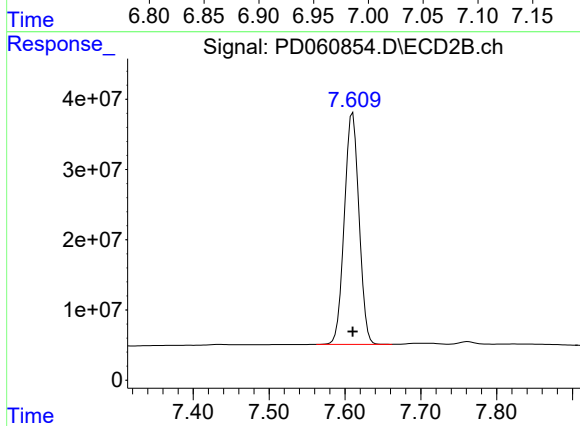

#20 Methoxychlor


R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 443261757
Conc: 200.00 ng/ml

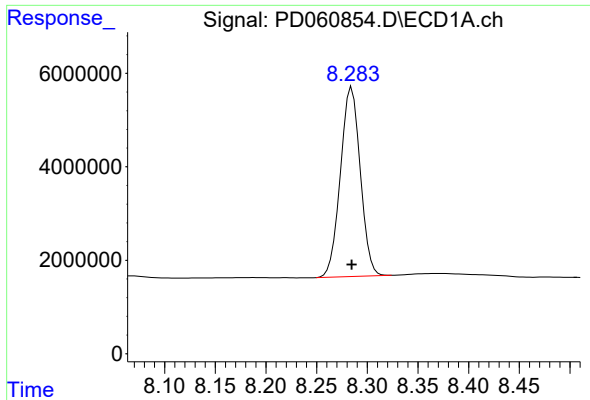

#27 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 55195468
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

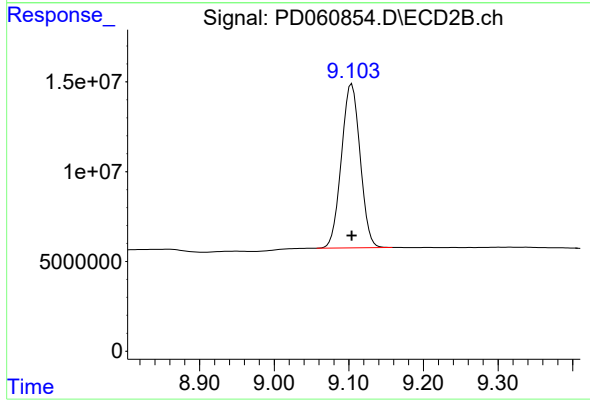

#27 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 159045168
Conc: 40.00 ng/ml